
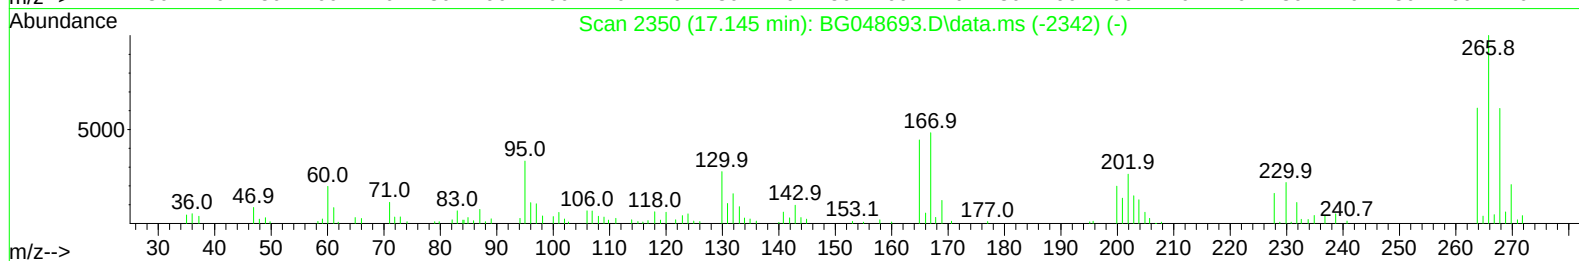
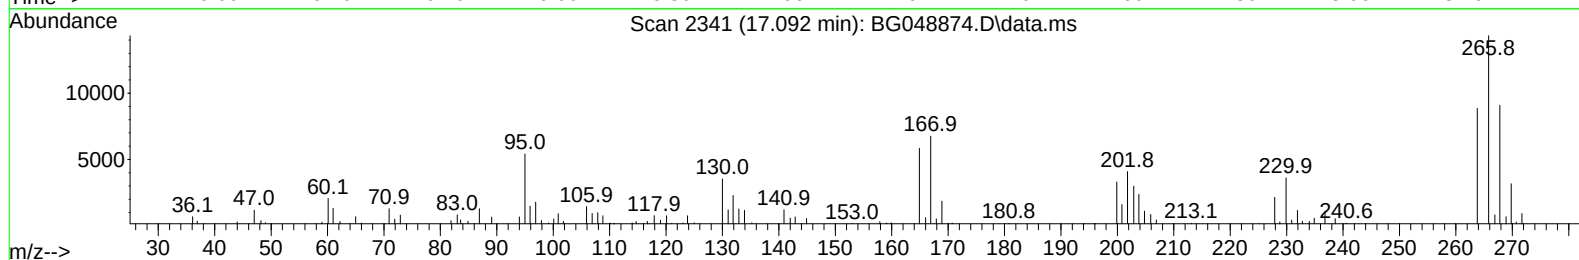


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042621\
Data File : BG048874.D
Acq On : 26 Apr 2021 12:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 26 12:51:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 20 17:33:30 2021
Response via : Initial Calibration

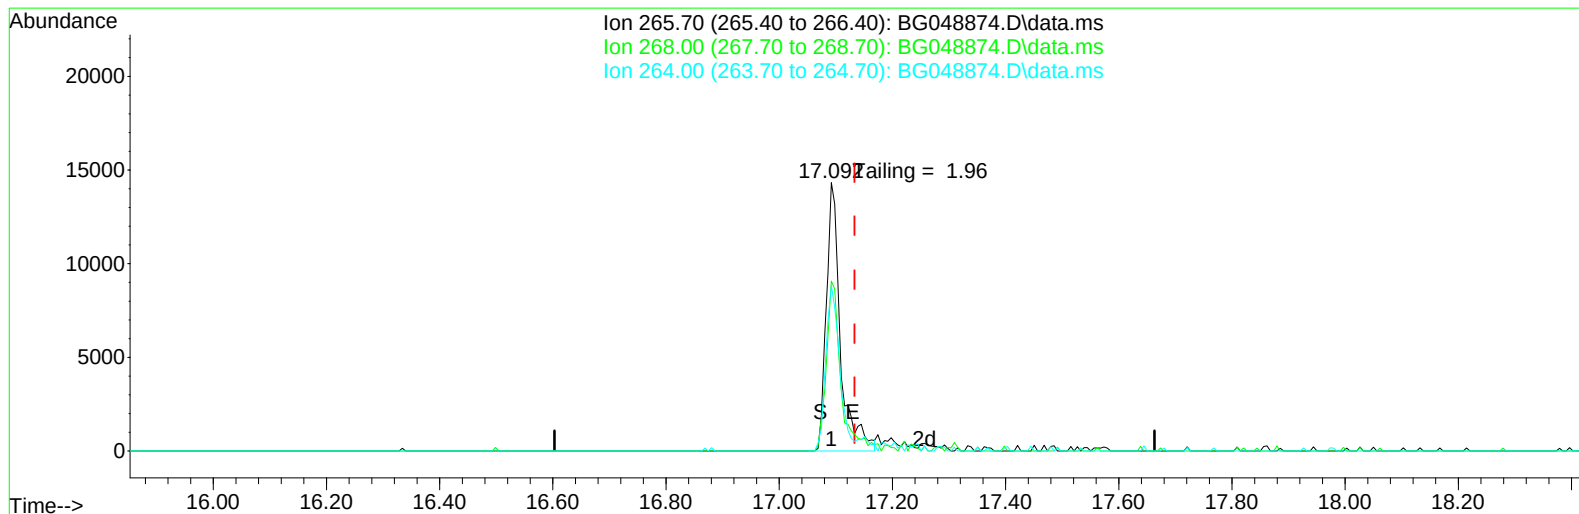

TIC: BG048874.D\data.ms

(70) Pentachlorophenol (C)




17.092min (-0.041) 75890.86 ng

response 24987

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.34
264.00	61.30	61.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042621\
Data File : BG048874.D
Acq On : 26 Apr 2021 12:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 26 12:51:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 20 17:33:30 2021
Response via : Initial Calibration

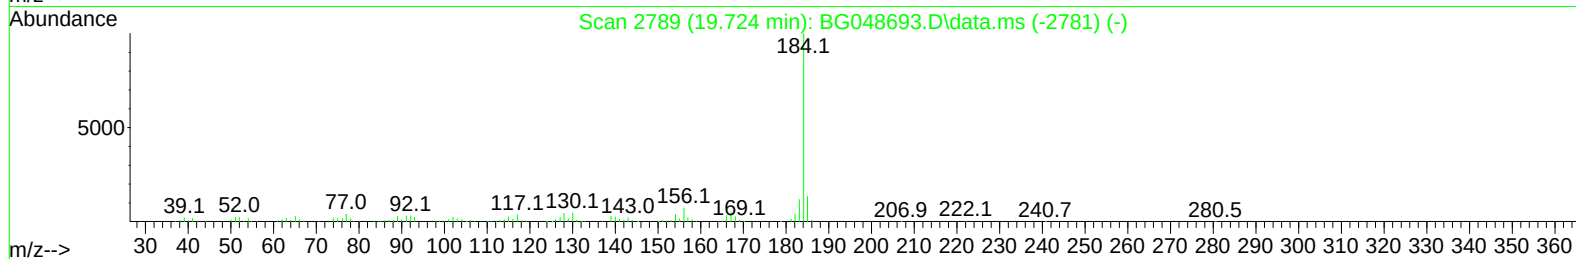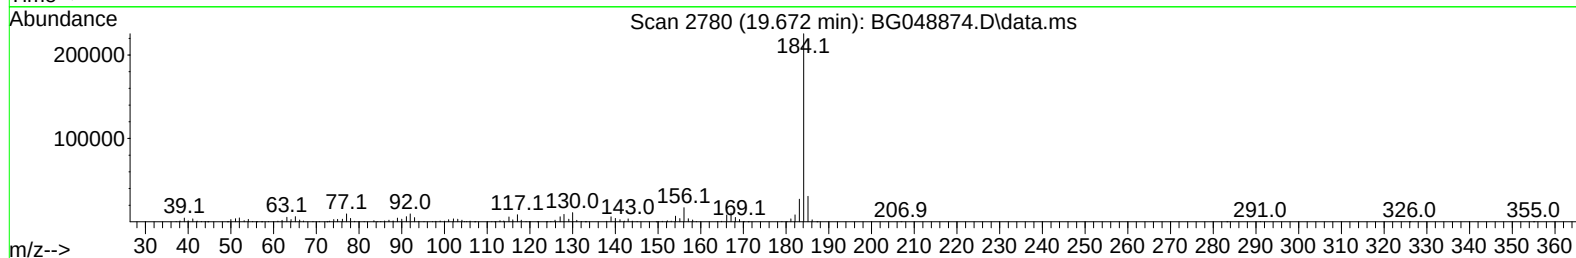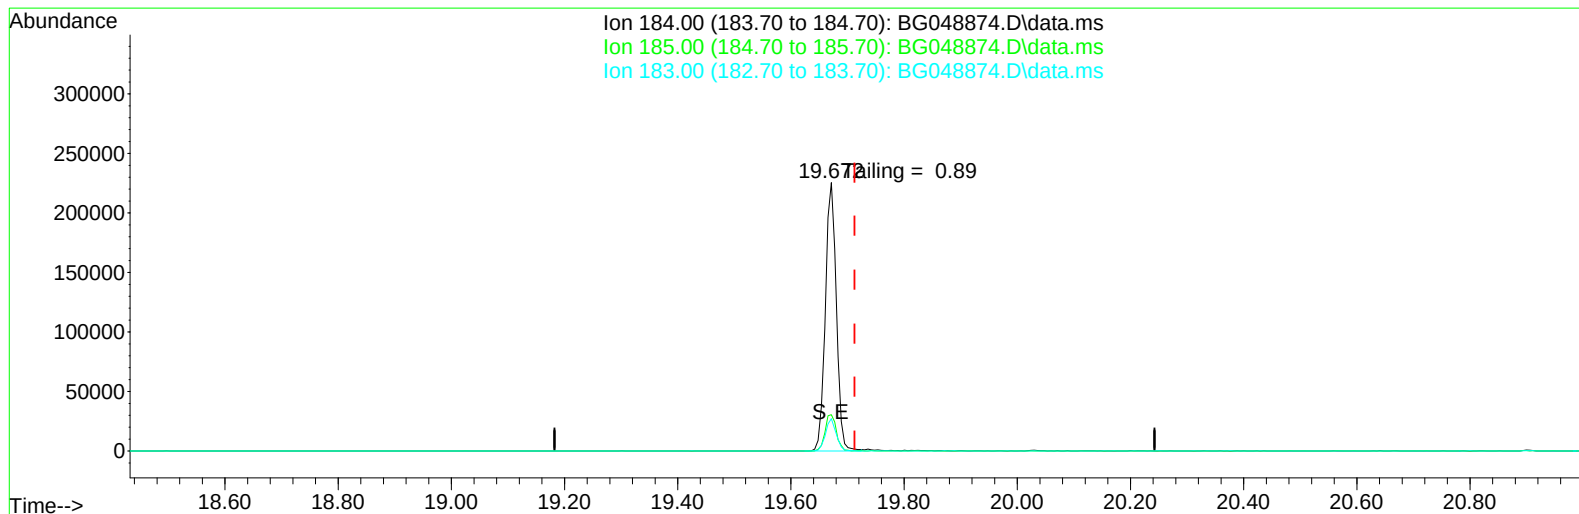

TIC: BG048874.D\data.ms

(77) Benzidine**19.672min (-0.041) 6762.41 ng****response 304295**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.56
183.00	11.70	12.05
0.00	0.00	0.00