
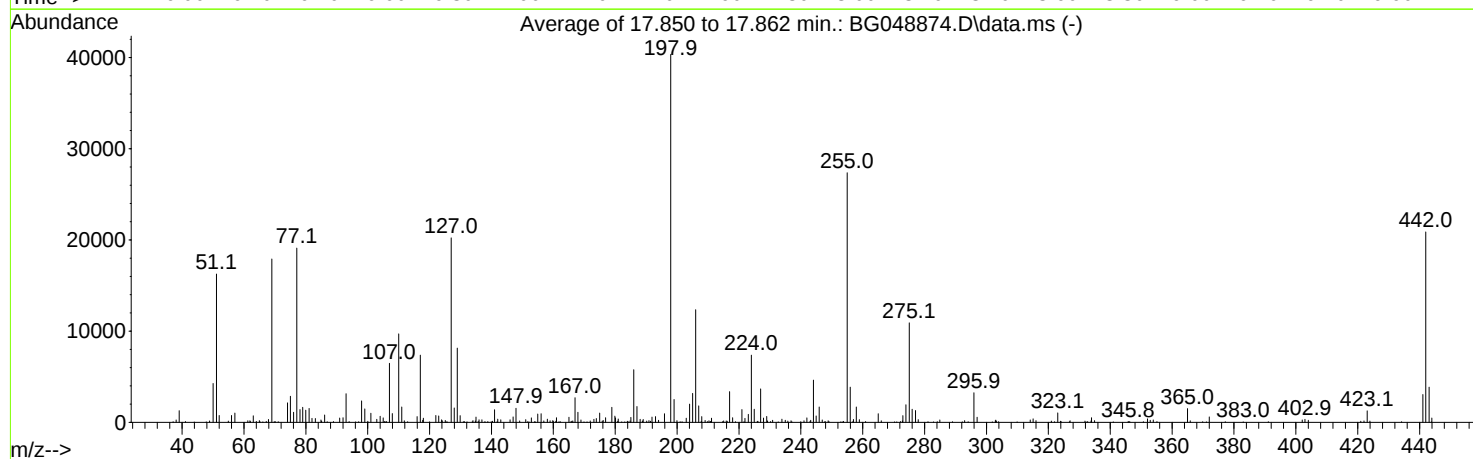


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042621\
 Data File : BG048874.D
 Acq On : 26 Apr 2021 12:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 27 04:39:25 2021

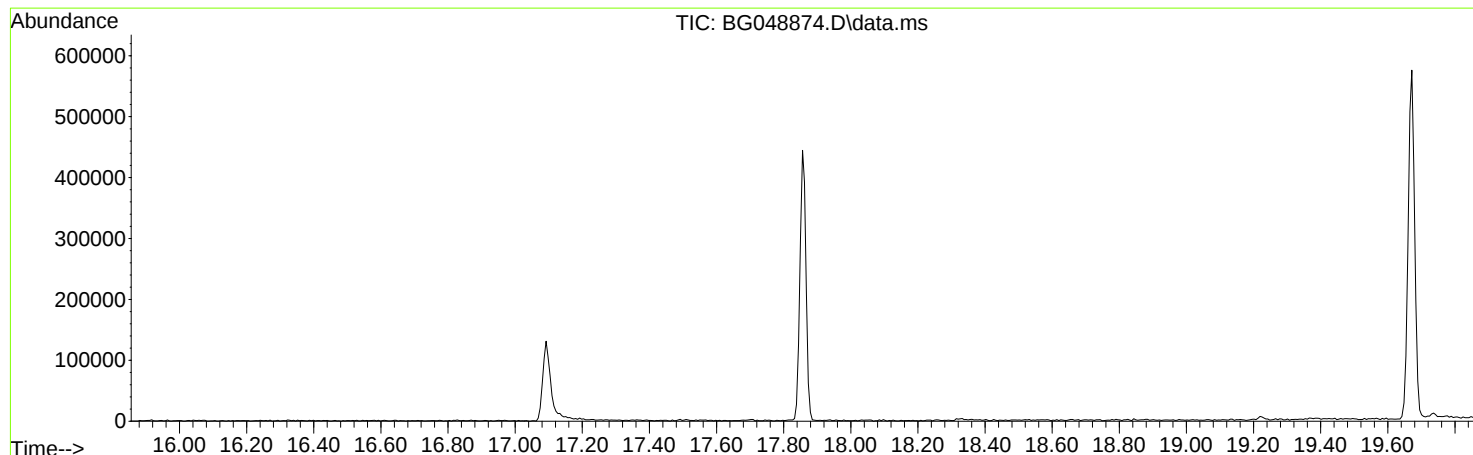

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	16267	PASS
68	69	0.00	2	1.7	312	PASS
69	198	0.00	100	44.4	17925	PASS
70	69	0.00	2	0.5	97	PASS
127	198	10	80	50.2	20237	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	40341	PASS
199	198	5	9	6.2	2512	PASS
275	198	10	60	27.0	10907	PASS
365	198	1	100	3.7	1502	PASS
441	198	0.01	100	7.6	3061	PASS
442	198	50	100	51.8	20877	PASS
443	442	15	24	18.5	3864	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/26/2021	BNA_G	BG048874.D
Compound Name	Response	Retention Time
DDT	139594	20.89
DDD	4682	20.45
DDE	405	19.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5087	144681	3.52

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042621\
Data File : BG048874.D
Acq On : 26 Apr 2021 12:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 26 12:51:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 20 17:33:30 2021
Response via : Initial Calibration

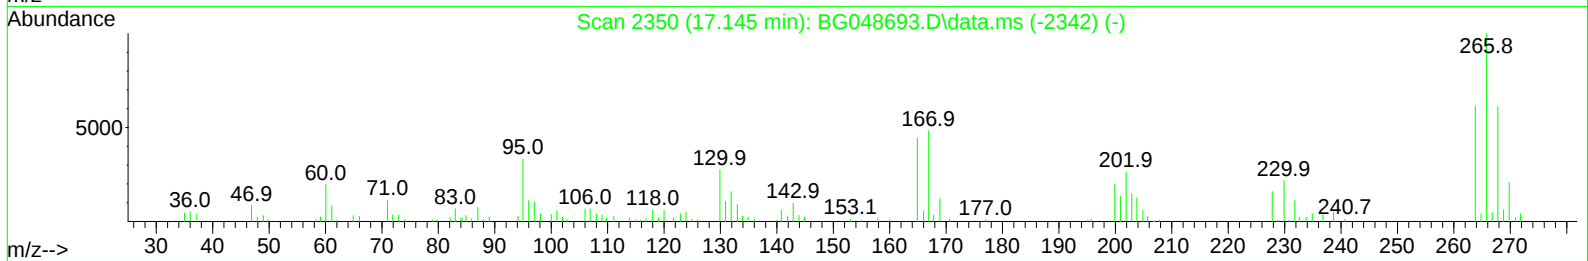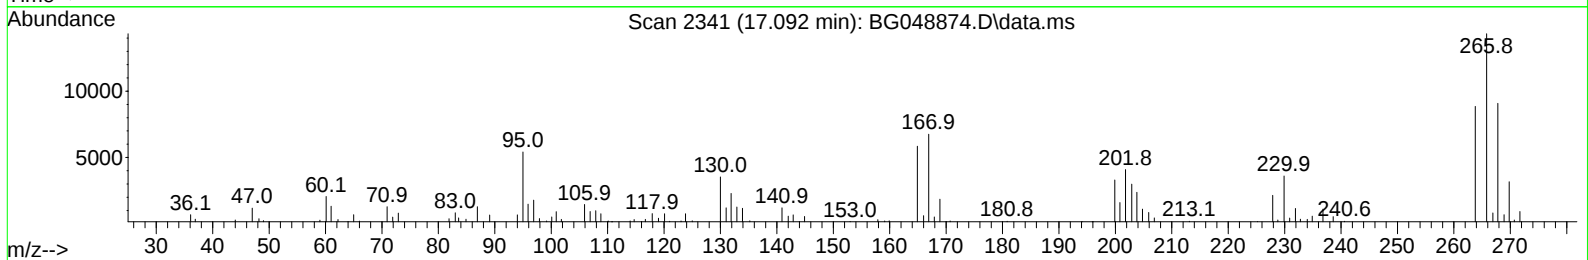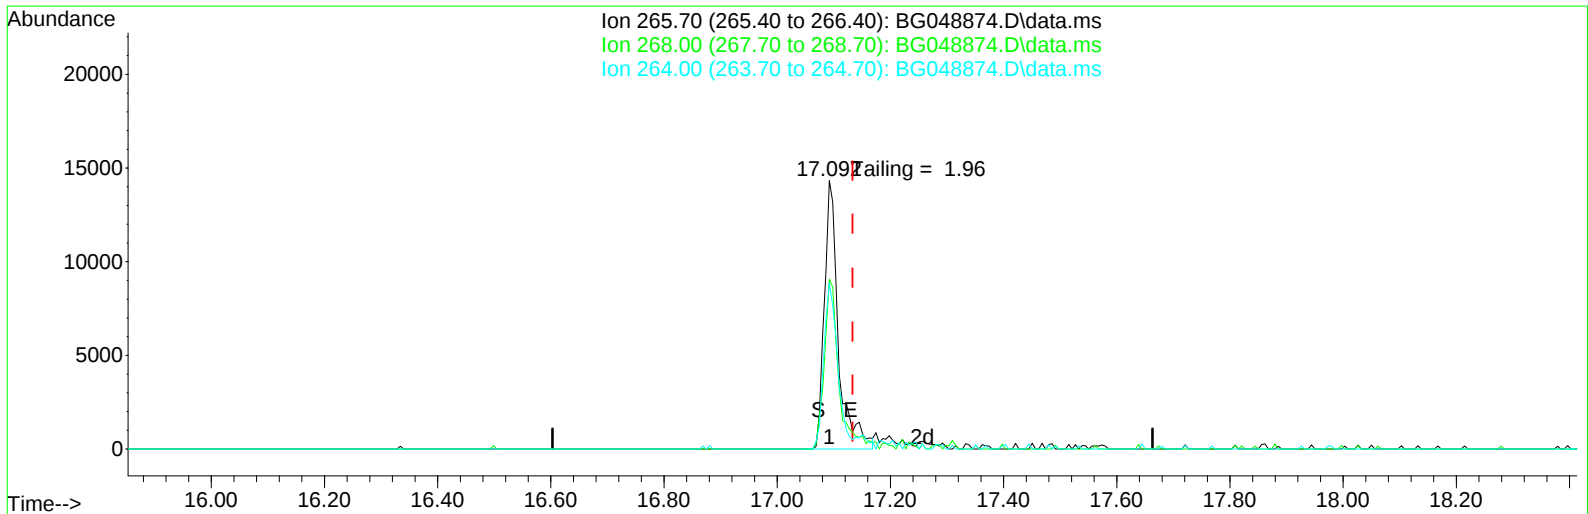

TIC: BG048874.D\data.ms

(70) Pentachlorophenol (C)

17.092min (-0.041) 75890.86 ng




response 24987

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.34
264.00	61.30	61.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042621\
Data File : BG048874.D
Acq On : 26 Apr 2021 12:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 26 12:51:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 20 17:33:30 2021
Response via : Initial Calibration

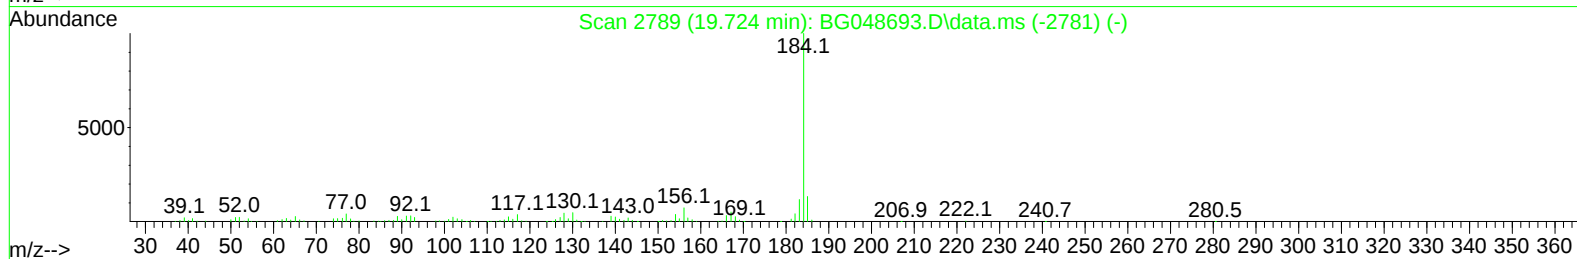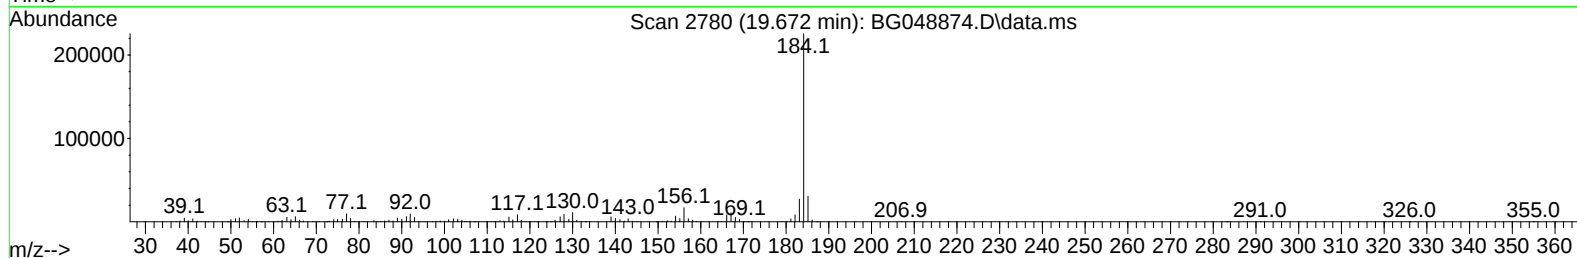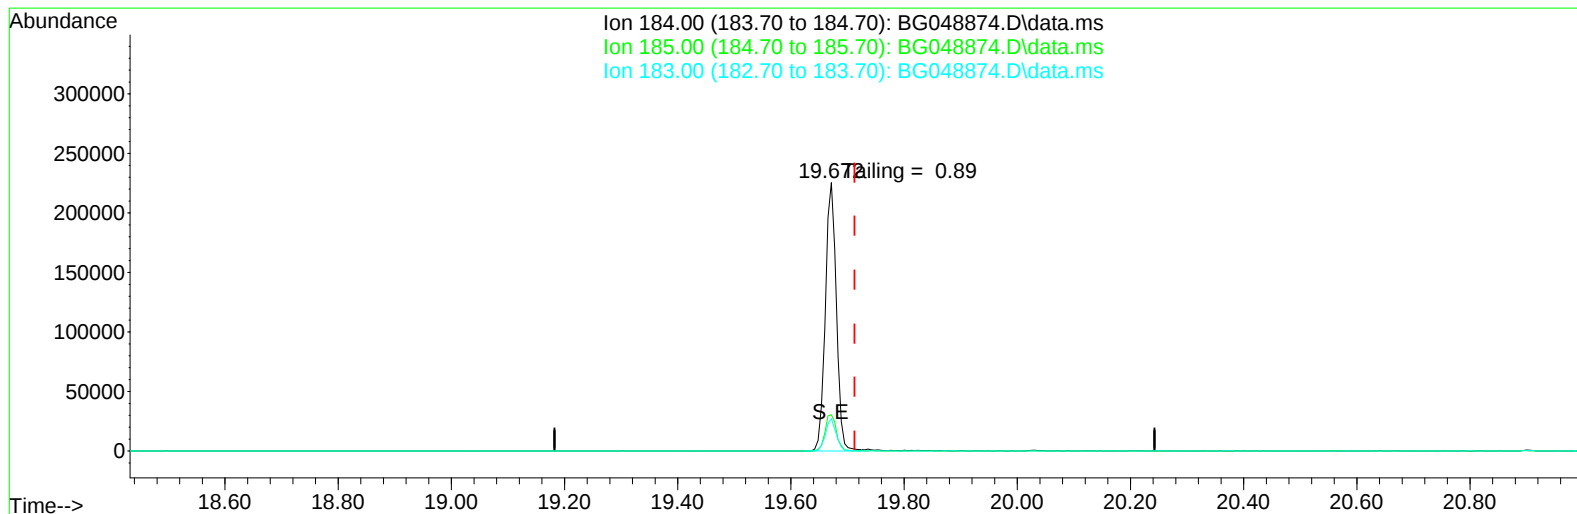

TIC: BG048874.D\data.ms

(77) Benzidine

19.672min (-0.041) 6762.41 ng

response 304295

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.56
183.00	11.70	12.05
0.00	0.00	0.00