
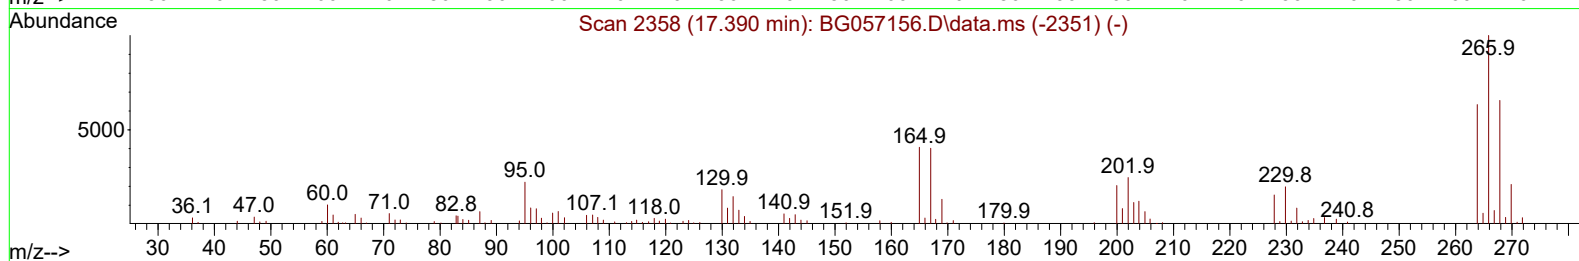
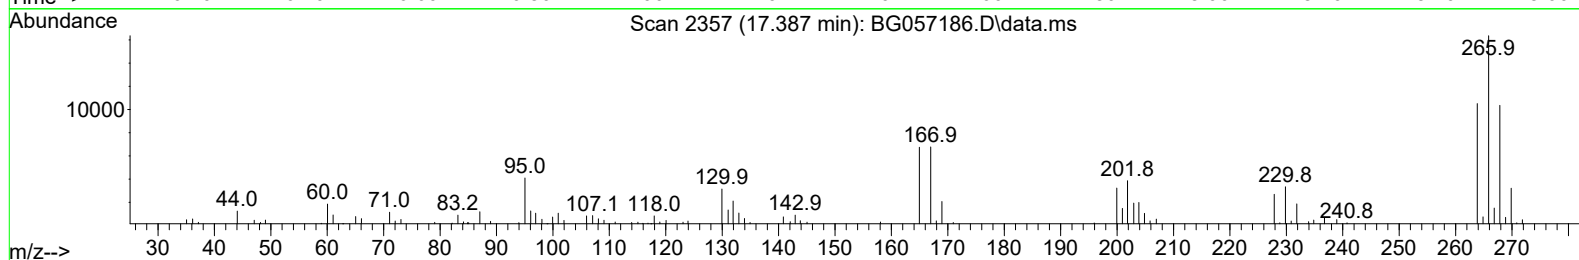


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042623\
Data File : BG057186.D
Acq On : 26 Apr 2023 9:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 05:49:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 27 03:02:41 2023
Response via : Initial Calibration

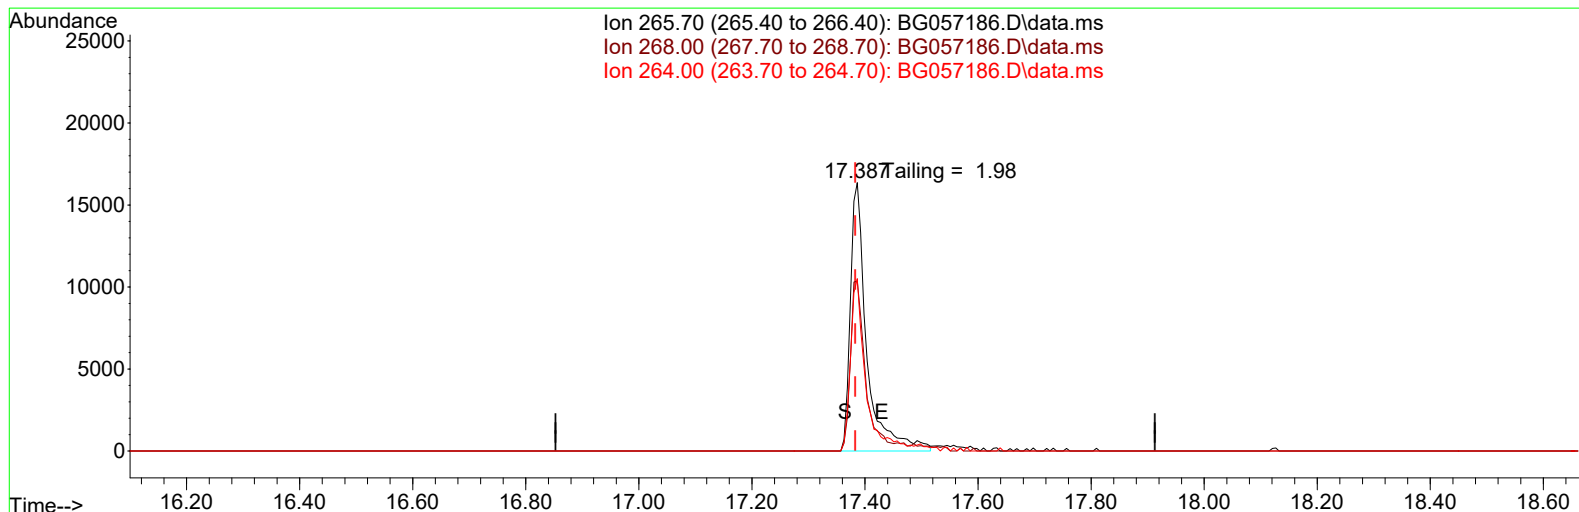

TIC: BG057186.D\data.ms

(70) Pentachlorophenol (C)




17.387min (+ 0.004) 44501.99 ng

response 32246

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.60	63.35
264.00	63.40	64.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042623\
Data File : BG057186.D
Acq On : 26 Apr 2023 9:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 05:49:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 27 03:02:41 2023
Response via : Initial Calibration

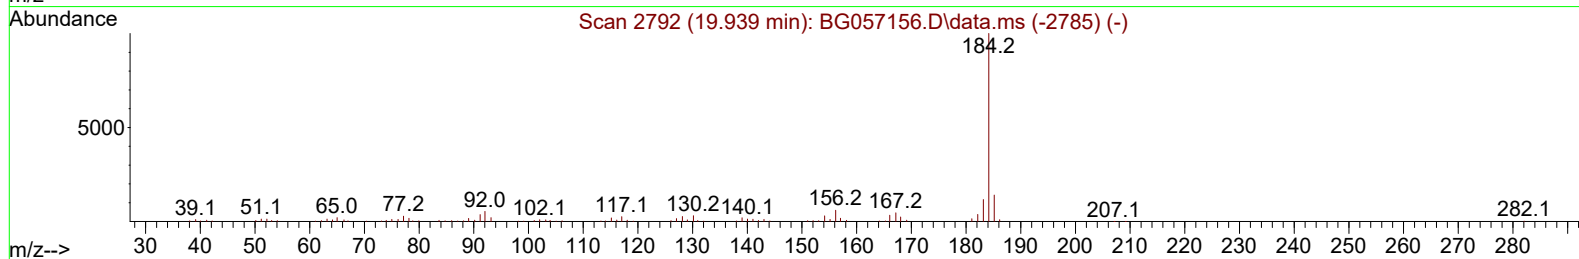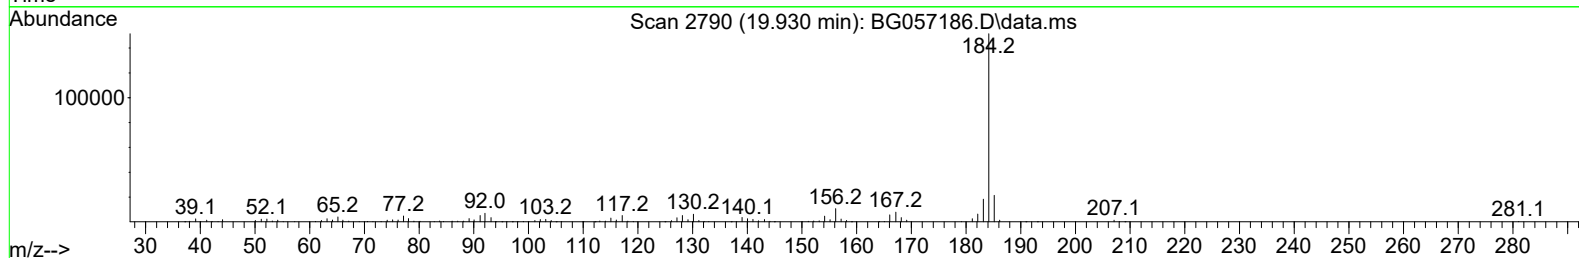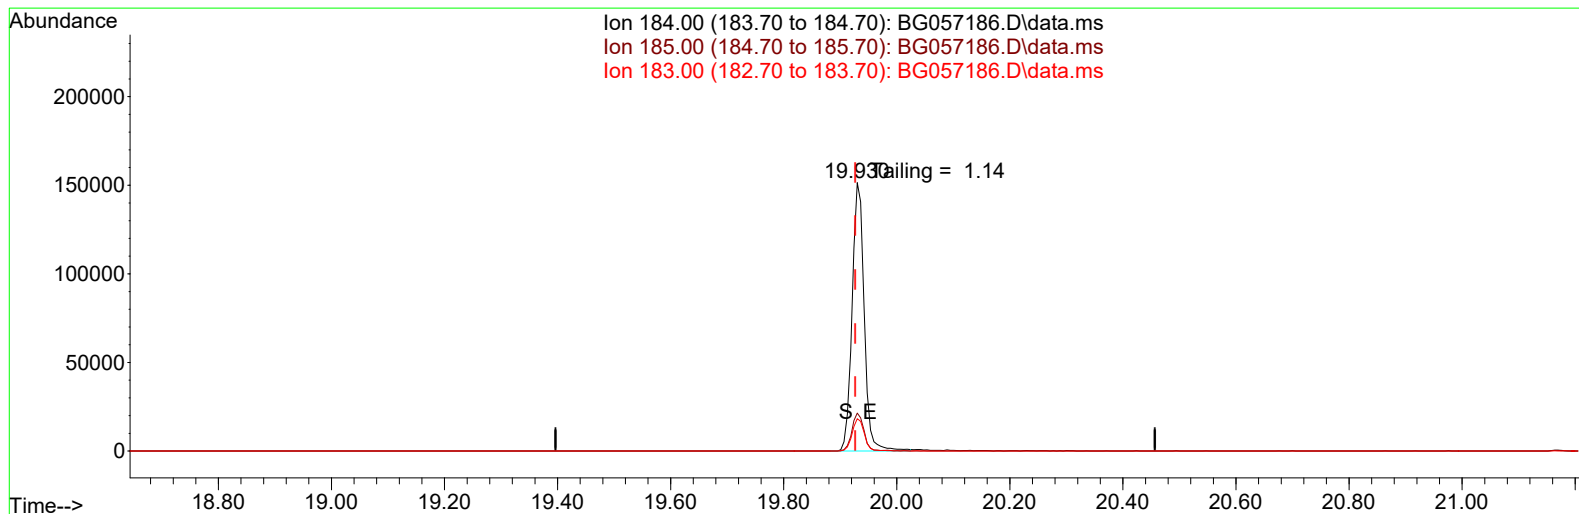

TIC: BG057186.D\data.ms

(77) Benzidine

19.930min (+ 0.004) 0.00 ng

response 227146

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.17
183.00	11.70	12.07
0.00	0.00	0.00