
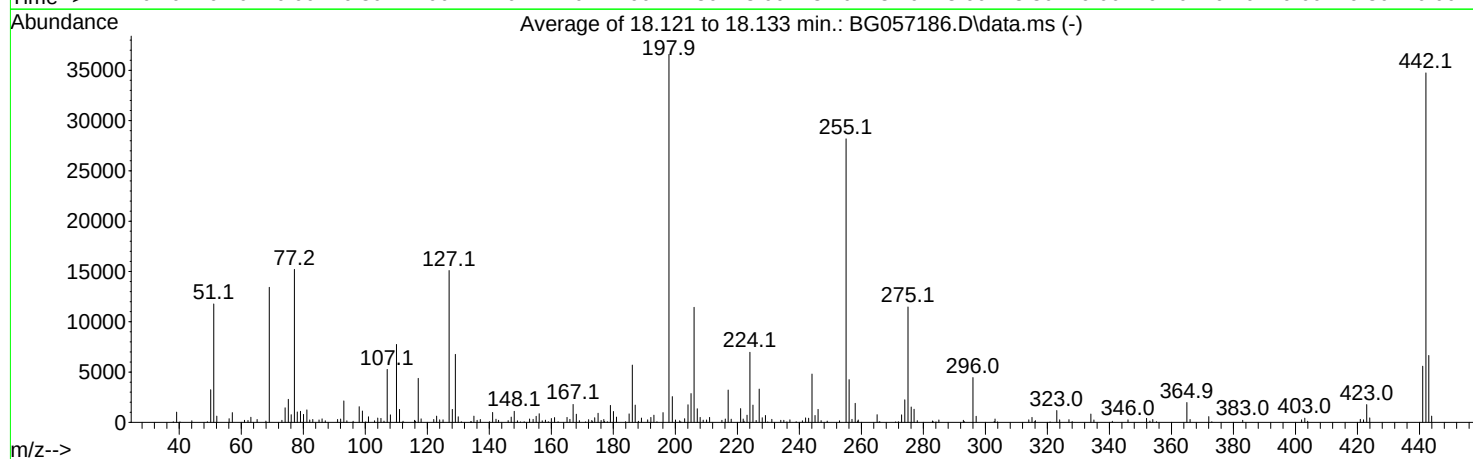


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042623\
Data File : BG057186.D
Acq On : 26 Apr 2023 9:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042423.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Apr 27 03:02:41 2023

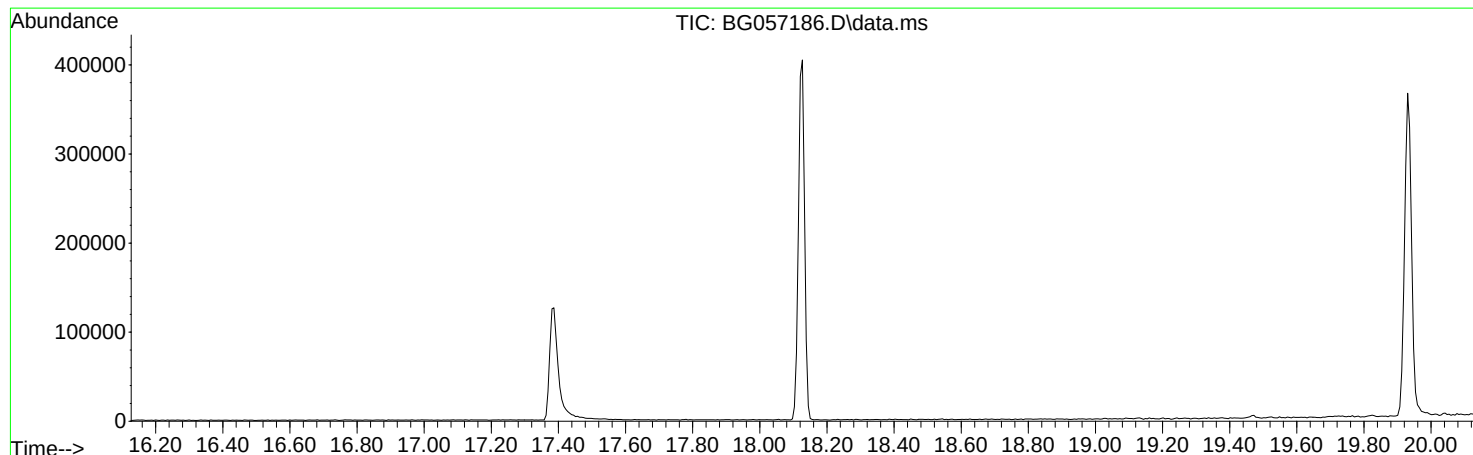

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	11769	PASS
68	69	0.00	2	0.9	124	PASS
69	198	0.00	100	36.7	13423	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.3	15092	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	36568	PASS
199	198	5	9	7.0	2561	PASS
275	198	10	60	31.4	11477	PASS
365	198	1	100	5.4	1981	PASS
441	198	0.01	100	15.3	5587	PASS
442	442	50	100	100.0	34747	PASS
443	442	15	24	19.2	6657	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/26/2023	BNA_G	<u>BG057186.D</u>
Compound Name	Response	Retention Time
DDT	107838	21.17
DDD	3041	20.706
DDE	146	20.206
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3187	111025	2.87

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042623\
Data File : BG057186.D
Acq On : 26 Apr 2023 9:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 27 05:49:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 27 03:02:41 2023
Response via : Initial Calibration

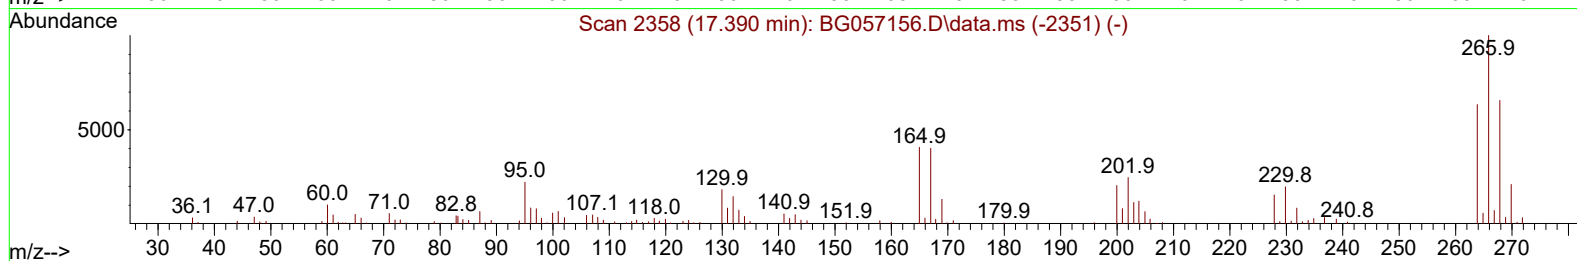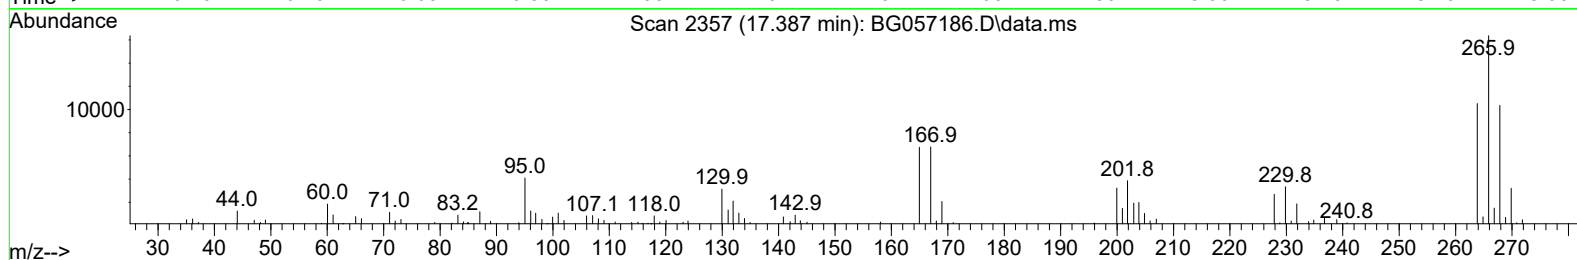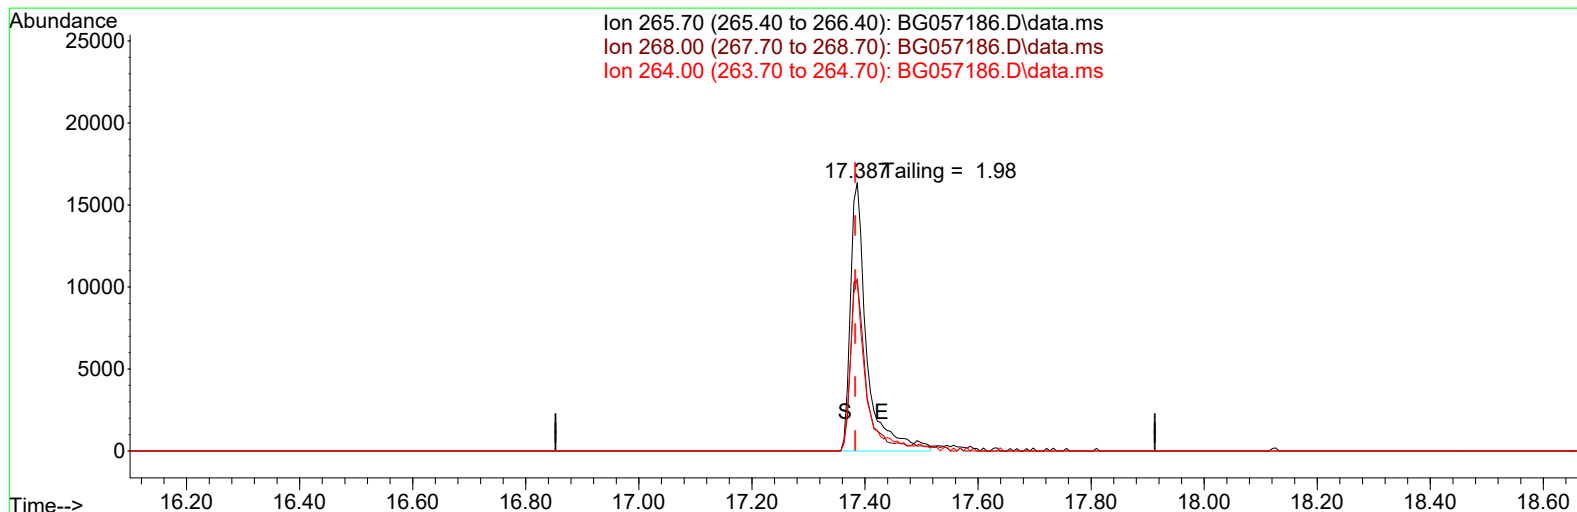

TIC: BG057186.D\data.ms

(70) Pentachlorophenol (C)

17.387min (+ 0.004) 44501.99 ng




response 32246

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.60	63.35
264.00	63.40	64.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042623\
Data File : BG057186.D
Acq On : 26 Apr 2023 9:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 27 05:49:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 27 03:02:41 2023
Response via : Initial Calibration

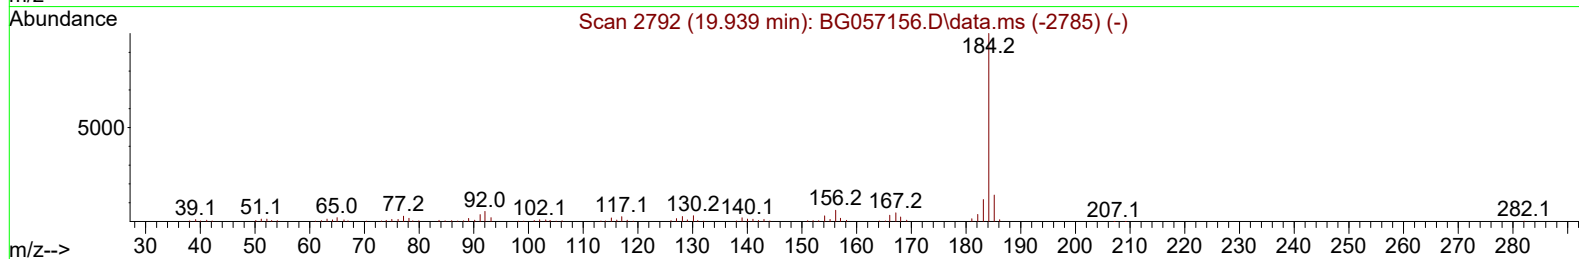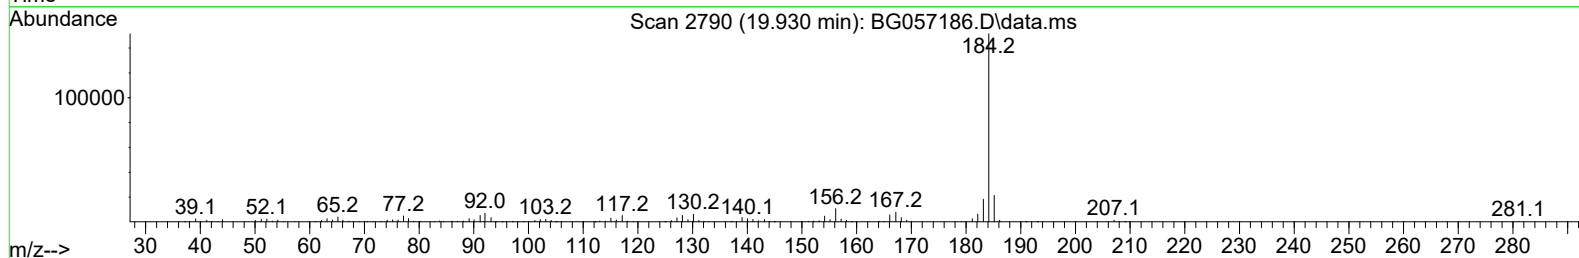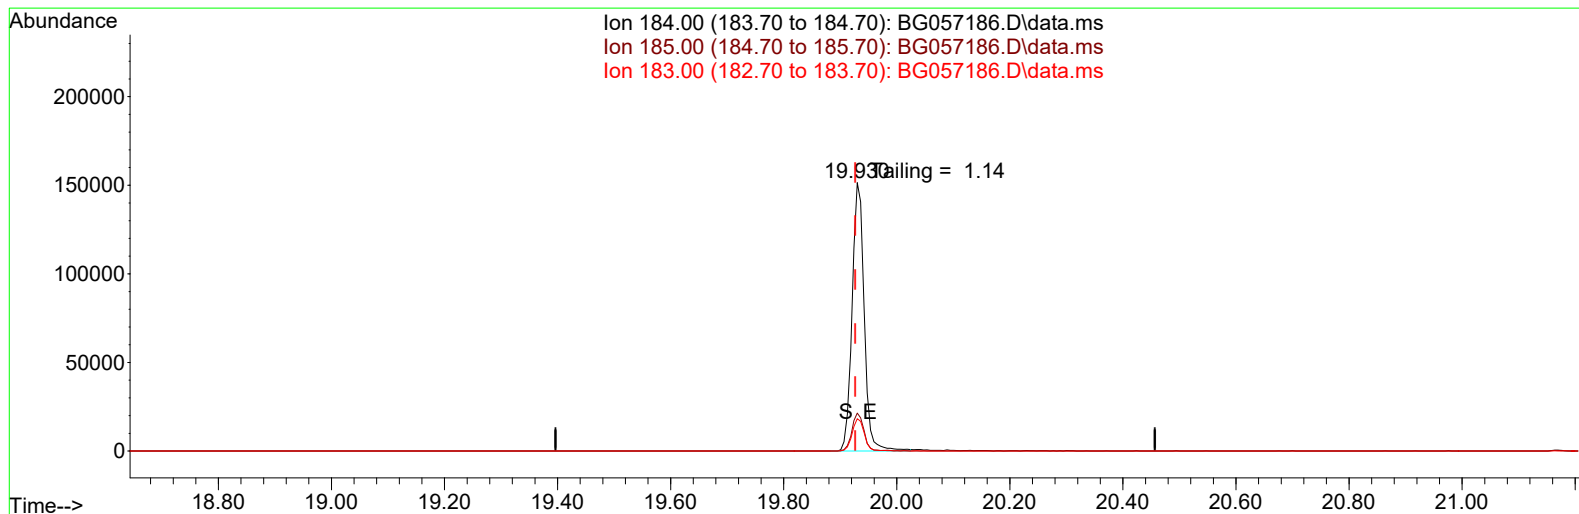

TIC: BG057186.D\data.ms

(77) Benzidine

19.930min (+ 0.004) 0.00 ng

response 227146

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.17
183.00	11.70	12.07
0.00	0.00	0.00