
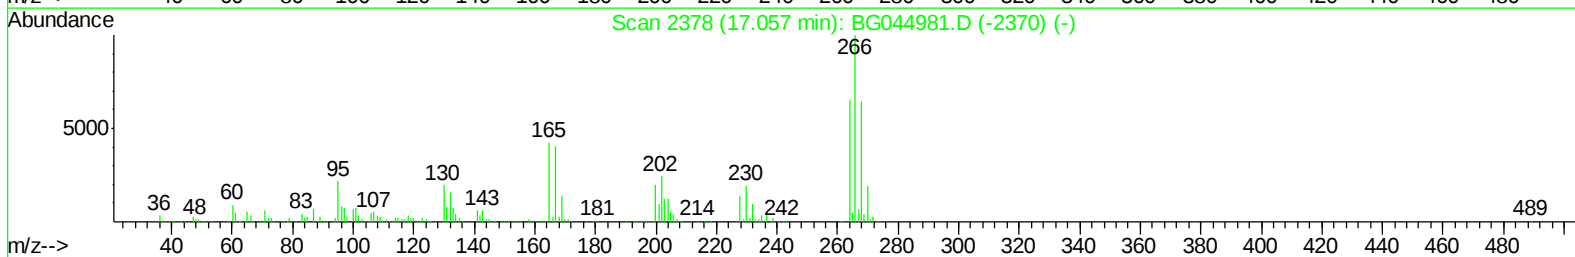
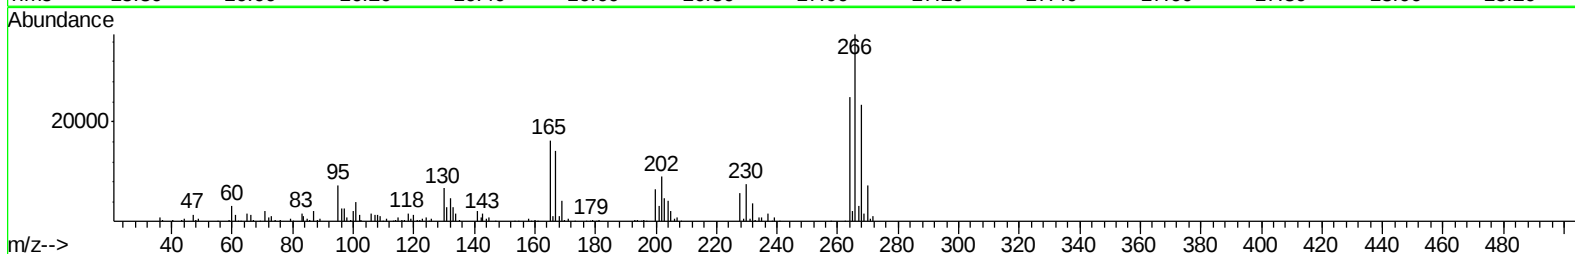


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG042720\
Data File : BG045174.D
Acq On : 27 Apr 2020 11:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 04:35:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 27 12:48:53 2020
Response via : Initial Calibration

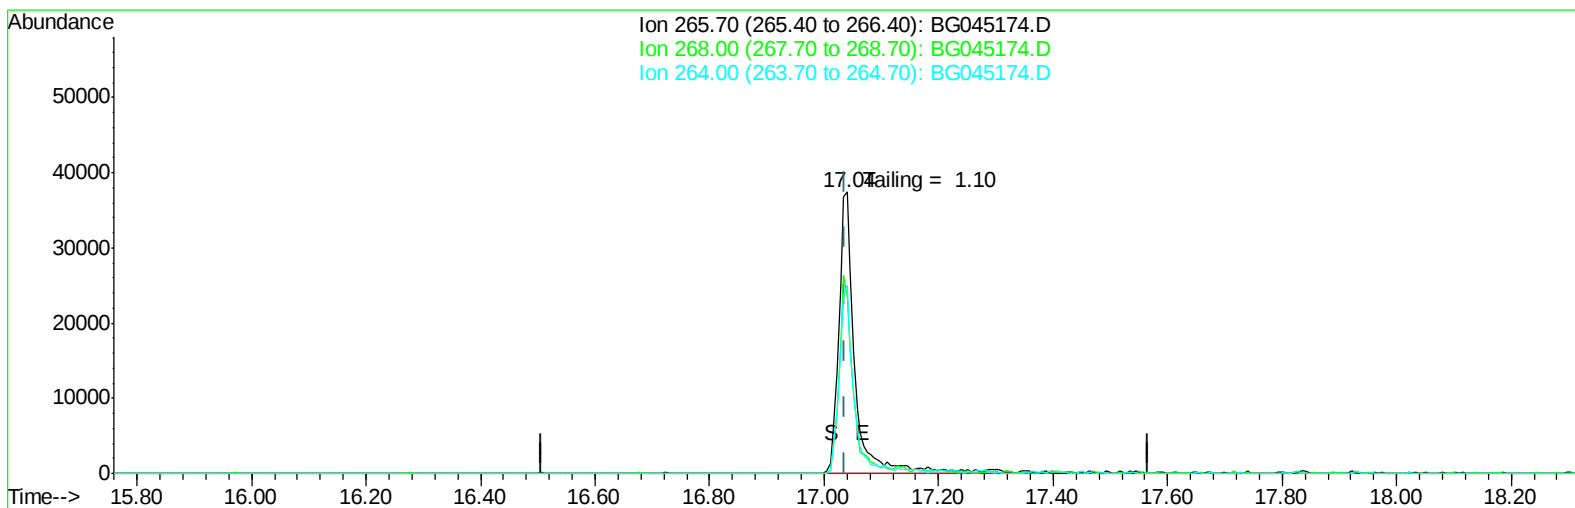

TIC: BG045174.D

(70) Pentachlorophenol (C)




17.040min (+0.003) 131758.01ng

response 68132

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	62.55
264.00	65.30	66.87
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG042720\
Data File : BG045174.D
Acq On : 27 Apr 2020 11:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 04:35:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 27 12:48:53 2020
Response via : Initial Calibration

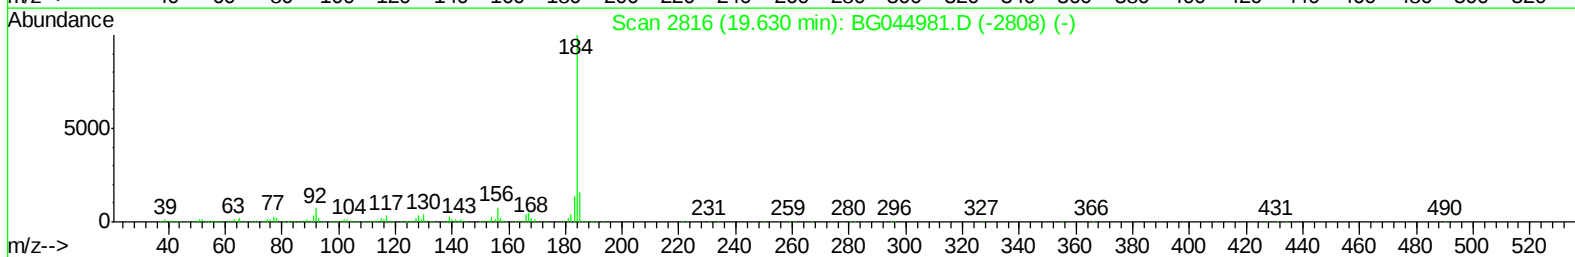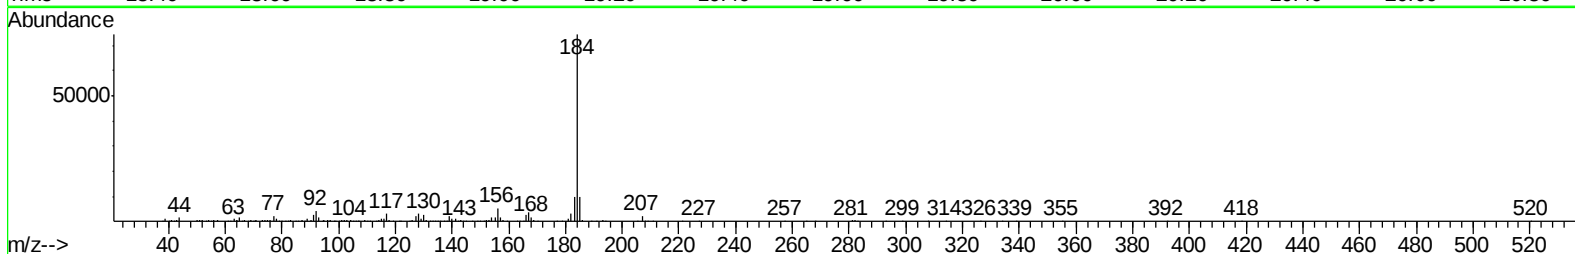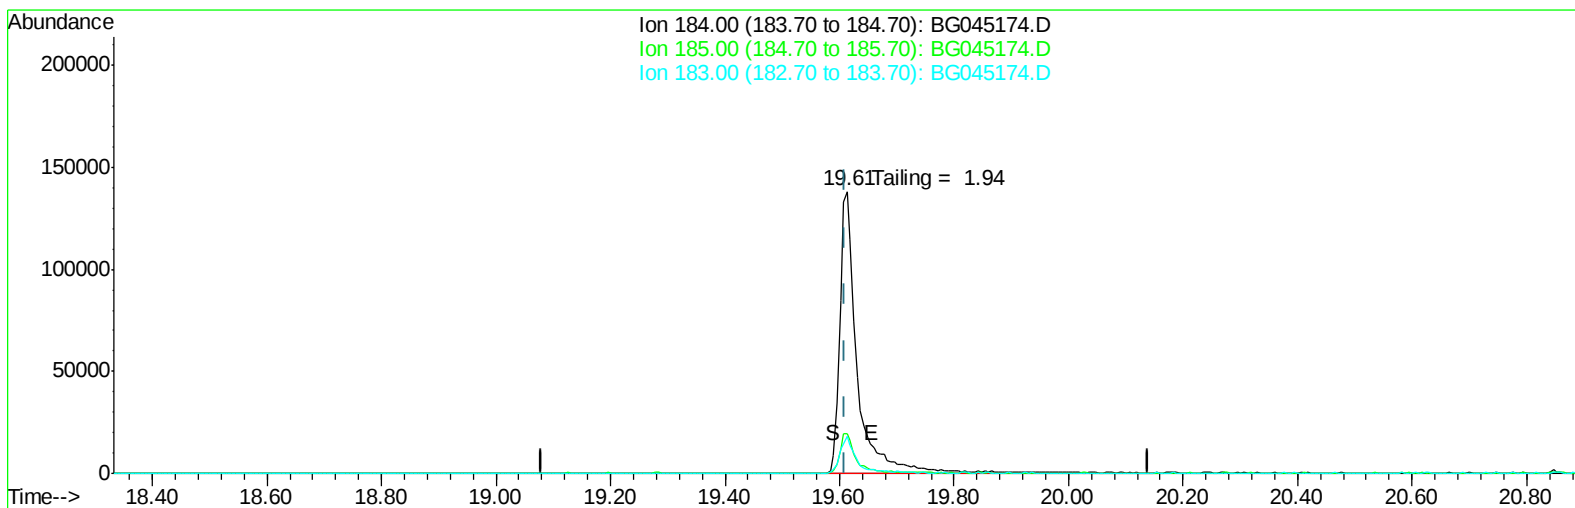

TIC: BG045174.D

(77) Benzidine

19.613min (+0.003) 138230.55ng

response 291818

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	13.94
183.00	14.10	13.22
0.00	0.00	0.00