


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG042720\
 Data File : BG045174.D
 Acq On : 27 Apr 2020 11:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 27 12:48:53 2020

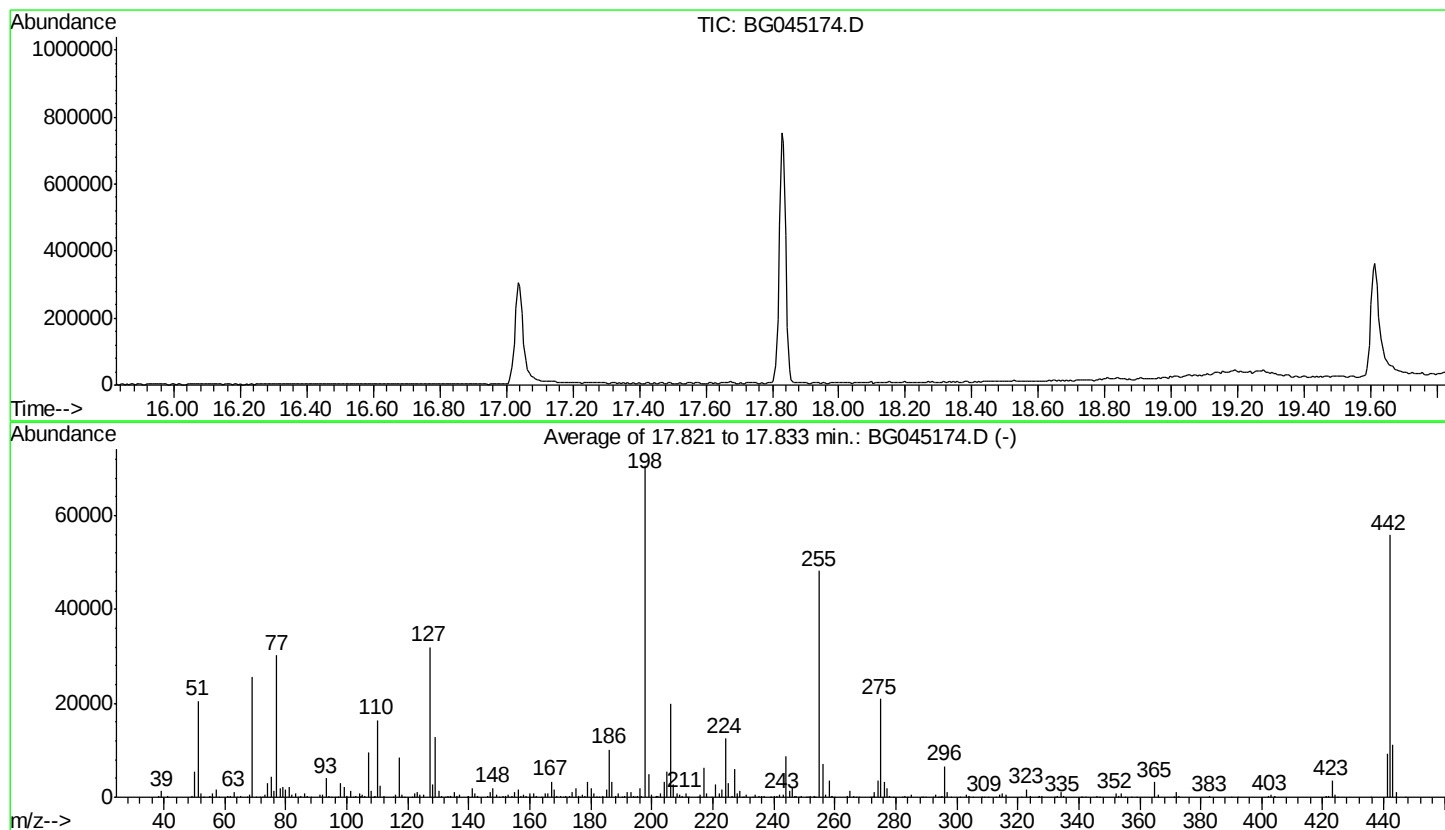

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2502

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.0	20480	PASS
68	69	0.00	2	1.7	435	PASS
69	198	0.00	100	36.2	25584	PASS
70	69	0.00	2	0.5	137	PASS
127	198	10	80	45.3	32010	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	70608	PASS
199	198	5	9	7.0	4947	PASS
275	198	10	60	29.6	20868	PASS
365	198	1	100	4.5	3186	PASS
441	198	0.01	100	13.1	9220	PASS
442	198	50	100	79.0	55808	PASS
443	442	15	24	20.0	11135	PASS