
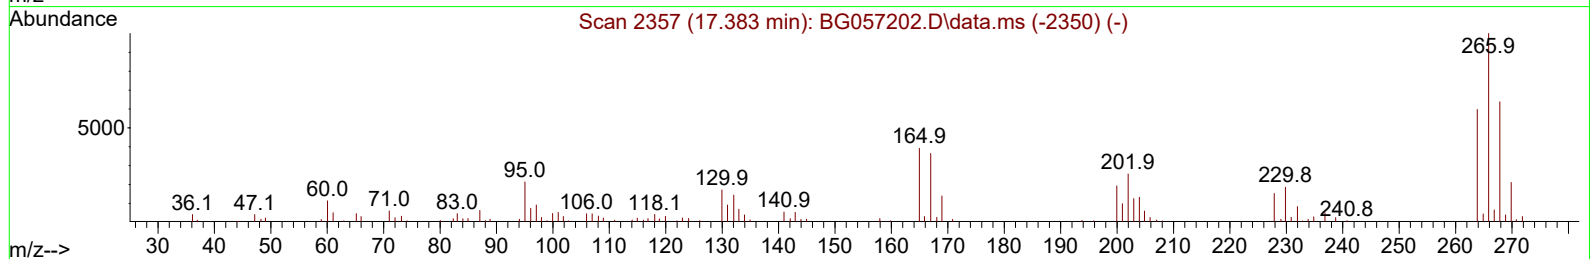
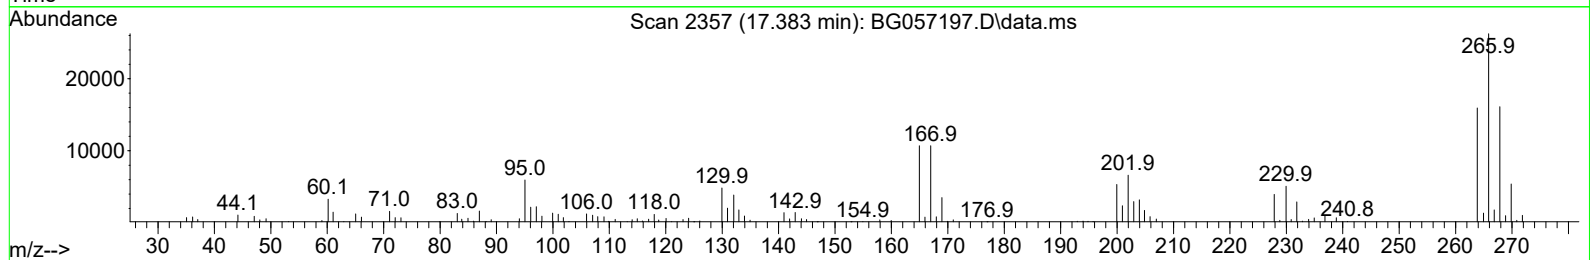


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042723\
Data File : BG057197.D
Acq On : 27 Apr 2023 16:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 05:29:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 28 04:39:54 2023
Response via : Initial Calibration

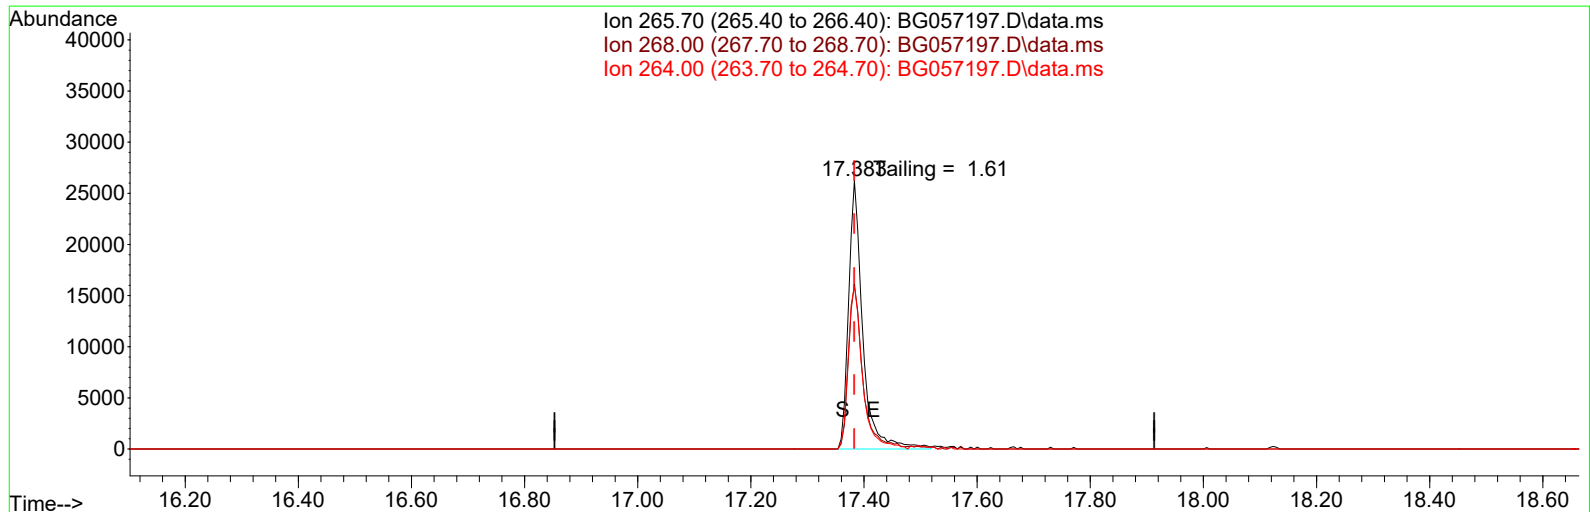

TIC: BG057197.D\data.ms

(70) Pentachlorophenol (C)




17.383min (+ 0.000) 26571.93 ng

response 45780

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	61.39
264.00	59.70	60.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042723\
Data File : BG057197.D
Acq On : 27 Apr 2023 16:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 05:29:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 28 04:39:54 2023
Response via : Initial Calibration

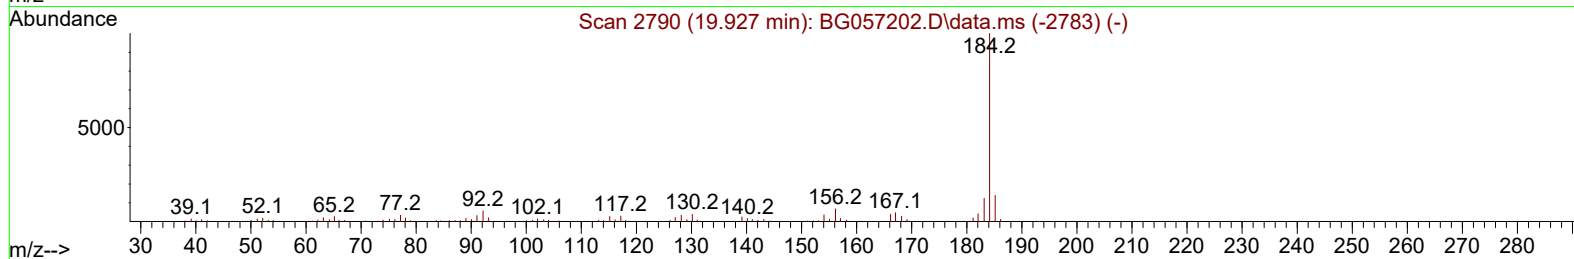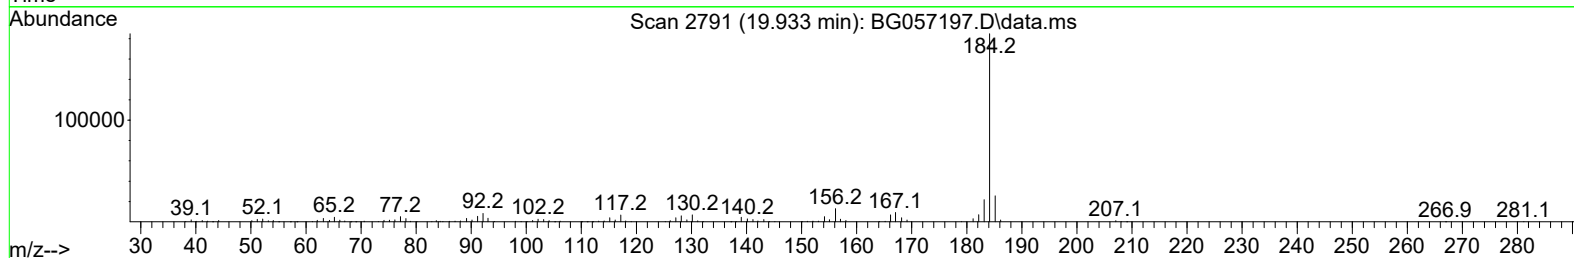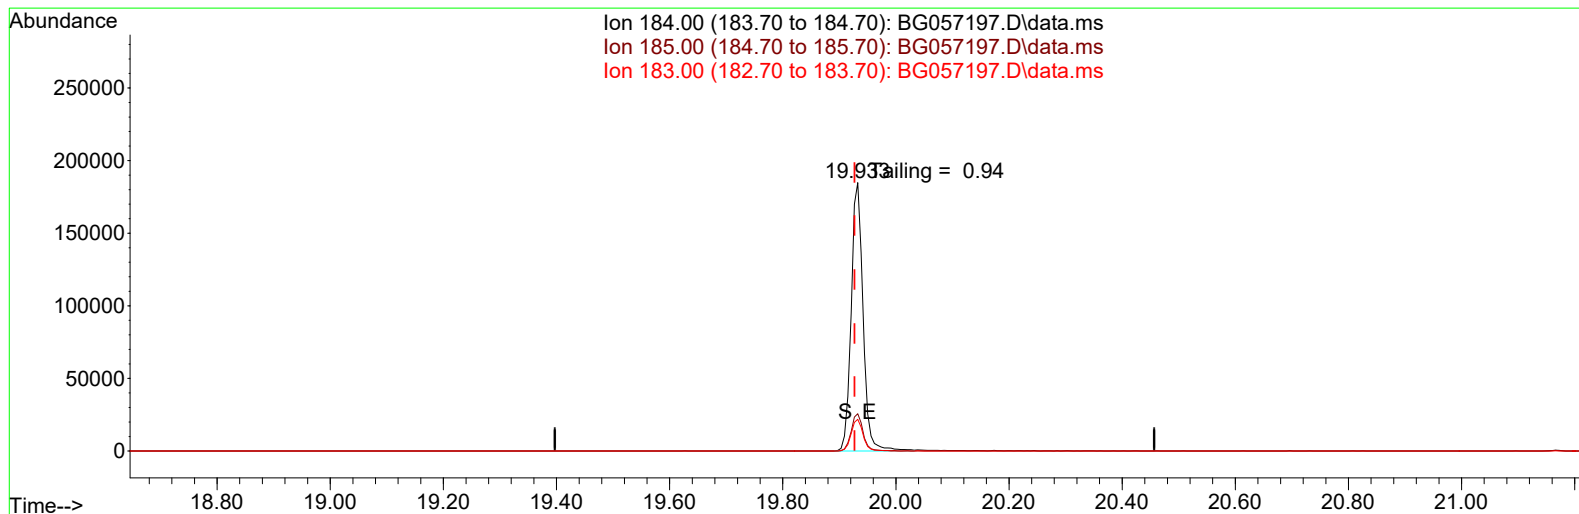

TIC: BG057197.D\data.ms

(77) Benzidine

19.933min (+ 0.006) 0.00 ng

response 271900

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.90
183.00	12.40	11.85
0.00	0.00	0.00