


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042723\
Data File : BG057197.D
Acq On : 27 Apr 2023 16:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 28 04:39:54 2023

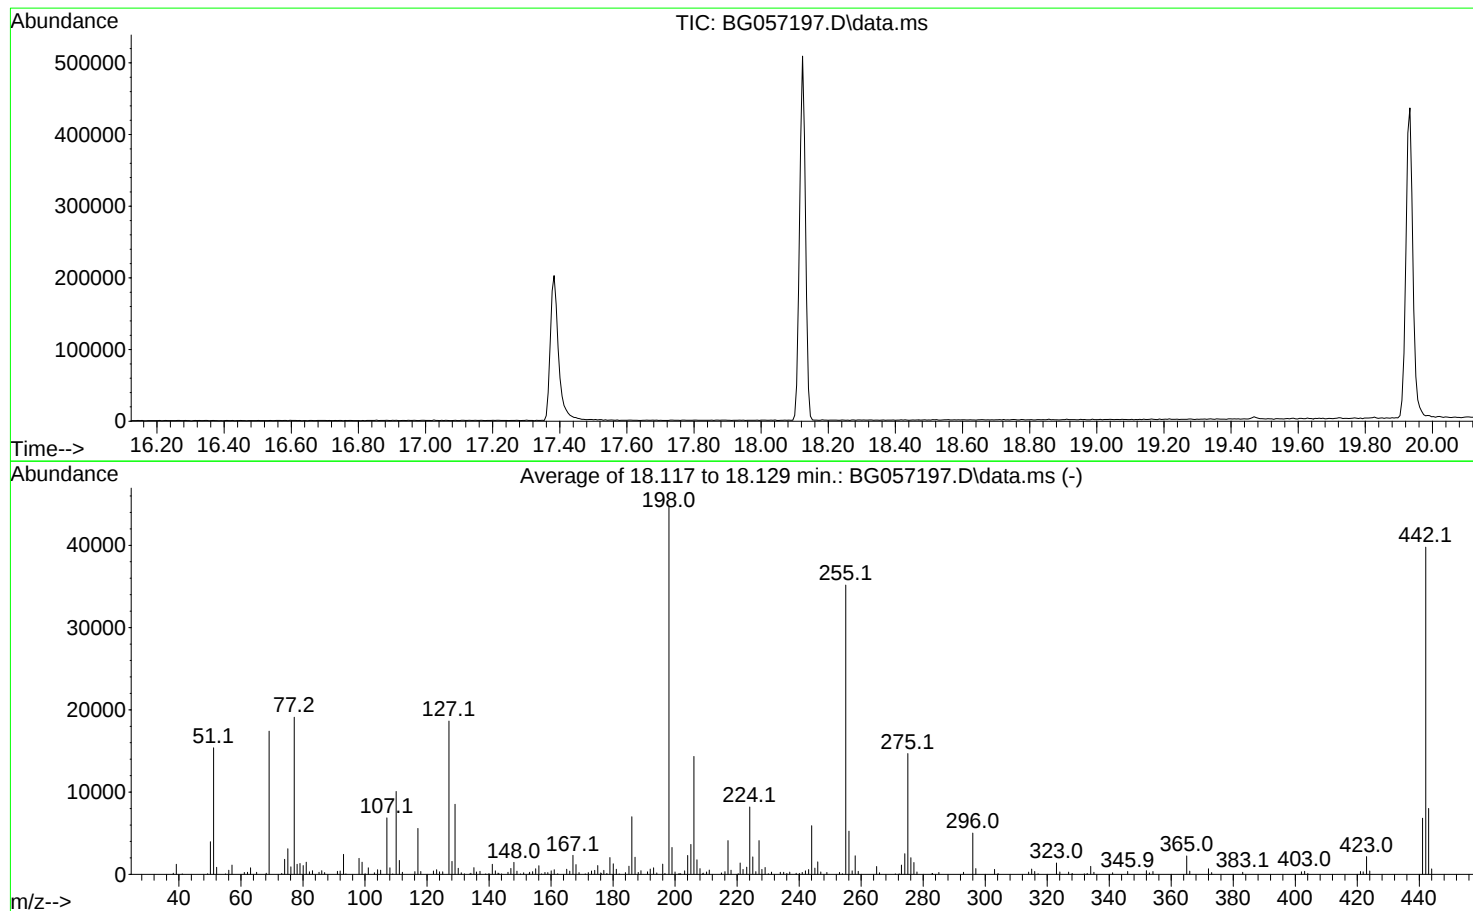

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	15381	PASS
68	69	0.00	2	0.8	140	PASS
69	198	0.00	100	38.9	17404	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.7	18632	PASS
197	198	0.00	2	0.3	117	PASS
198	198	100	100	100.0	44720	PASS
199	198	5	9	7.3	3279	PASS
275	198	10	60	32.9	14696	PASS
365	198	1	100	5.0	2247	PASS
441	198	0.01	100	15.3	6834	PASS
442	442	50	100	100.0	39787	PASS
443	442	15	24	20.2	8018	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/27/2023	BNA_G	<u>BG057197.D</u>
Compound Name	Response	Retention Time
DDT	136726	21.166
DDD	1788	20.761
DDE	0	20.206
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1788	138514	1.29

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042723\
Data File : BG057197.D
Acq On : 27 Apr 2023 16:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 28 05:29:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 28 04:39:54 2023
Response via : Initial Calibration

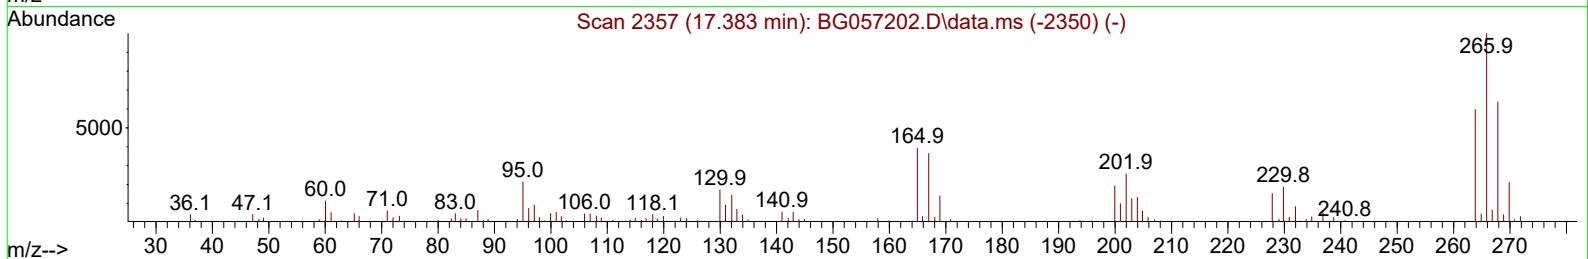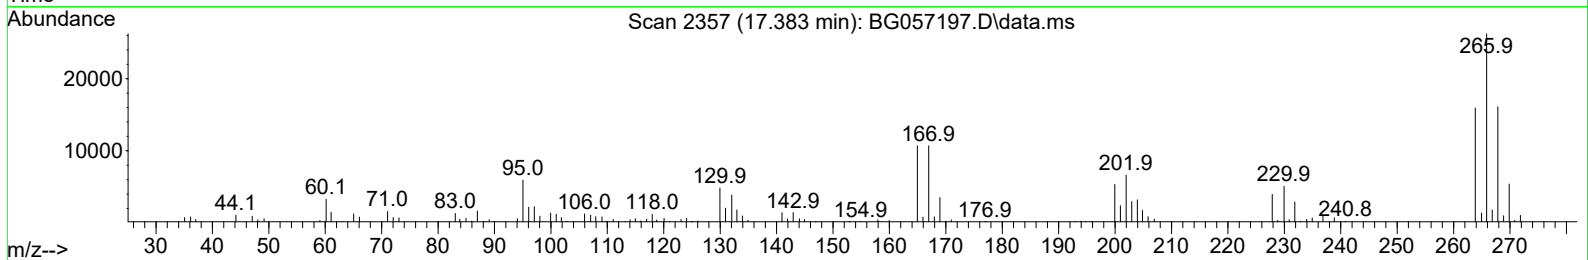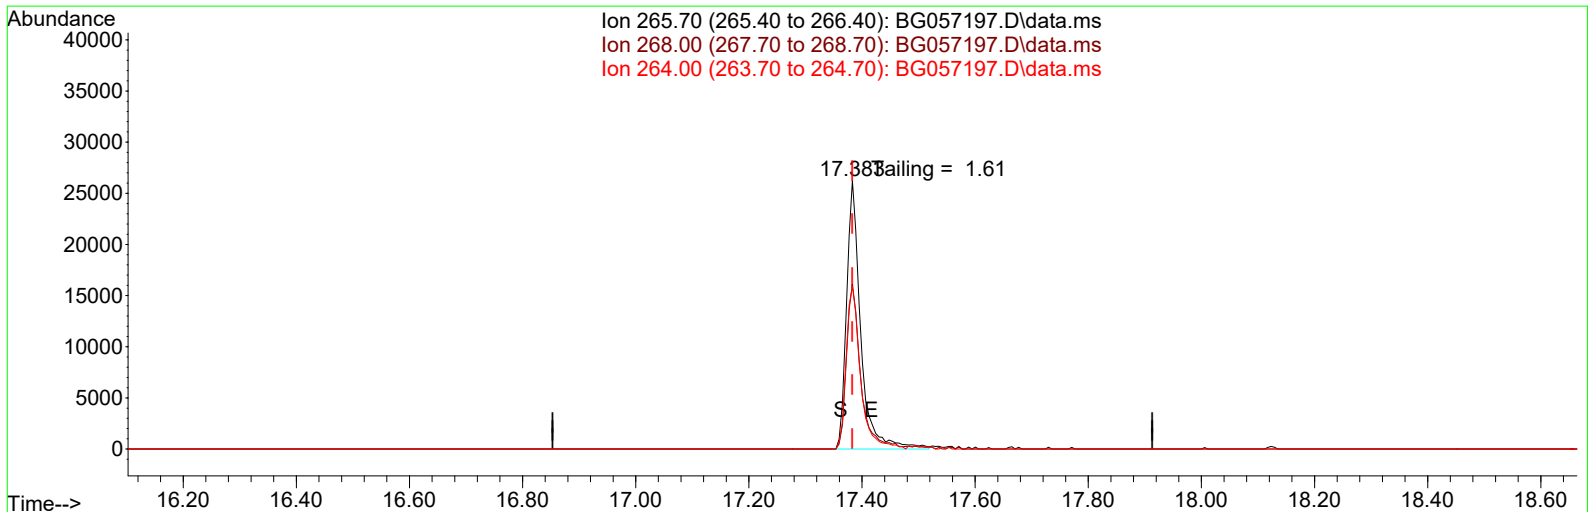

TIC: BG057197.D\data.ms

(70) Pentachlorophenol (C)

17.383min (+ 0.000) 26571.93 ng




response 45780

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	61.39
264.00	59.70	60.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042723\
Data File : BG057197.D
Acq On : 27 Apr 2023 16:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 28 05:29:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 28 04:39:54 2023
Response via : Initial Calibration

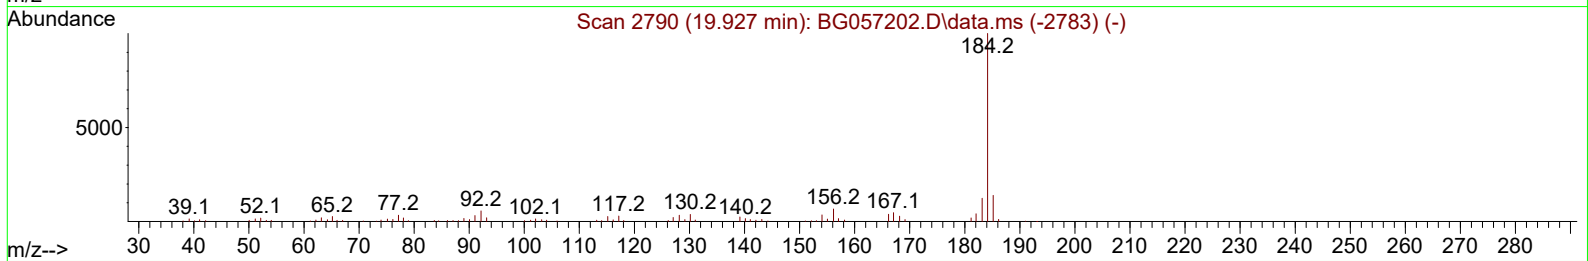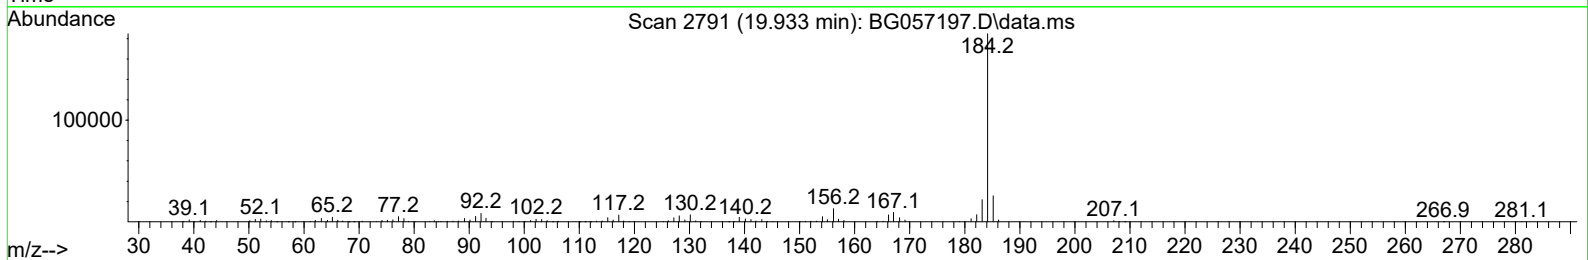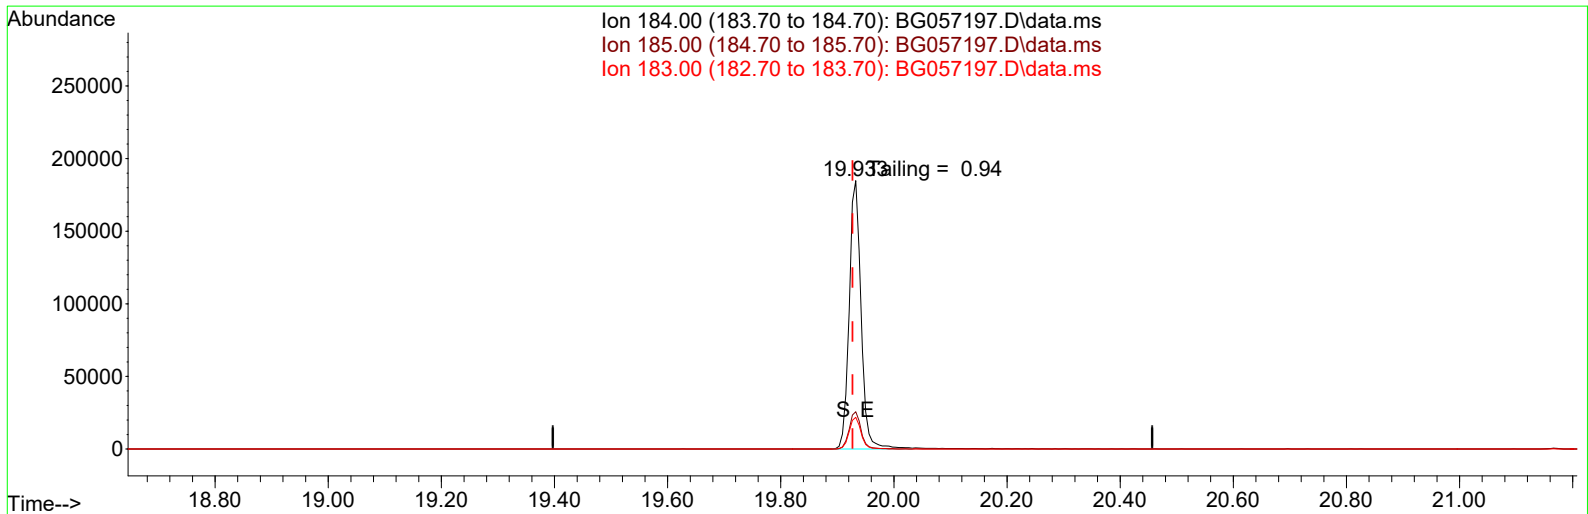

TIC: BG057197.D\data.ms

(77) Benzidine

19.933min (+ 0.006) 0.00 ng

response 271900

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.90
183.00	12.40	11.85
0.00	0.00	0.00