

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG042820\
 Data File : BG045196.D
 Acq On : 28 Apr 2020 22:13
 Operator : CG/JU
 Sample : L2428-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Apr 29 01:20:05 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 28 14:34:23 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.99	152	50122	20.00	ng	0.00
21) Naphthalene-d8	10.80	136	207428	20.00	ng	0.00
39) Acenaphthene-d10	14.63	164	169984	20.00	ng	0.00
64) Phenanthrene-d10	17.38	188	417524	20.00	ng	0.00
76) Chrysene-d12	21.64	240	409032	20.00	ng	0.00
87) Perylene-d12	24.81	264	431701	20.00	ng	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.56	112	207138	68.23	ng	0.00
7) Phenol-d6	7.15	99	330757	73.33	ng	0.00
23) Nitrobenzene-d5	9.15	82	223234	49.11	ng	0.00
42) 2,4,6-Tribromophenol	16.12	330	214942	81.85	ng	0.00
45) 2-Fluorobiphenyl	13.25	172	603010	52.02	ng	0.00
79) Terphenyl-d14	19.99	244	1155302	61.56	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
9) Benzaldehyde	7.11	77	134	Below Cal	#	4
19) n-Nitroso-di-n-propylamine	9.15	70	29897	9.372 ng	#	78
32) Benzoic acid	10.05	122	79	6.400 ng	#	1
50) Dimethylphthalate	14.08	163	87293	6.307 ng		98
57) 2,4-Dinitrotoluene	14.63	165	21720	4.801 ng	#	22
67) 4-Bromophenyl-phenylether	16.12	248	13726	2.548 ng	#	1
69) Atrazine	16.99	200	61	Below Cal	#	35
74) Di-n-butylphthalate	18.34	149	786	Below Cal	#	61
75) Fluoranthene	19.43	202	7307	Below Cal		94
77) Benzidine	19.99	184	19765	Below Cal	#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG042820\
Data File : BG045196.D
Acq On : 28 Apr 2020 22:13
Operator : CG/JU
Sample : L2428-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Apr 29 01:20:05 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 28 14:34:23 2020
Response via : Initial Calibration

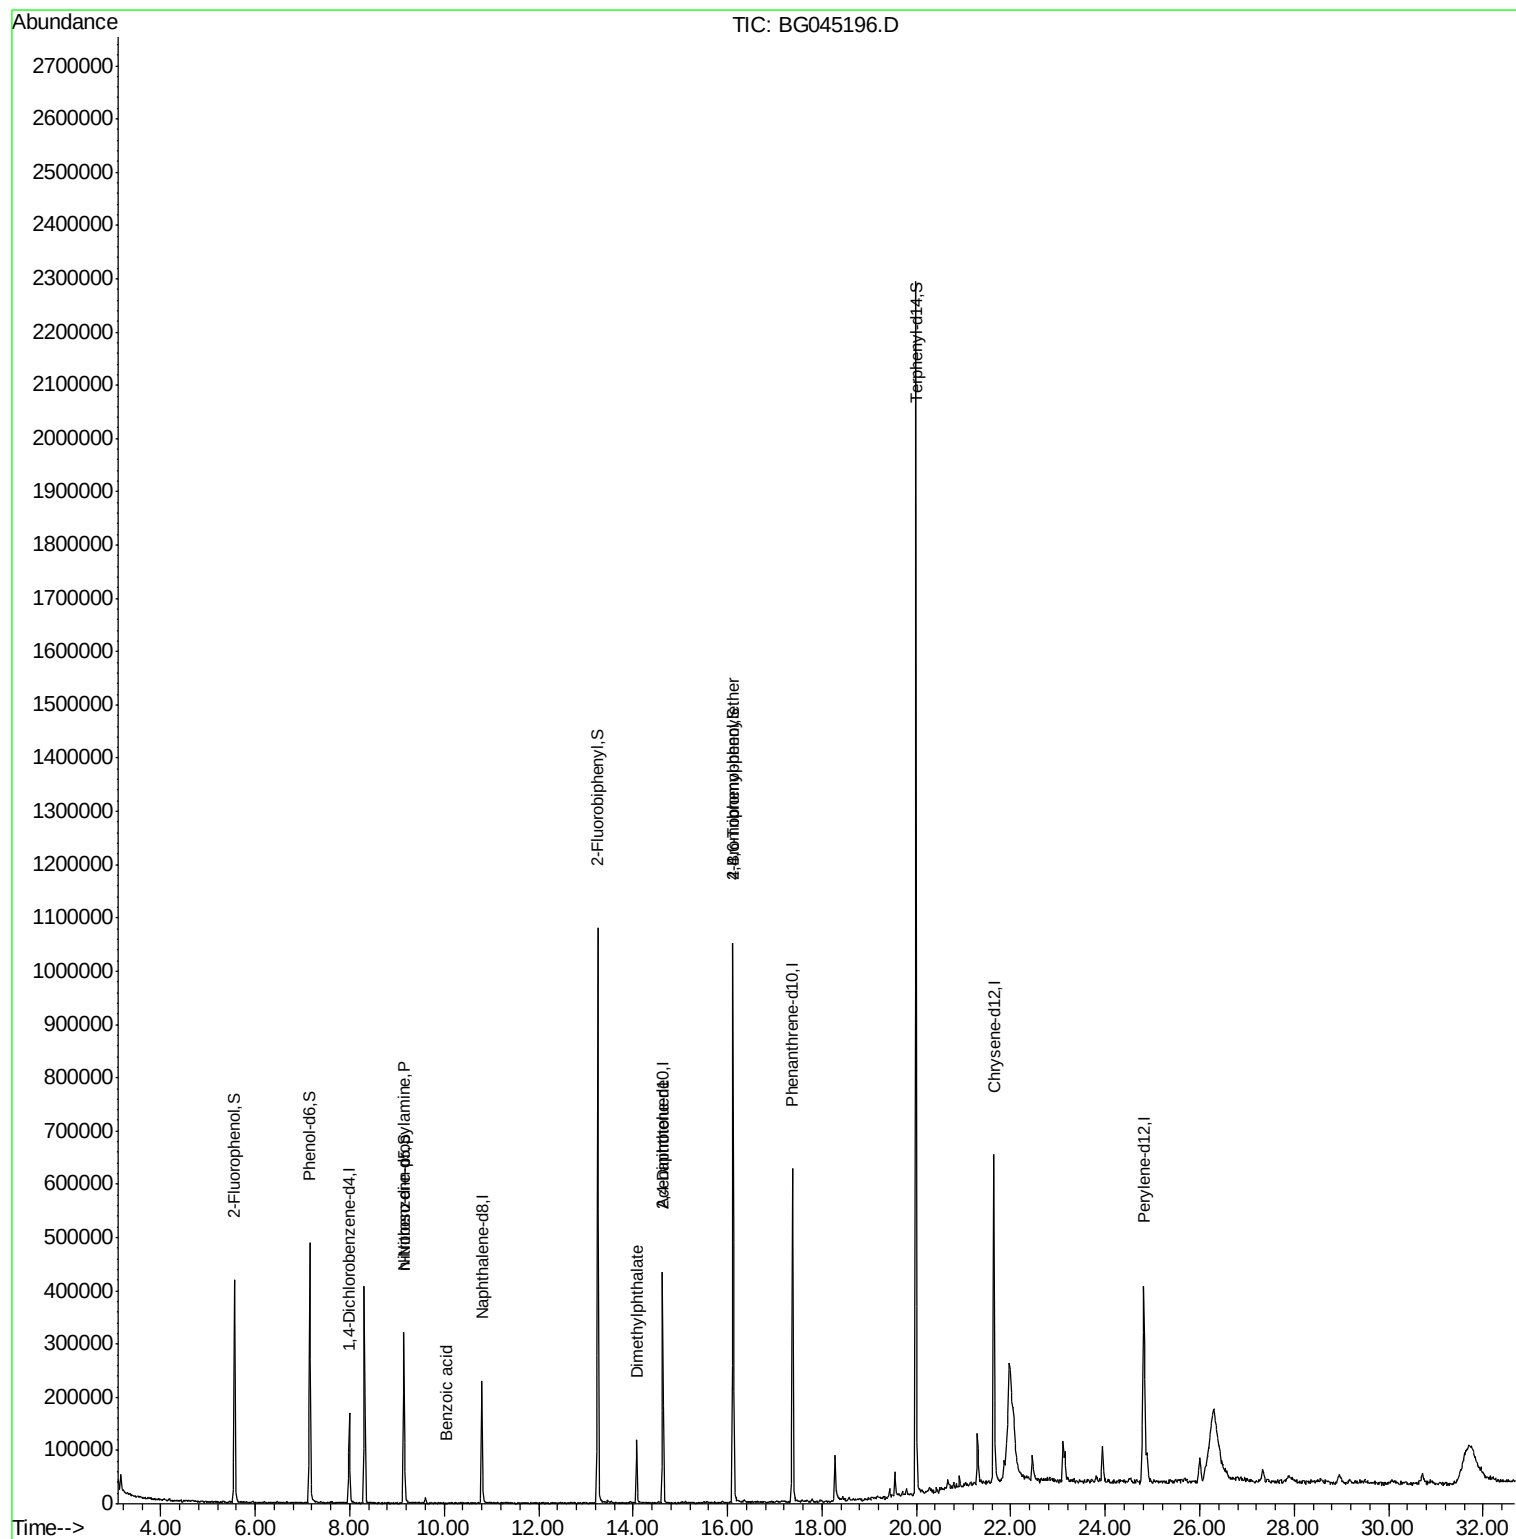




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.99 min Scan# 834
Delta R.T. 0.00 min
Lab File: BG045196.D
Acq: 28 Apr 2020 22:13

Instrument :
BNA_G
ClientSampled :

Tot Ion	Ratio	Lower	Upper
152	100		
150	168.8	123.6	185.4
115	68.6	49.1	73.7

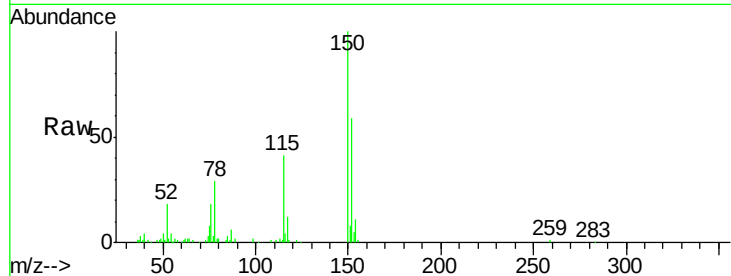


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

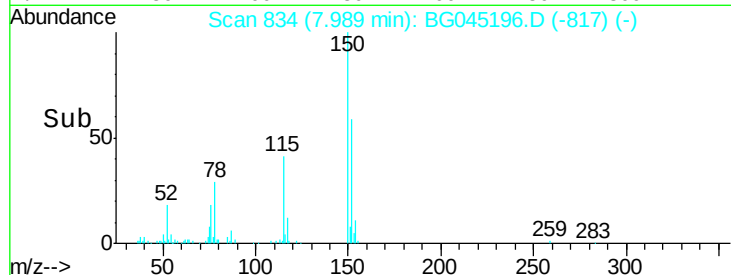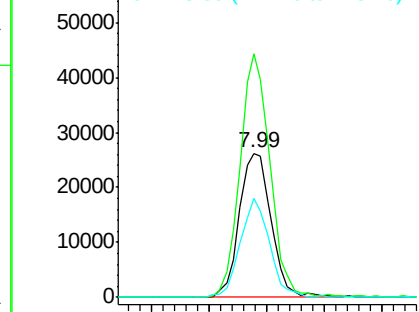



#5




2-Fluorophenol
Concen: 68.228 ng
RT: 5.56 min Scan# 420
Delta R.T. -0.00 min
Lab File: BG045196.D
Acq: 28 Apr 2020 22:13

Tgt Ion	Ratio	Lower	Upper
112	100		
64	59.0	42.4	63.6
63	31.0	23.1	34.7



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG0
Ion 63.00 (62.70 to 63.70): BG0

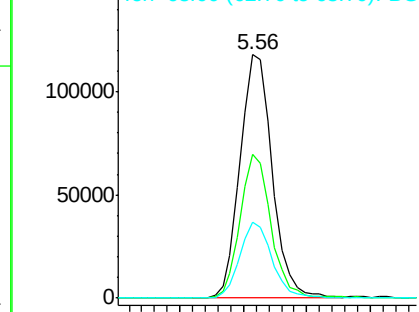

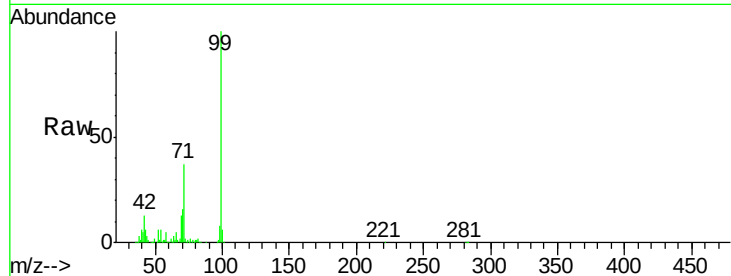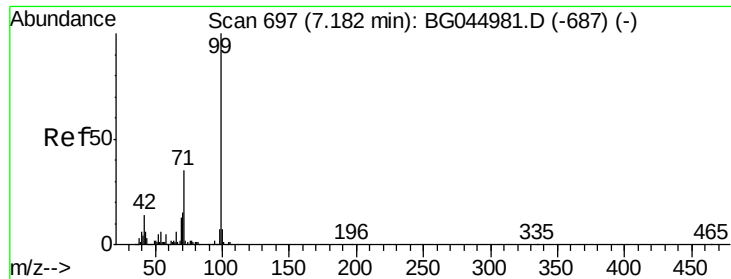

#7

Phenol-d6

Concen: 73.328 ng

RT: 7.15 min Scan# 692

Delta R.T. 0.00 min

Lab File: BG045196.D

Acq: 28 Apr 2020 22:13

Instrument :

BNA_G

ClientSampleId :





Tot Ion: 99 Resp: 330757

Ion Ratio Lower Upper

99 100

42 13.2 11.3 16.9

71 36.7 28.3 42.5

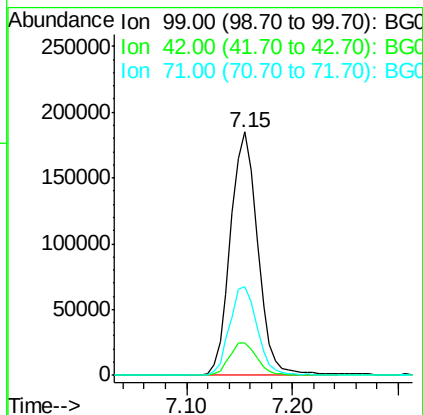

#19

n-Nitroso-di-n-propylamine

Concen: 9.372 ng

RT: 9.15 min Scan# 1031

Delta R.T. 0.35 min

Lab File: BG045196.D

Acq: 28 Apr 2020 22:13

Tgt Ion: 70 Resp: 29897


Ion Ratio Lower Upper


70 100

42 33.5 33.3 49.9

101 0.0 7.8 11.8#

130 2.4 15.8 23.6#




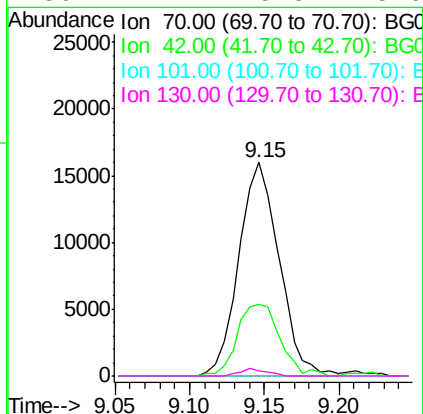


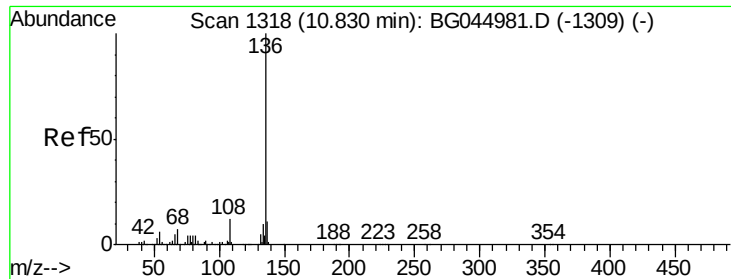

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.80 min Scan# 1312
Delta R.T. -0.00 min
Lab File: BG045196.D
Acq: 28 Apr 2020 22:13




Instrument :
BNA_G
ClientSampleId :


Tot Ion:136	Resp:	207428
Ion	Ratio	Lower Upper
136	100	
137	10.4	8.6 13.0
54	6.6	4.8 7.2
68	4.8	5.2 7.8

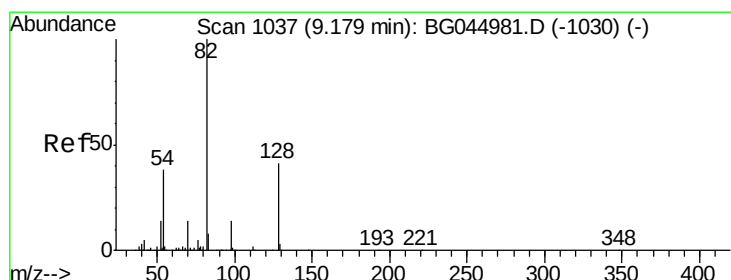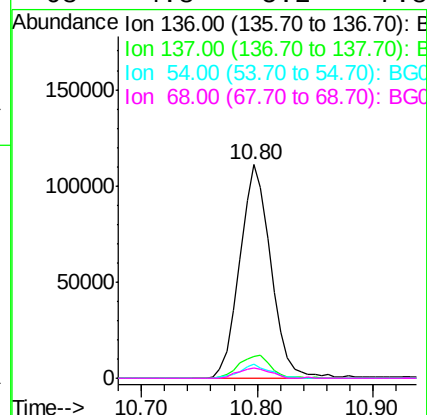

#23
Nitrobenzene-d5
Concen: 49.106 ng
RT: 9.15 min Scan# 1031
Delta R.T. -0.00 min
Lab File: BG045196.D
Acq: 28 Apr 2020 22:13

Tgt Ion: 82	Resp:	223234
Ion	Ratio	Lower Upper
82	100	
128	40.8	33.0 49.4
54	42.6	30.4 45.6

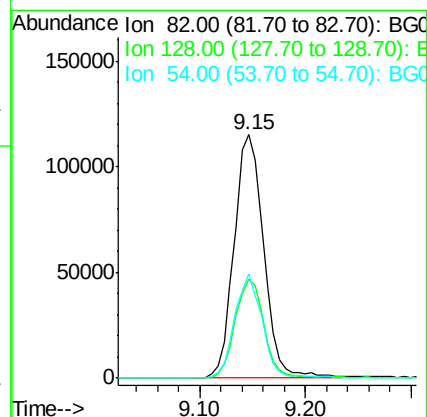



#32

Benzoic acid

Concen: 6.400 ng

RT: 10.05 min Scan# 1185

Delta R.T. -0.06 min

Lab File: BG045196.D


Acq: 28 Apr 2020 22:13

Instrument :

BNA_G

ClientSampleId :




Tot Ion	Ratio	Lower	Upper
122	100		
105	0.0	108.4	148.4#
77	0.0	78.8	118.8#

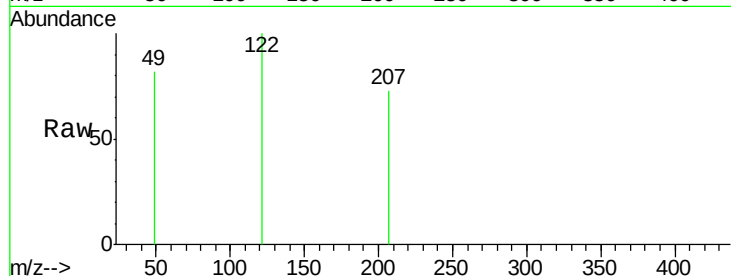

Abundance Ion 122.00 (121.70 to 122.70): E

Ion 105.00 (104.70 to 105.70): E

Ion 77.00 (76.70 to 77.70): B

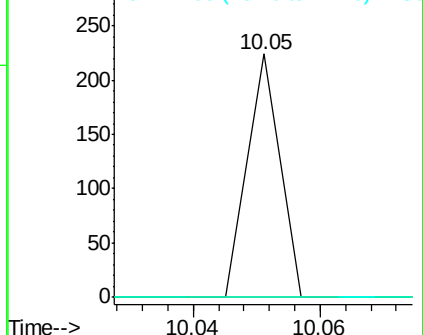

#39

Acenaphthene-d10

Concen: 20.000 ng


RT: 14.63 min Scan# 1964

Delta R.T. -0.00 min

Lab File: BG045196.D

Acq: 28 Apr 2020 22:13



Tgt Ion	Ratio	Lower	Upper
164	100		
162	96.6	78.7	118.1
160	43.7	32.8	49.2




Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E



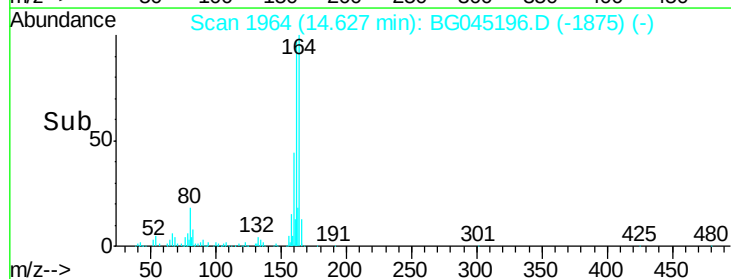
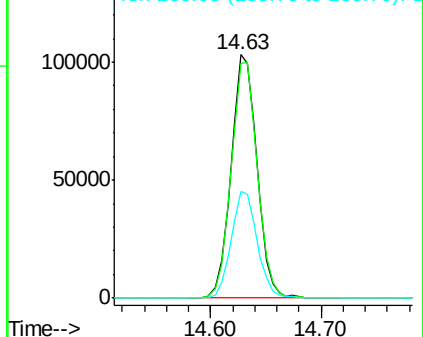


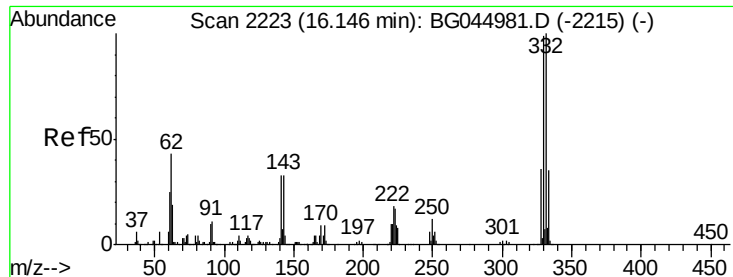

#42
2,4,6-Tribromophenol
Concen: 81.851 ng
RT: 16.12 min Scan# 2218
Delta R.T. -0.00 min
Lab File: BG045196.D
Acq: 28 Apr 2020 22:13




Instrument :
BNA_G
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
330	100		
332	96.7	79.1	118.7
141	34.6	27.1	40.7

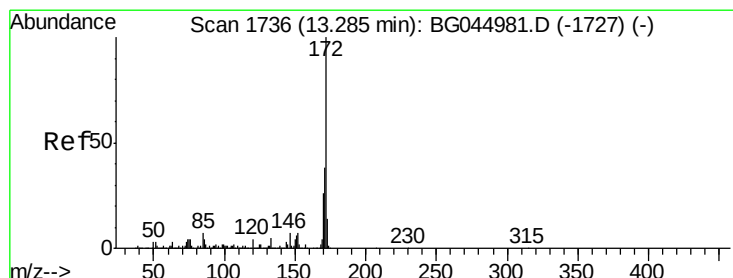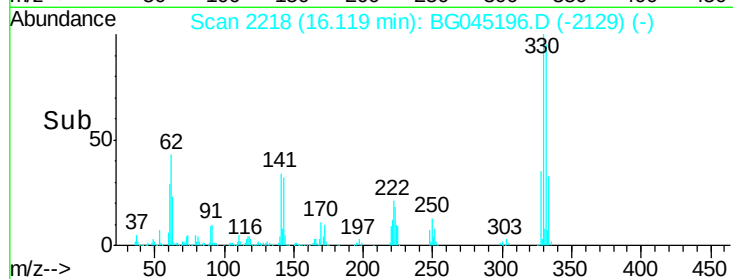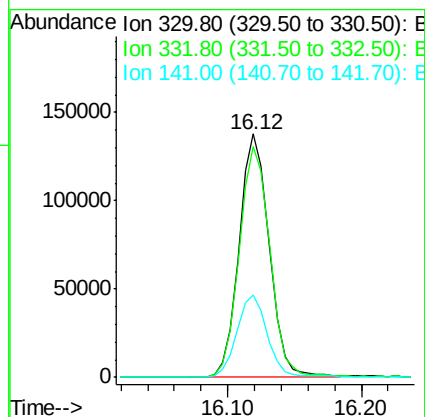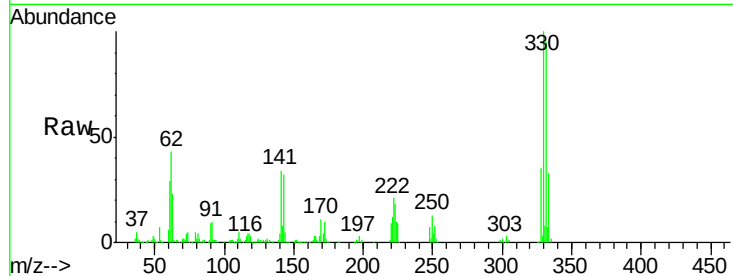

#45
2-Fluorobiphenyl
Concen: 52.017 ng
RT: 13.25 min Scan# 1730
Delta R.T. -0.00 min
Lab File: BG045196.D
Acq: 28 Apr 2020 22:13

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.1	30.6	46.0
170	23.8	20.5	30.7


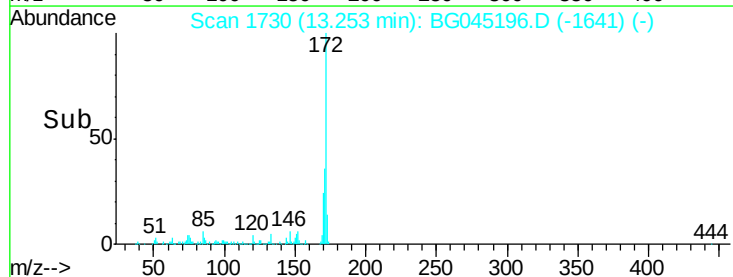
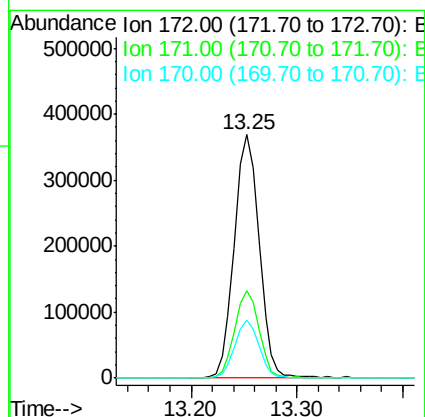
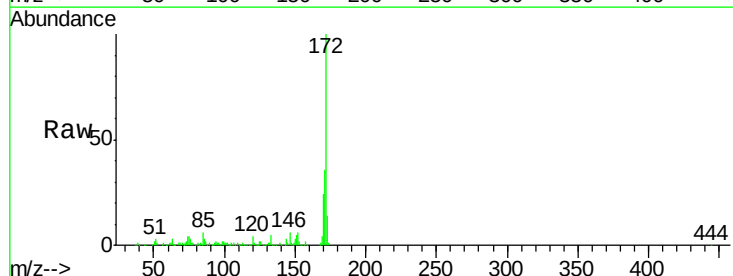




#50
Dimethylphthalate
Concen: 6.307 ng
RT: 14.08 min Scan# 1870
Delta R.T. -0.01 min
Lab File: BG045196.D
Acq: 28 Apr 2020 22:13




Instrument :
BNA_G
ClientSampleId :


Tot Ion	Ion	Ratio	Lower	Upper
163	100			
194	3.6	3.5	5.3	
164	11.0	8.2	12.4	

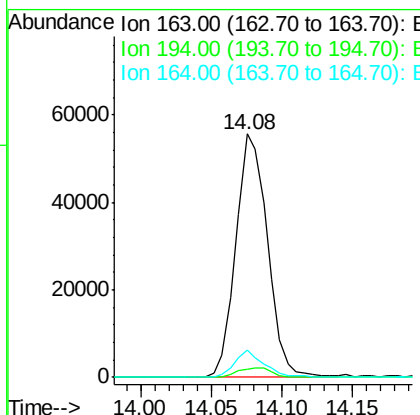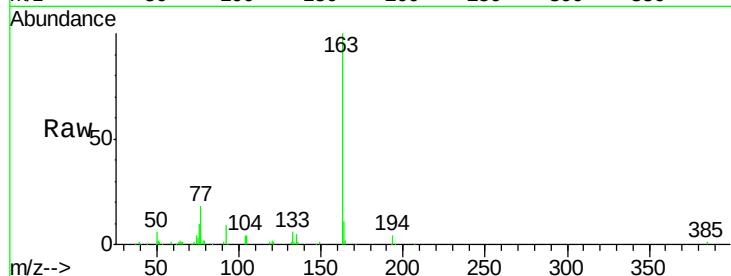

#57
2,4-Dinitrotoluene
Concen: 4.801 ng
RT: 14.63 min Scan# 1964
Delta R.T. -0.36 min
Lab File: BG045196.D
Acq: 28 Apr 2020 22:13

Tgt Ion	Ion	Ratio	Lower	Upper
165	100			
63	2.3	32.2	48.2#	
89	0.0	61.7	92.5#	
182	0.0	2.0	3.0#	


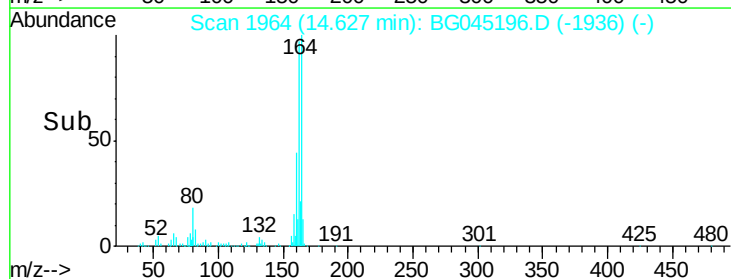
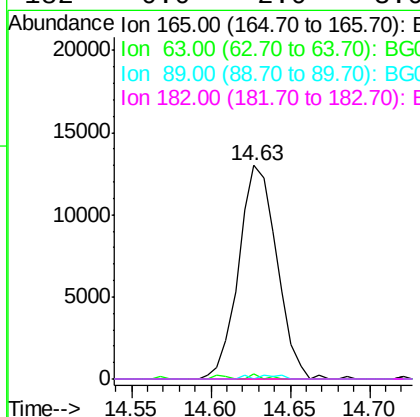



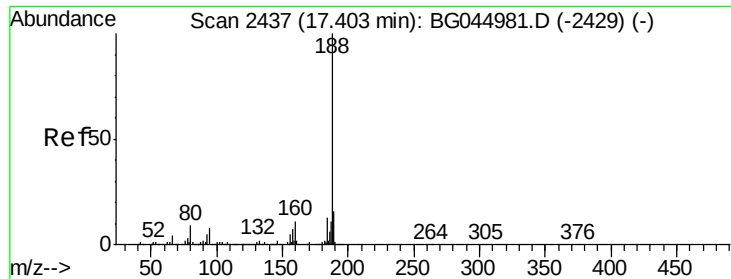

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.38 min Scan# 2432
 Delta R.T. -0.00 min
 Lab File: BG045196.D
 Acq: 28 Apr 2020 22:13




Instrument :
 BNA_G
 ClientSampleId :


Tot Ion:188 Resp: 417524
 Ion Ratio Lower Upper
 188 100
 94 6.7 6.2 9.4
 80 8.4 7.0 10.6

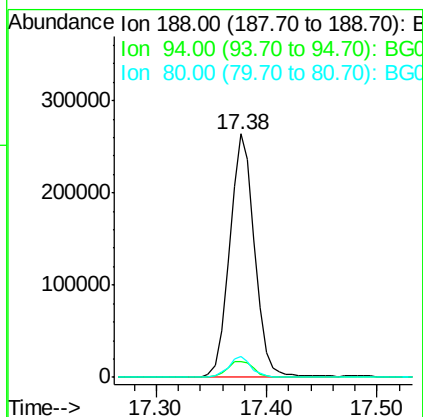

#67
 4-Bromophenyl-phenylether
 Concen: 2.548 ng
 RT: 16.12 min Scan# 2218
 Delta R.T. -0.45 min
 Lab File: BG045196.D
 Acq: 28 Apr 2020 22:13

Tgt Ion:248 Resp: 13726
 Ion Ratio Lower Upper
 248 100
 250 202.7 75.4 113.2#
 141 519.1 54.4 81.6#

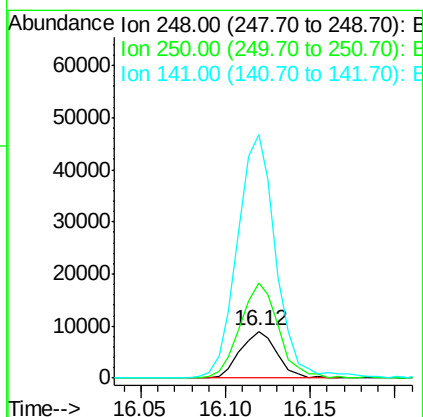



#69

Atrazine

Concen: Below Cal

RT: 16.99 min Scan# 2366

Delta R.T. 0.15 min

Lab File: BG045196.D


Acq: 28 Apr 2020 22:13

Instrument :

BNA_G

ClientSampleId :




Tot Ion	Ratio	Lower	Upper
200	100		
173	0.0	4.5	44.5#
215	0.0	30.0	70.0#

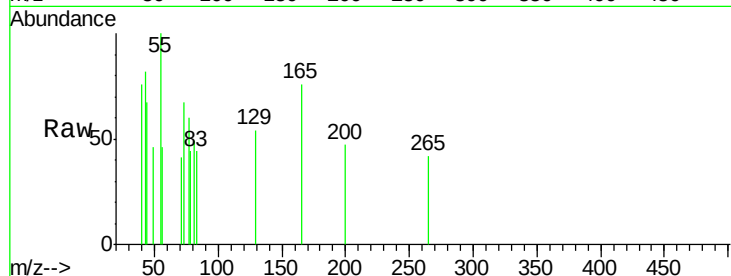

Abundance Ion 200.00 (199.70 to 200.70): E

Ion 173.00 (172.70 to 173.70): E

Ion 215.00 (214.70 to 215.70): E

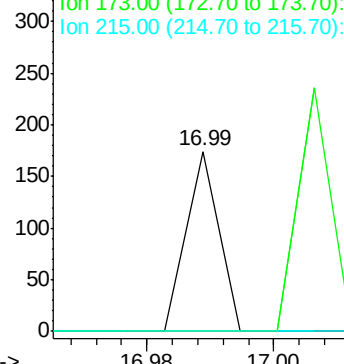

#74

Di-n-butylphthalate

Concen: Below Cal


RT: 18.34 min Scan# 2596

Delta R.T. -0.00 min

Lab File: BG045196.D

Acq: 28 Apr 2020 22:13



Tgt Ion	Ratio	Lower	Upper
149	100		
150	29.5	8.2	12.2#
104	0.0	4.8	7.2#




Abundance Ion 149.00 (148.70 to 149.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 104.00 (103.70 to 104.70): E

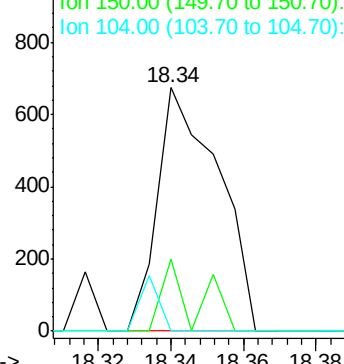



#75

Fluoranthene

Concen: Below Cal

RT: 19.43 min Scan# 2781

Delta R.T. -0.00 min

Lab File: BG045196.D





Acq: 28 Apr 2020 22:13

Instrument :

BNA_G

ClientSampleId :

Tot Ion:	202	Resp:	7307
Ion	Ratio	Lower	Upper
202	100		
101	6.1	0.0	29.6
203	18.1	0.0	39.7

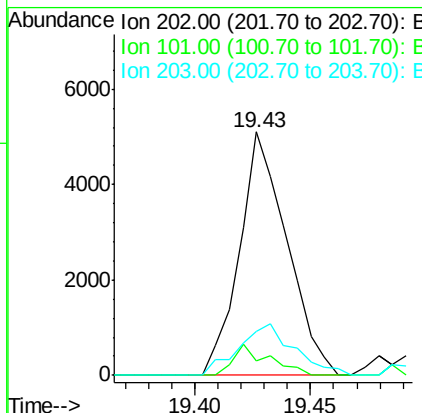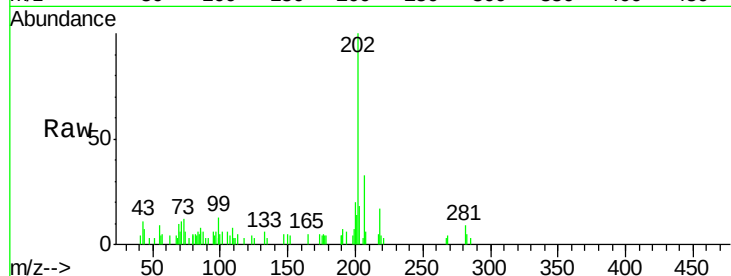

#76

Chrysene-d12

Concen: 20.000 ng




RT: 21.64 min Scan# 3158


Delta R.T. -0.00 min

Lab File: BG045196.D

Acq: 28 Apr 2020 22:13

Tgt Ion:	240	Resp:	409032
Ion	Ratio	Lower	Upper
240	100		
120	7.6	6.6	10.0
236	26.4	22.2	33.2

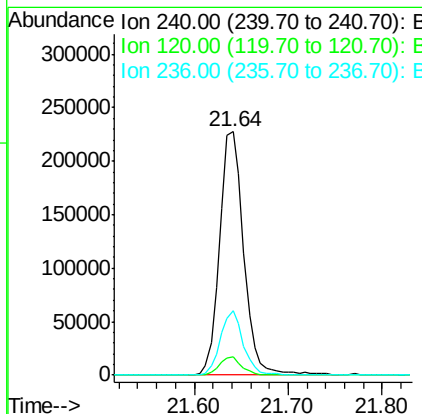

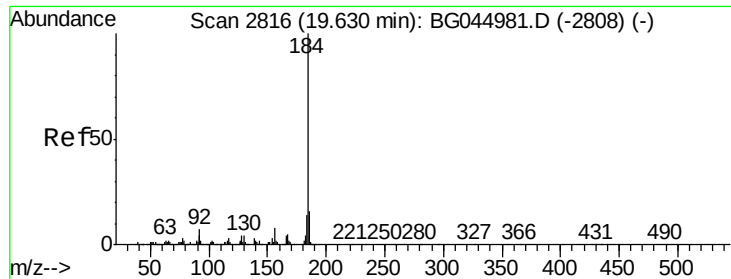

#77

Benzidine

Concen: Below Cal

RT: 19.99 min Scan# 2877

Delta R.T. 0.38 min

Lab File: BG045196.D

Acq: 28 Apr 2020 22:13

Instrument :

BNA_G

ClientSampleId :


Tot Ion:184 Resp: 19765

Ion Ratio Lower Upper

184 100

185 16.4 12.6 19.0




183 9.0 11.3 16.9#

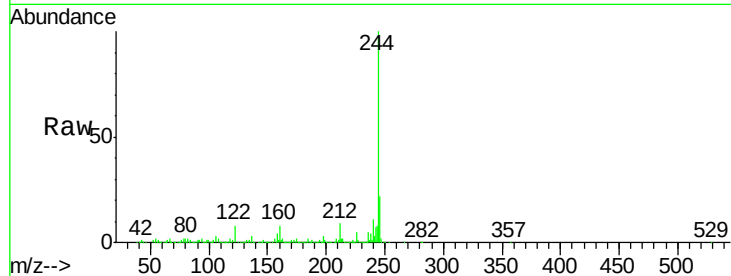

Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

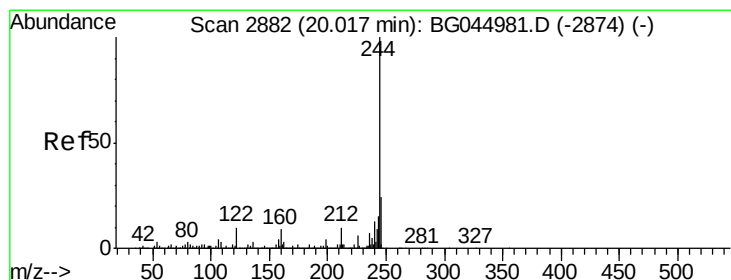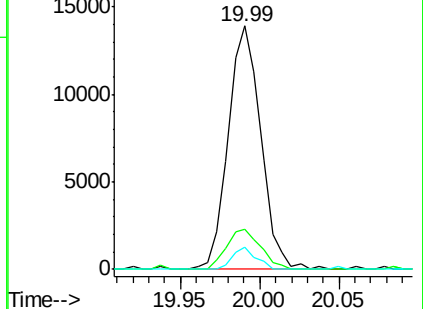

#79

Terphenyl-d14

Concen: 61.561 ng

RT: 19.99 min Scan# 2877

Delta R.T. -0.00 min

Lab File: BG045196.D

Acq: 28 Apr 2020 22:13


Tgt Ion:244 Resp: 1155302

Ion Ratio Lower Upper

244 100

212 8.6 7.9 11.9



122 7.7 7.7 11.5#






Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

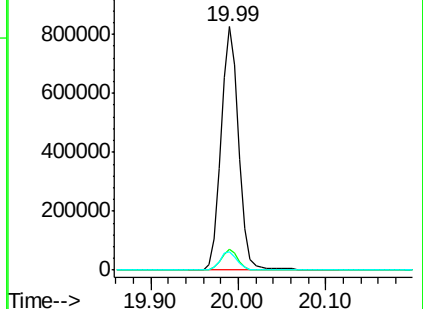

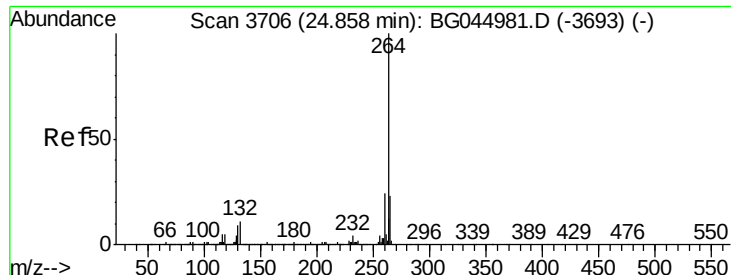

#87
Pervlene-d12
Concen: 20.000 ng
RT: 24.81 min Scan# 3698
Delta R.T. -0.01 min
Lab File: BG045196.D
Acq: 28 Apr 2020 22:13

Instrument :
BNA_G
ClientSampleId :

Tot Ion:	264	Resp:	431701
Ion	Ratio	Lower	Upper
264	100		
260	23.6	19.2	28.8
265	21.3	19.0	28.4

