
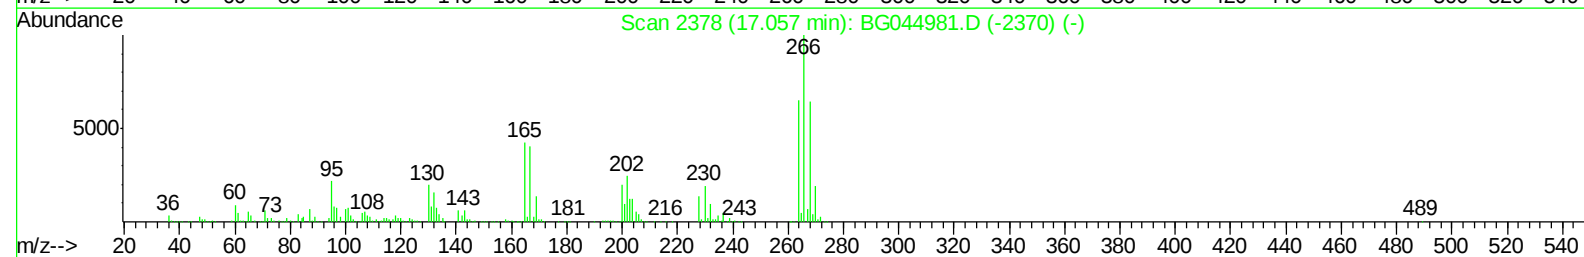
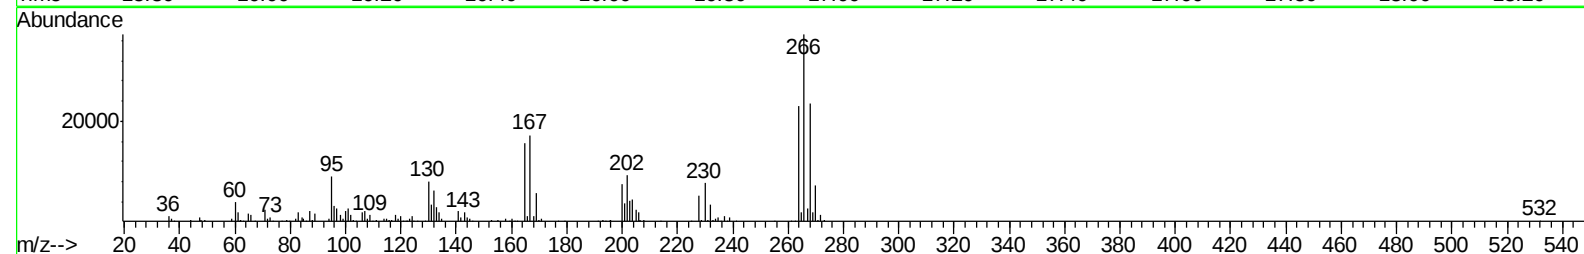


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG042820\
 Data File : BG045183.D
 Acq On : 28 Apr 2020 13:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 02:33:17 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 28 14:34:23 2020
 Response via : Initial Calibration

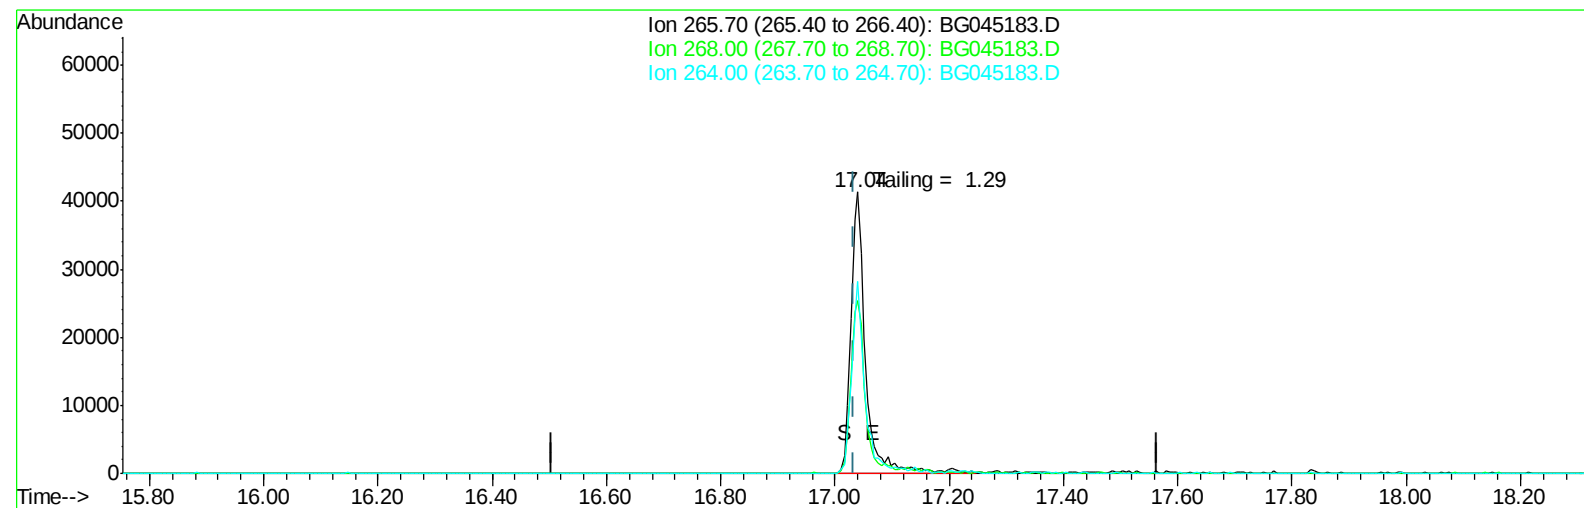

TIC: BG045183.D

(70) Pentachlorophenol (C)




17.040min (+0.005) 121354.66ng

response 70721

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	61.38
264.00	65.30	68.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG042820\
 Data File : BG045183.D
 Acq On : 28 Apr 2020 13:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 02:33:17 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 28 14:34:23 2020
 Response via : Initial Calibration

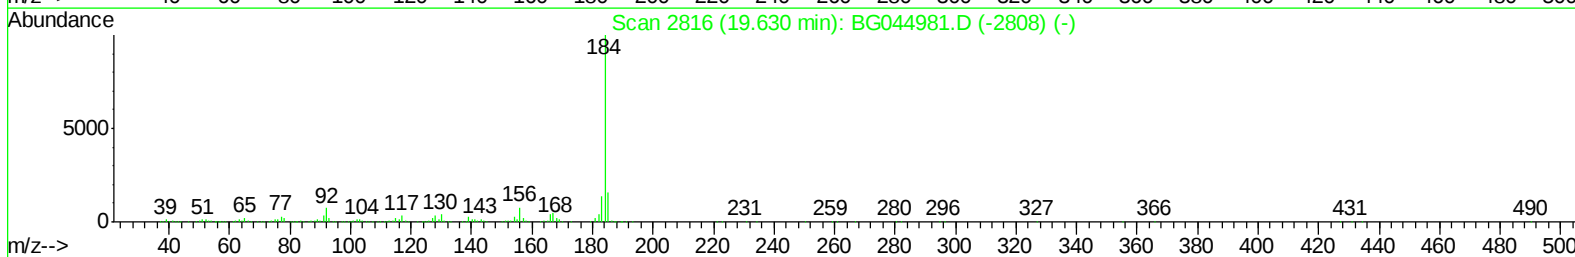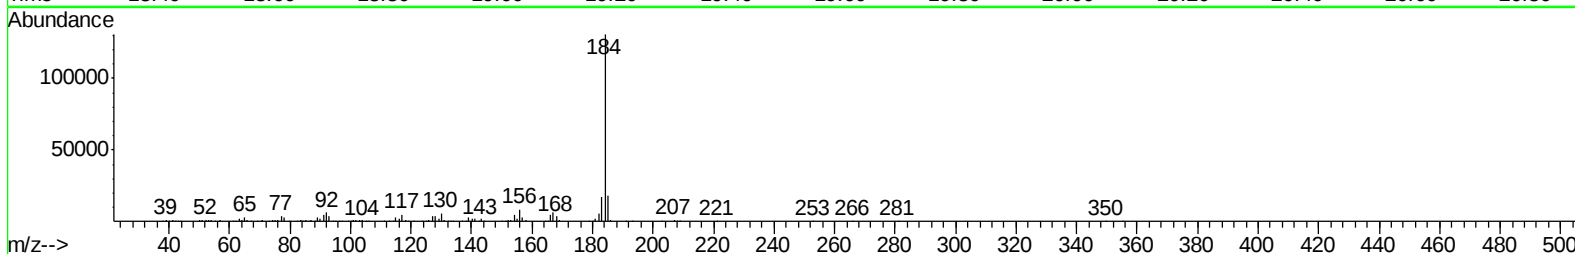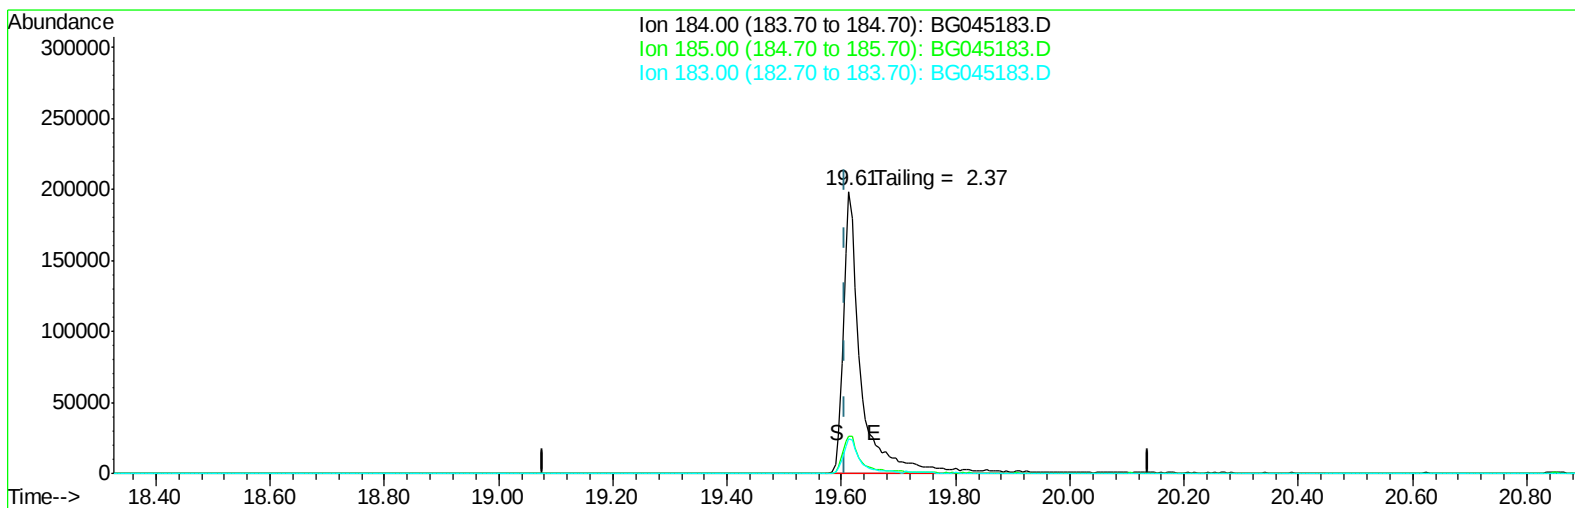

TIC: BG045183.D

(77) Benzidine

19.613min (+0.005) 0.00ng

response 422444

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	13.34
183.00	14.10	12.40
0.00	0.00	0.00