
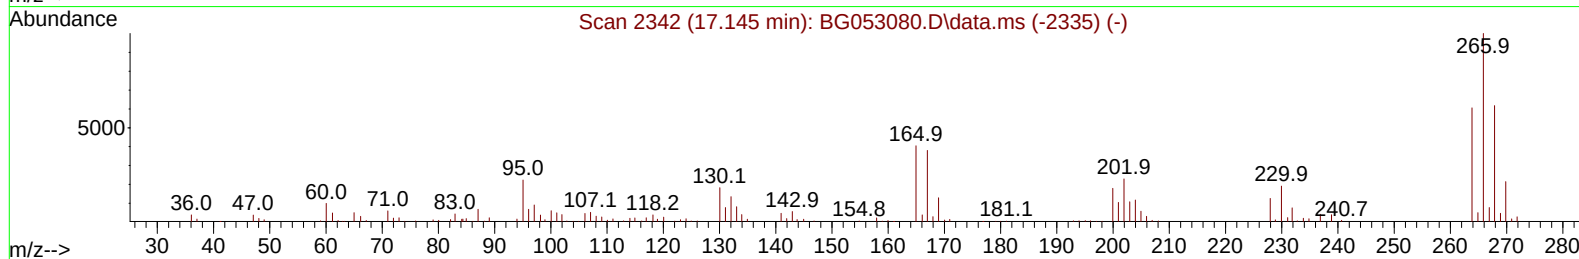
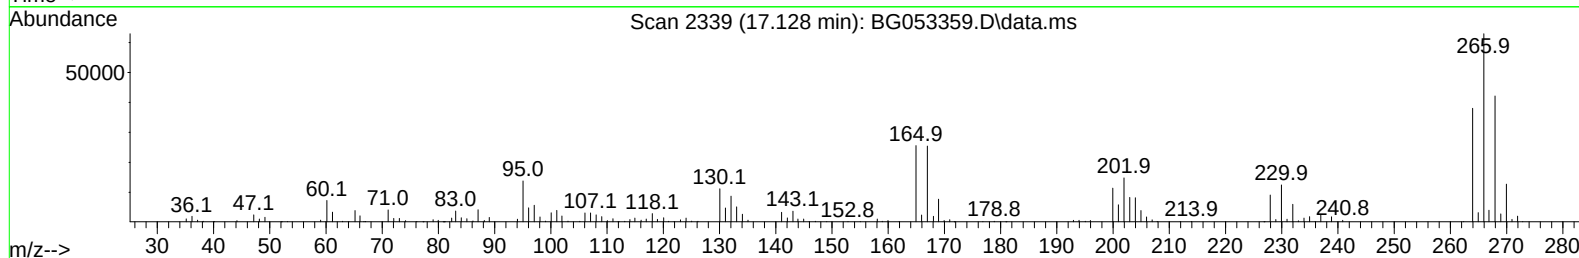


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042822\
Data File : BG053359.D
Acq On : 28 Apr 2022 9:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 06:13:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 01:13:30 2022
Response via : Initial Calibration

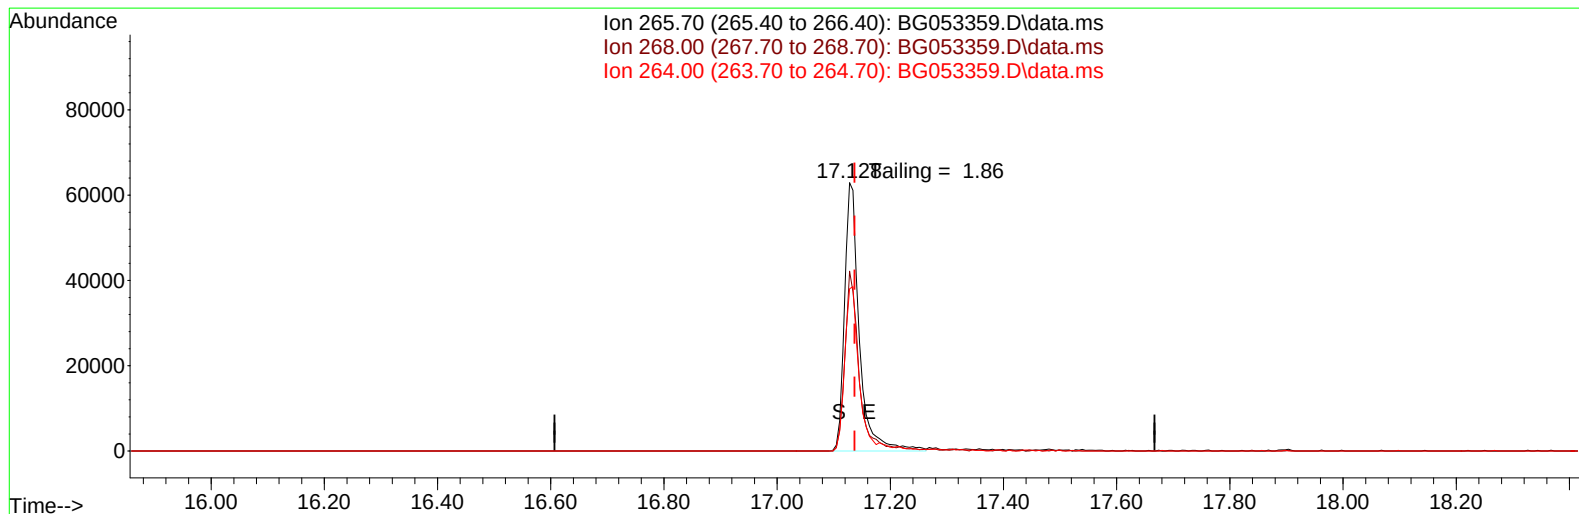

TIC: BG053359.D\data.ms

(70) Pentachlorophenol (C)




17.128min (-0.009) 28292.53 ng

response 114578

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	67.00
264.00	56.60	60.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042822\
 Data File : BG053359.D
 Acq On : 28 Apr 2022 9:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 06:13:30 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Apr 24 01:13:30 2022
 Response via : Initial Calibration

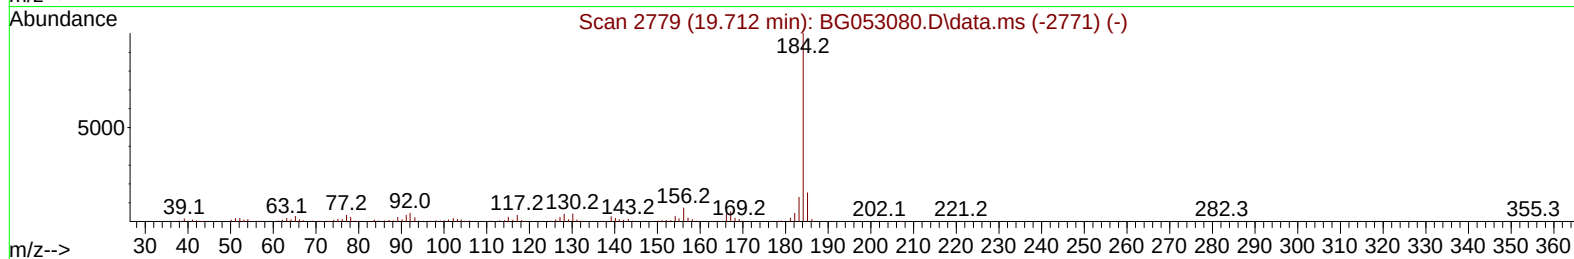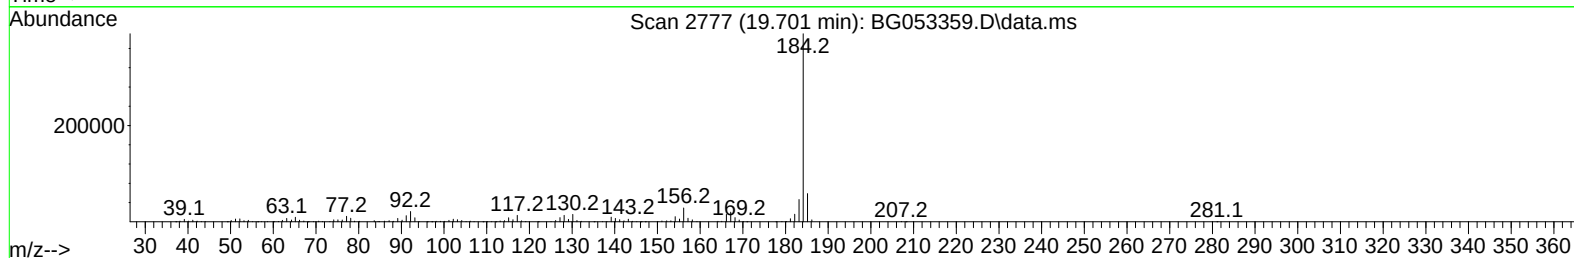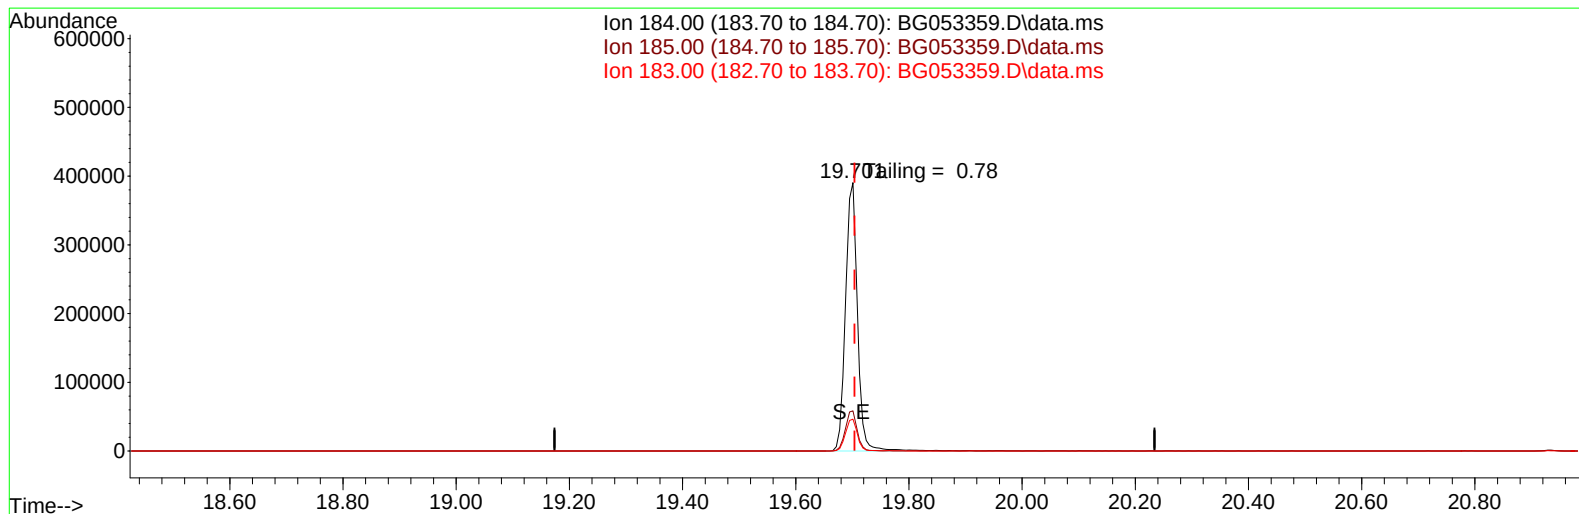

TIC: BG053359.D\data.ms

(77) Benzidine**19.701min (-0.003) 365515.66 ng****response 573581**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.97
183.00	11.80	11.89
0.00	0.00	0.00