
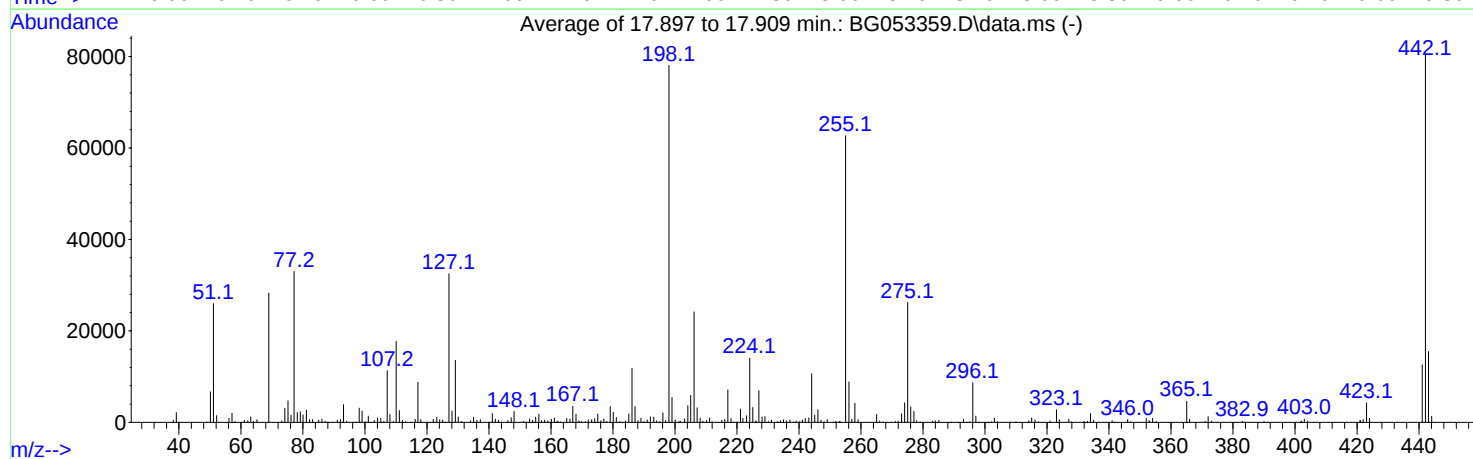


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042822\
 Data File : BG053359.D
 Acq On : 28 Apr 2022 9:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Apr 24 01:13:30 2022

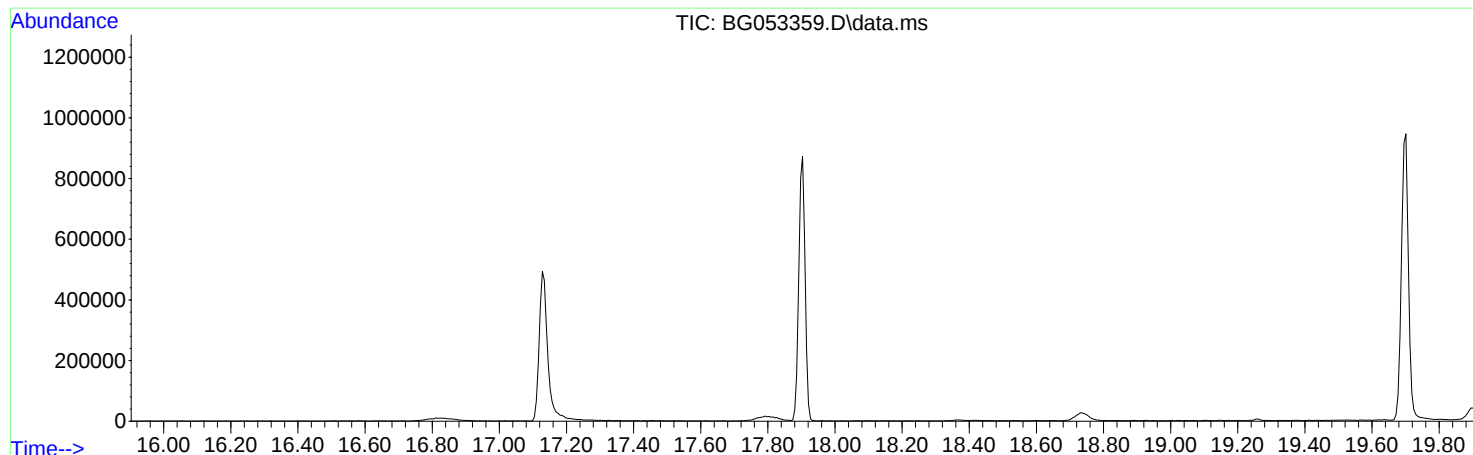




AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	25981	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.2	28290	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.6	32512	PASS
197	198	0.00	2	0.5	376	PASS
198	198	100	100	100.0	78061	PASS
199	198	5	9	7.0	5464	PASS
275	198	10	60	33.6	26208	PASS
365	198	1	100	5.9	4598	PASS
441	198	0.01	100	16.1	12600	PASS
442	442	50	100	100.0	80445	PASS
443	442	15	24	19.3	15493	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042822\
Data File : BG053359.D
Acq On : 28 Apr 2022 9:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 29 06:13:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 01:13:30 2022
Response via : Initial Calibration

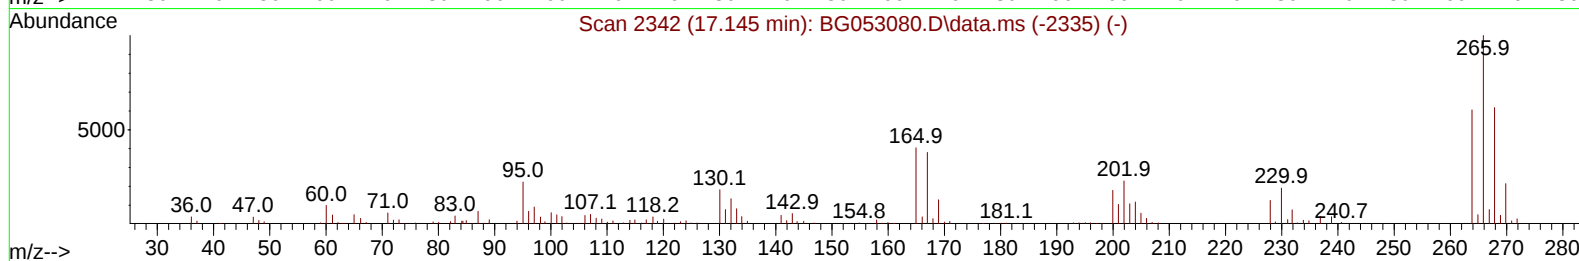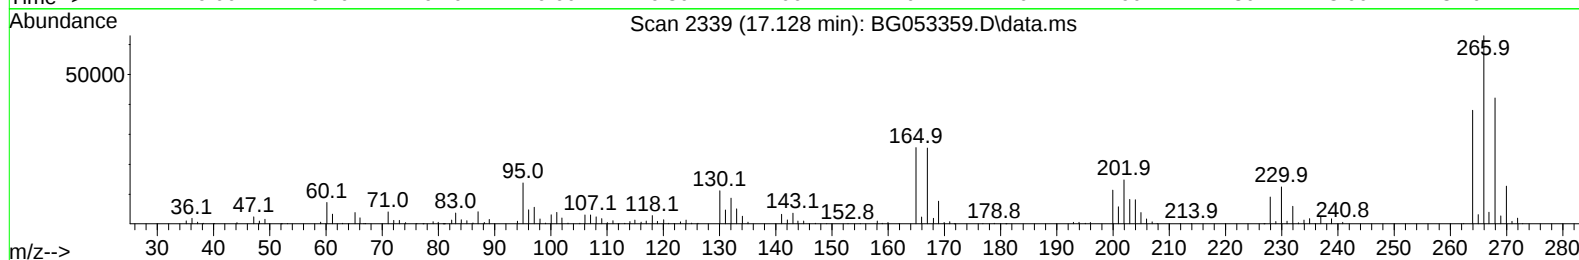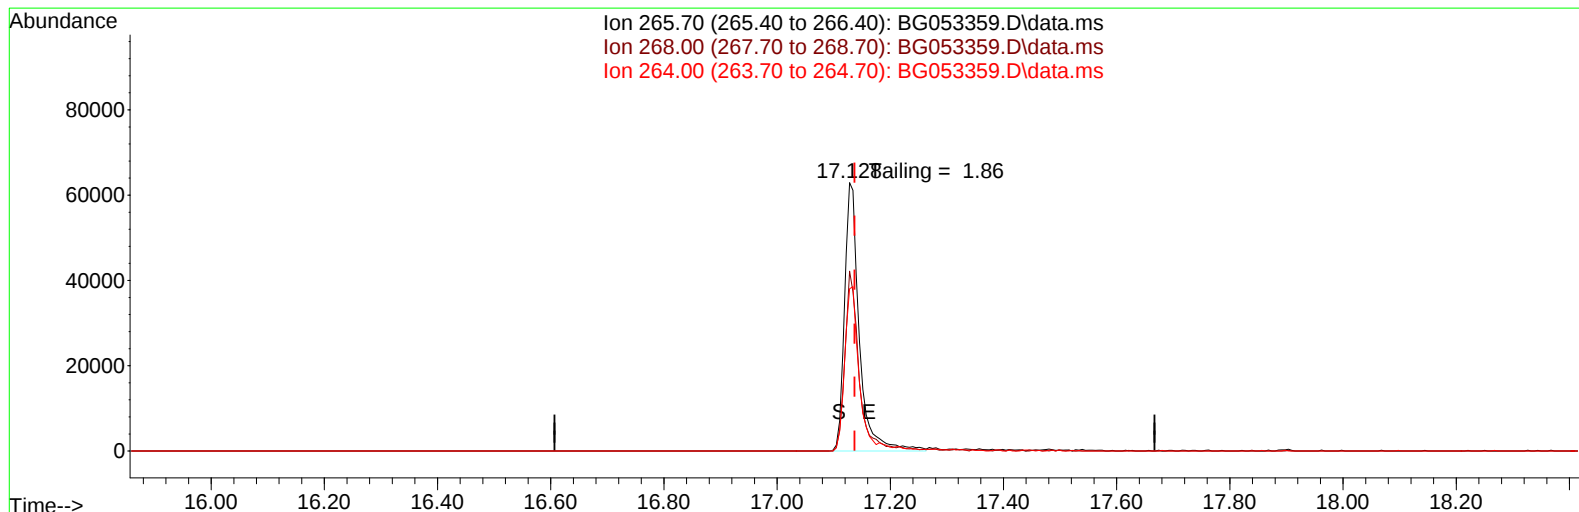

TIC: BG053359.D\data.ms

(70) Pentachlorophenol (C)

17.128min (-0.009) 28292.53 ng




response 114578

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	67.00
264.00	56.60	60.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042822\
Data File : BG053359.D
Acq On : 28 Apr 2022 9:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 29 06:13:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 01:13:30 2022
Response via : Initial Calibration

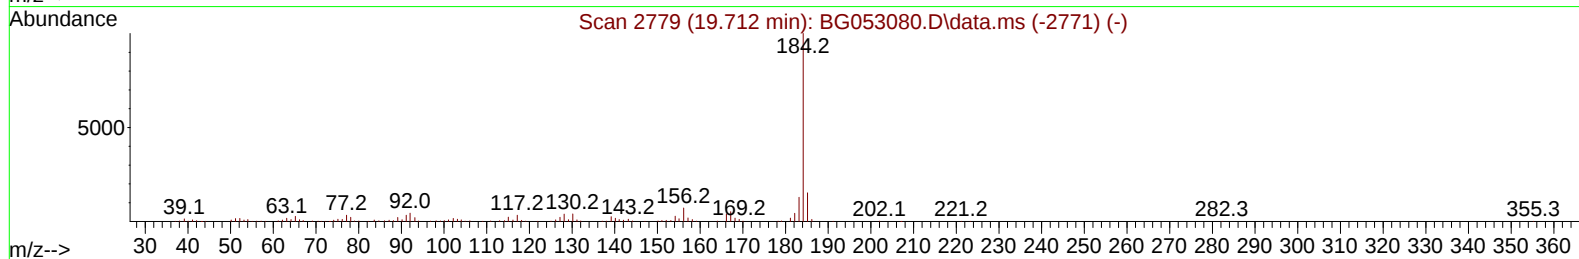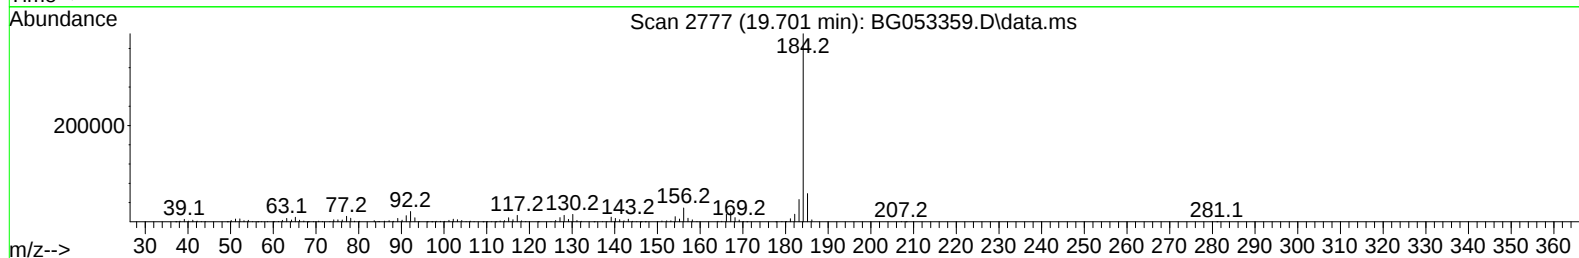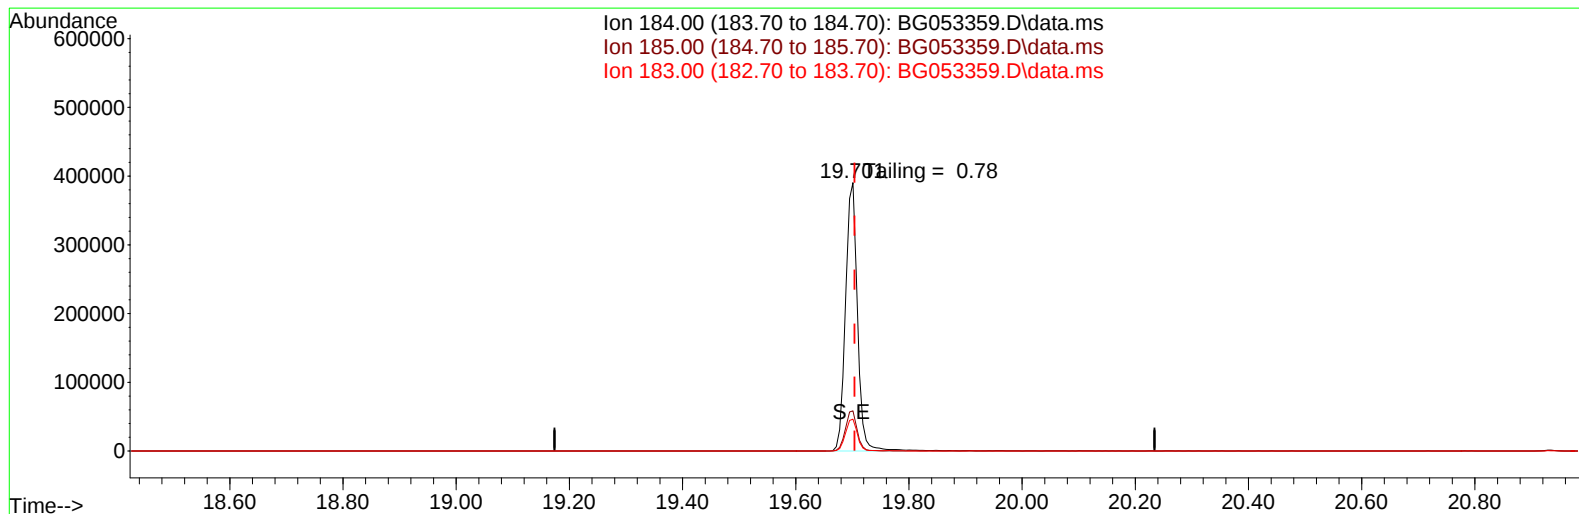

TIC: BG053359.D\data.ms

(77) Benzidine

19.701min (-0.003) 365515.66 ng

response 573581

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.97
183.00	11.80	11.89
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/28/2022	BNA_G	BG053359.D
Compound Name	Response	Retention Time
DDT	336766	20.93
DDD	1376	20.49
DDE	54	19.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1430	338196	0.42

Instrument :
BNA_G
ClientSampleId :
DFTPP