


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG042920\
 Data File : BG045199.D
 Acq On : 29 Apr 2020 11:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 29 12:24:27 2020

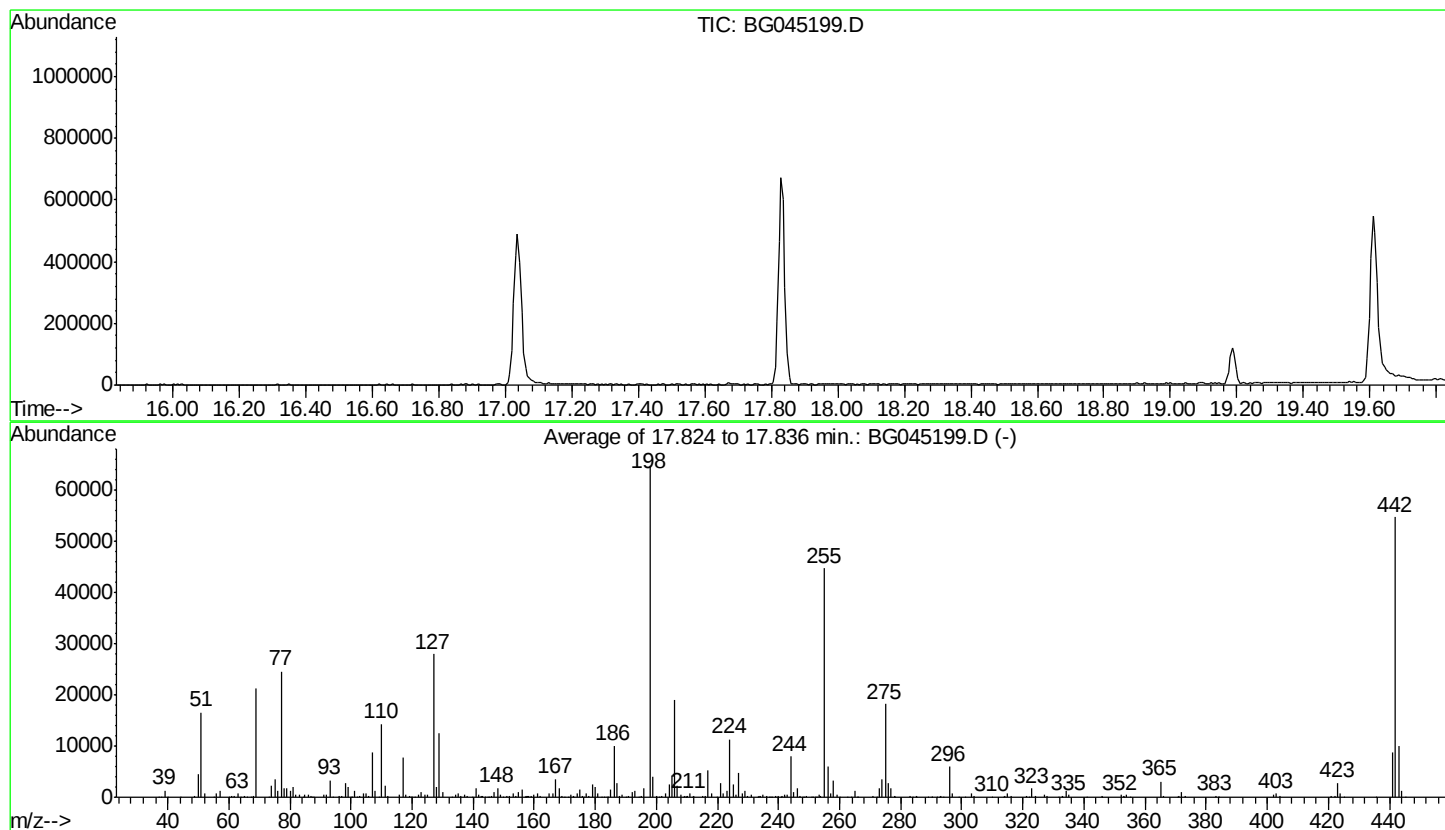

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.6	16607	PASS
68	69	0.00	2	1.6	336	PASS
69	198	0.00	100	32.8	21280	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.1	27970	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	64861	PASS
199	198	5	9	6.1	3950	PASS
275	198	10	60	28.0	18185	PASS
365	198	1	100	4.8	3101	PASS
441	198	0.01	100	13.6	8838	PASS
442	198	50	100	84.4	54749	PASS
443	442	15	24	18.4	10089	PASS