

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG050120\
 Data File : BG045226.D
 Acq On : 1 May 2020 21:38
 Operator : CG/JU
 Sample : L2452-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 209

Quant Time: May 02 05:26:42 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 01 11:17:49 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.99	152	67315	20.00	ng	0.00
21) Naphthalene-d8	10.80	136	247881	20.00	ng	0.00
39) Acenaphthene-d10	14.63	164	184020	20.00	ng	0.00
64) Phenanthrene-d10	17.38	188	467727	20.00	ng	0.00
76) Chrysene-d12	21.64	240	482141	20.00	ng	0.00
87) Perylene-d12	24.82	264	505636	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	495594	121.55	ng	0.00
7) Phenol-d6	7.16	99	613180	101.22	ng	0.00
23) Nitrobenzene-d5	9.15	82	521890	96.07	ng	0.00
42) 2,4,6-Tribromophenol	16.12	330	417402	146.82	ng	0.00
45) 2-Fluorobiphenyl	13.25	172	1221142	97.30	ng	0.00
79) Terphenyl-d14	20.00	244	2239994	101.26	ng	0.00
Target Compounds						
50) Dimethylphthalate	14.08	163	80329	5.361	ng	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG050120\
Data File : BG045226.D
Acq On : 1 May 2020 21:38
Operator : CG/JU
Sample : L2452-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
209

Quant Time: May 02 05:26:42 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 01 11:17:49 2020
Response via : Initial Calibration

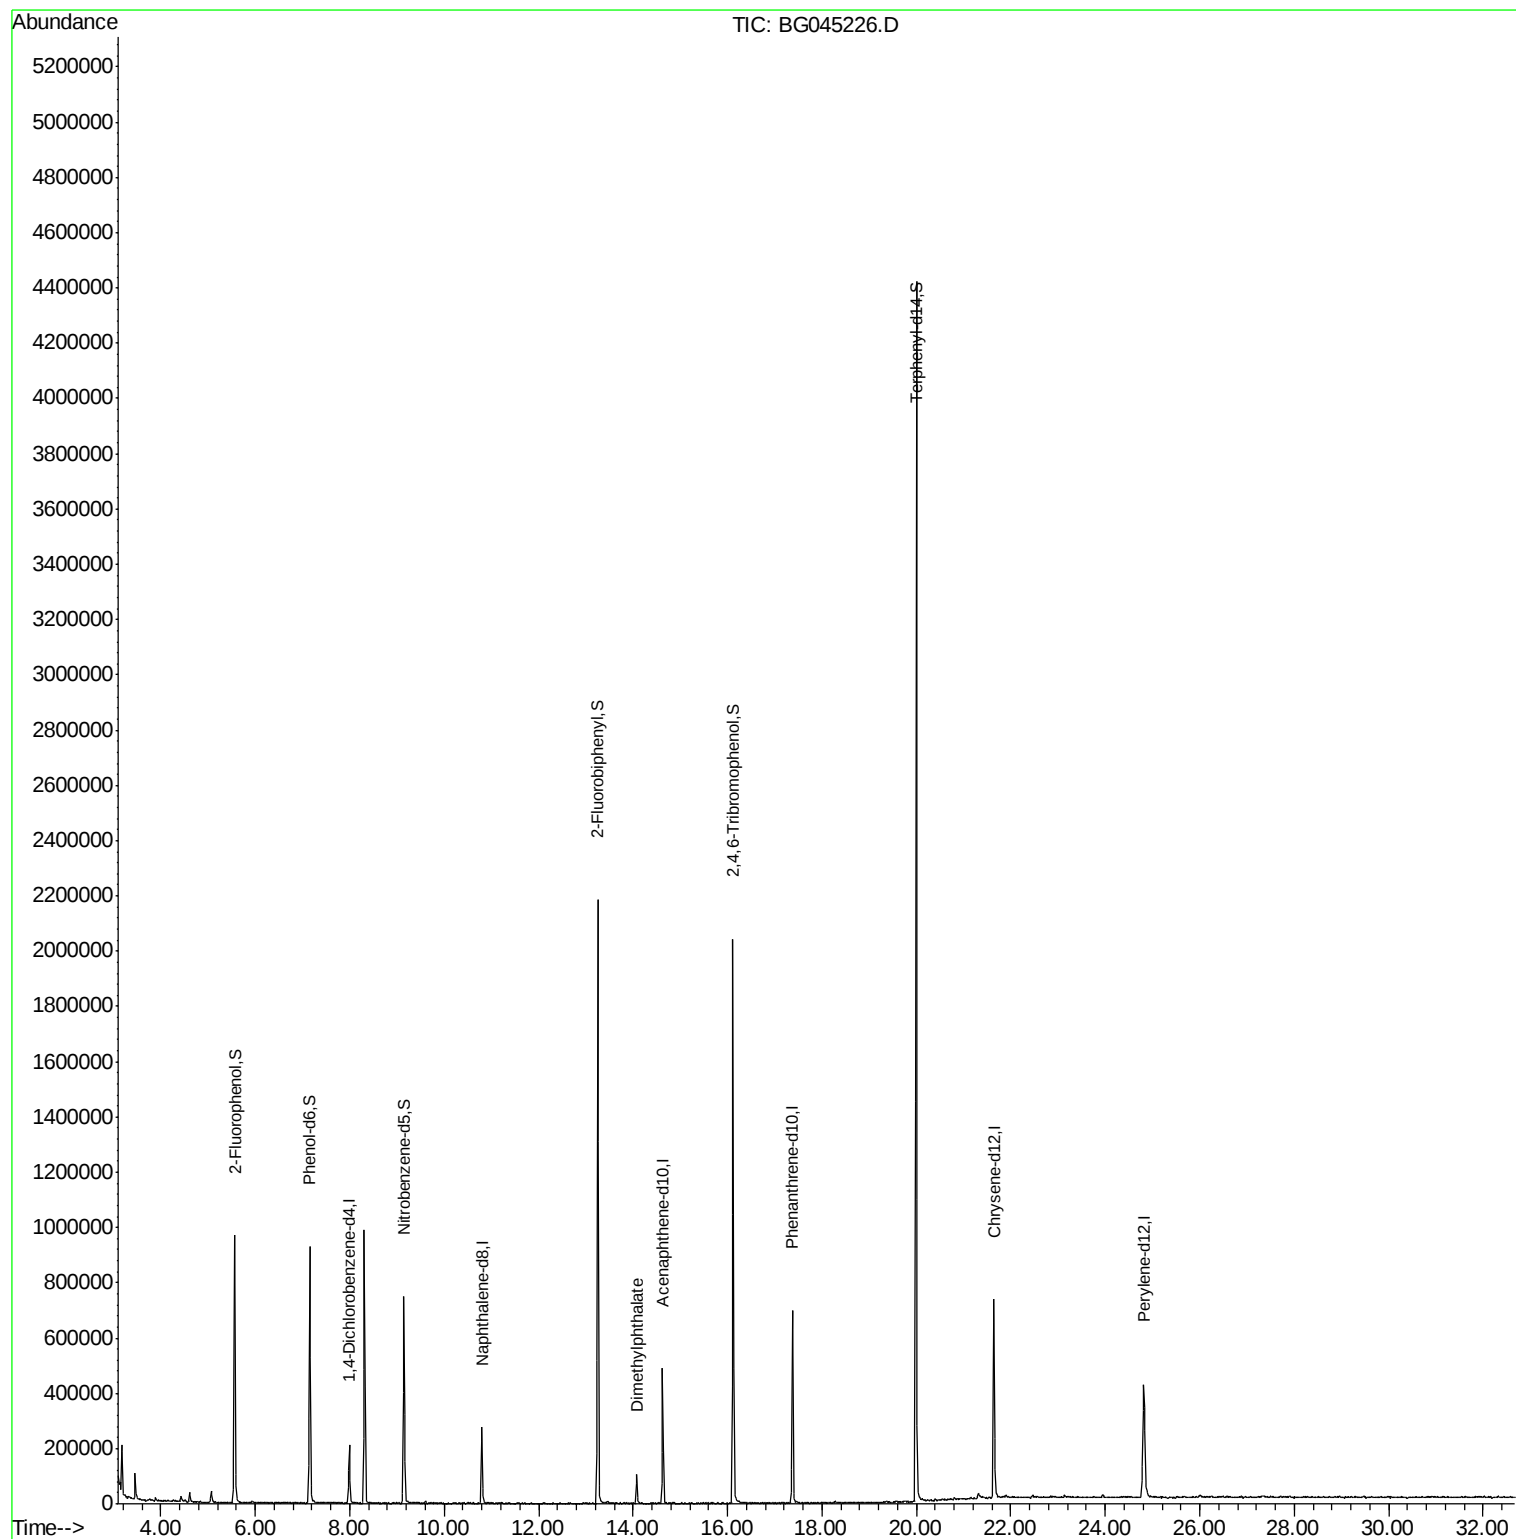




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.99 min Scan# 834
Delta R.T. 0.00 min
Lab File: BG045226.D
Acq: 1 May 2020 21:38

Instrument :
BNA_G
ClientSampleId :
209

Tot Ion	Ratio	Lower	Upper
152	100		
150	145.3	123.6	185.4
115	58.6	49.1	73.7

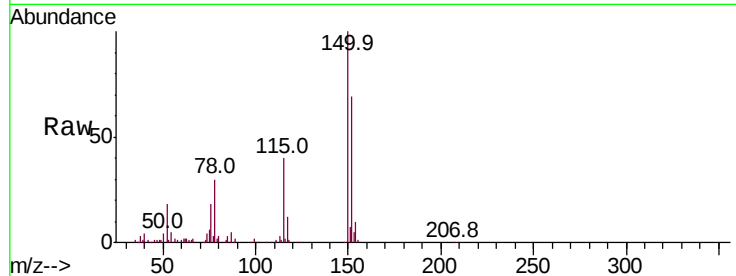


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

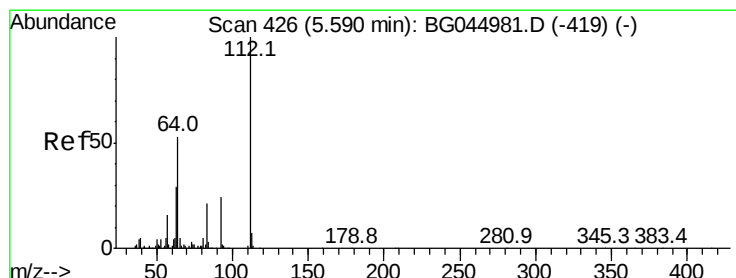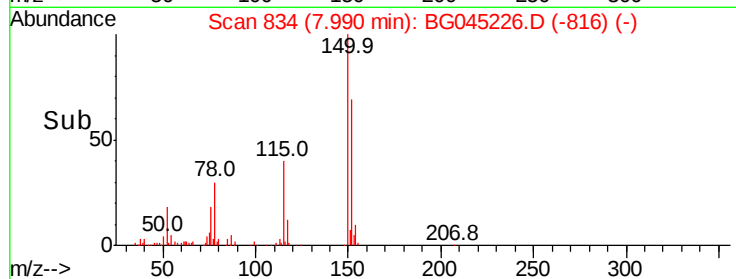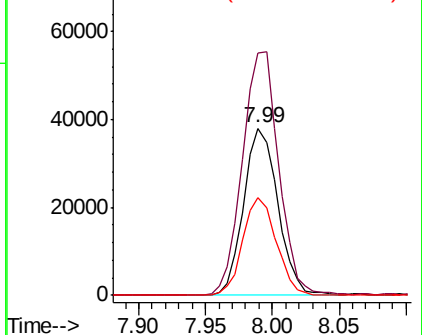



#5


2-Fluorophenol
Concen: 121.548 ng
RT: 5.56 min Scan# 421
Delta R.T. 0.00 min
Lab File: BG045226.D
Acq: 1 May 2020 21:38

Tgt Ion	Ratio	Lower	Upper
112	100		
64	56.5	42.4	63.6
63	32.3	23.1	34.7

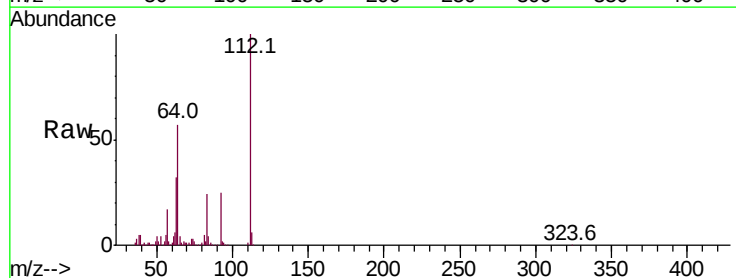

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

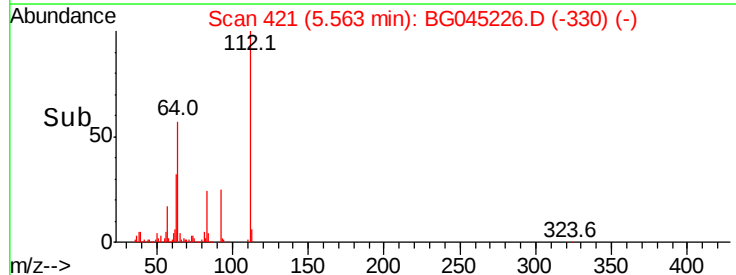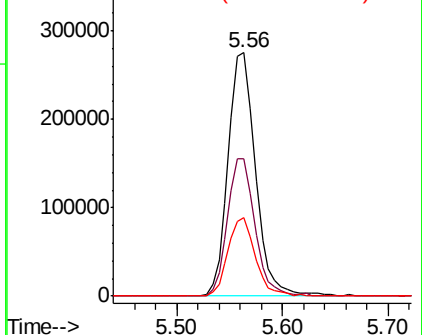

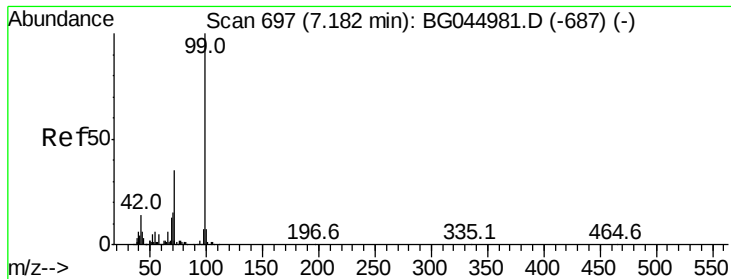

#7

Phenol-d6

Concen: 101.219 ng

RT: 7.16 min Scan# 692

Delta R.T. -0.00 min

Lab File: BG045226.D

Acq: 1 May 2020 21:38

Instrument :

BNA_G

ClientSampleId :

209


Tot Ion: 99 Resp: 613180

Ion Ratio Lower Upper




99 100

42 14.5 11.3 16.9

71 38.4 28.3 42.5

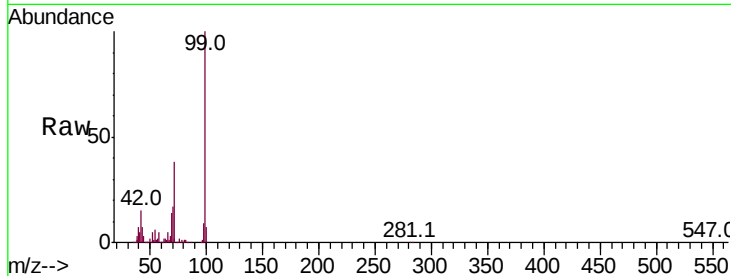

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

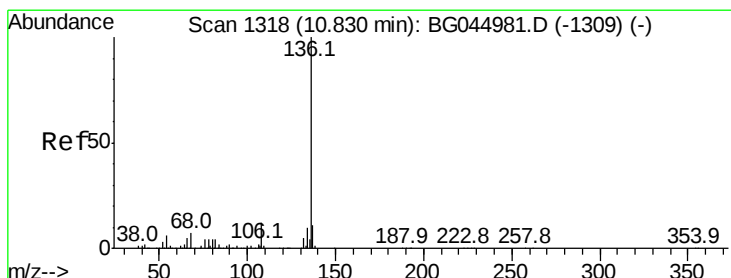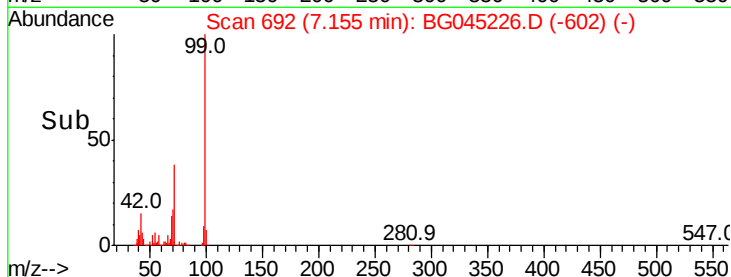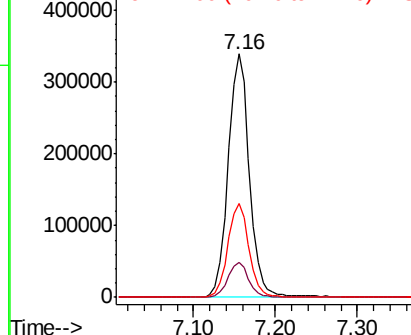

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.80 min Scan# 1312

Delta R.T. -0.00 min

Lab File: BG045226.D

Acq: 1 May 2020 21:38

Tgt Ion: 136 Resp: 247881


Ion Ratio Lower Upper

136 100



137 12.7 8.6 13.0


54 6.5 4.8 7.2

68 6.2 5.2 7.8

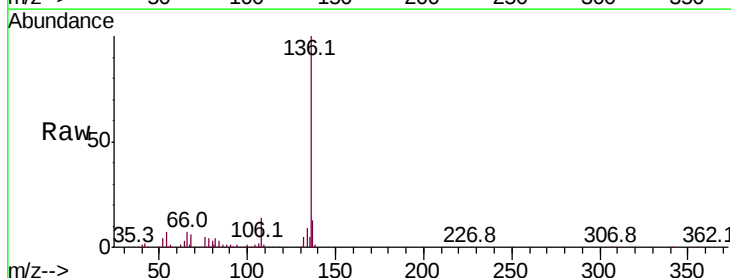

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



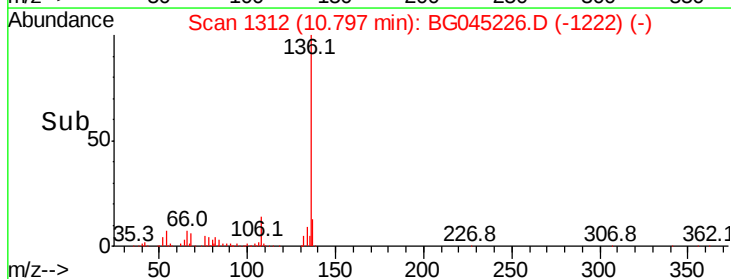
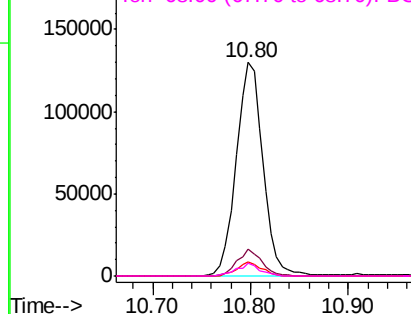


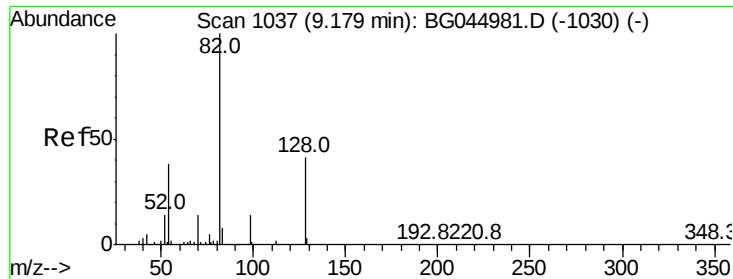

#23
Nitrobenzene-d5
Concen: 96.067 ng
RT: 9.15 min Scan# 1031
Delta R.T. -0.00 min
Lab File: BG045226.D
Acq: 1 May 2020 21:38




Instrument :
BNA_G
ClientSampleId :
209


Tot Ion	Ratio	Lower	Upper
82	100		
128	41.9	33.0	49.4
54	39.1	30.4	45.6

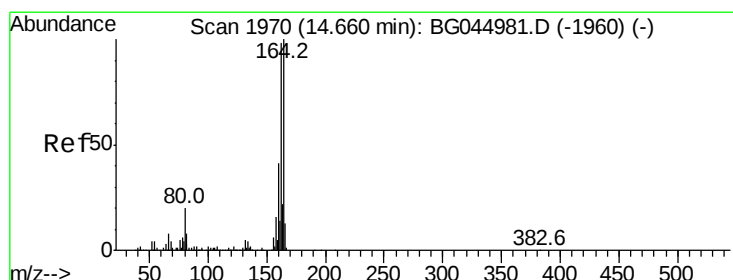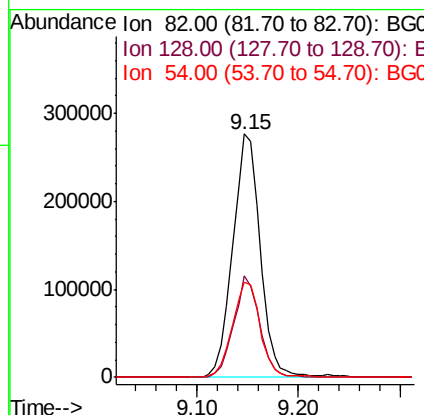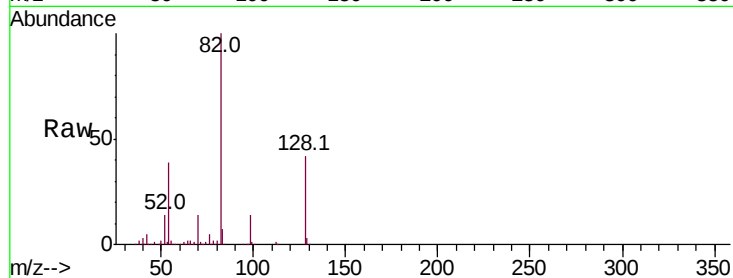

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.63 min Scan# 1964
Delta R.T. -0.01 min
Lab File: BG045226.D
Acq: 1 May 2020 21:38

Tgt Ion	Ratio	Lower	Upper
164	100		
162	98.7	78.7	118.1
160	45.3	32.8	49.2

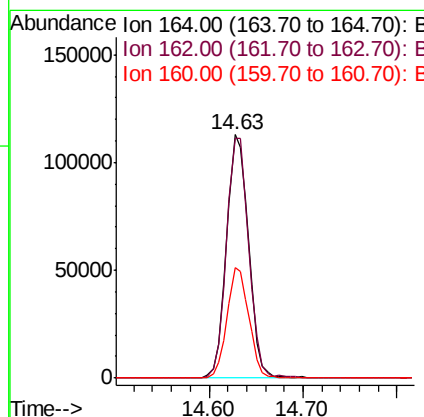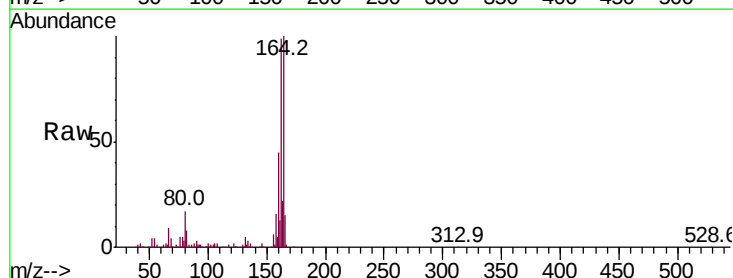







#42
 2,4,6-Tribromophenol
 Concen: 146.824 ng
 RT: 16.12 min Scan# 2218
 Delta R.T. -0.00 min
 Lab File: BG045226.D
 Acq: 1 May 2020 21:38

Instrument :
 BNA_G
 ClientSampleId :
 209

Tot Ion:330 Resp: 417402




Ion	Ratio	Lower	Upper
330	100		
332	97.8	79.1	118.7
141	35.9	27.1	40.7

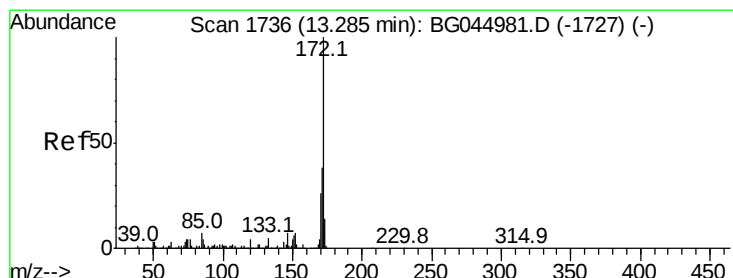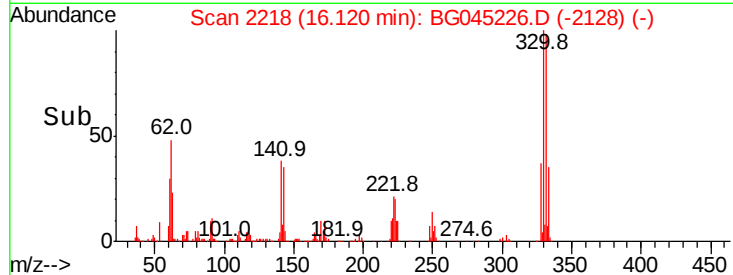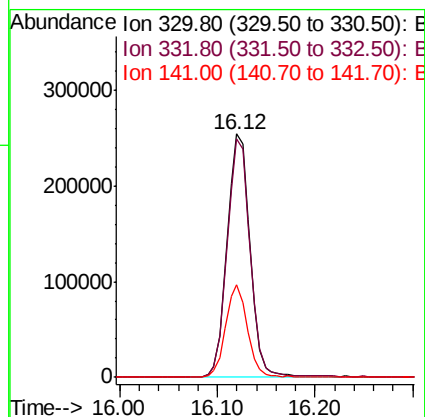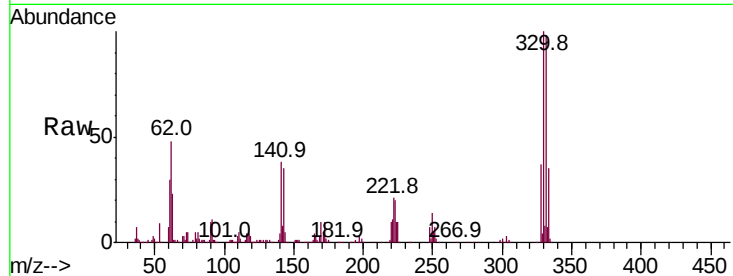


#45
 2-Fluorobiphenyl
 Concen: 97.304 ng
 RT: 13.25 min Scan# 1730
 Delta R.T. -0.00 min
 Lab File: BG045226.D
 Acq: 1 May 2020 21:38

Tgt Ion:172 Resp: 1221142

Ion	Ratio	Lower	Upper
172	100		
171	36.3	30.6	46.0
170	24.9	20.5	30.7



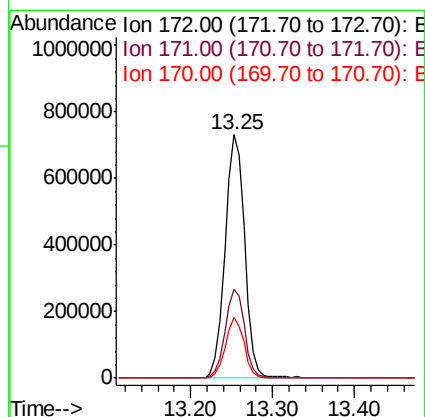
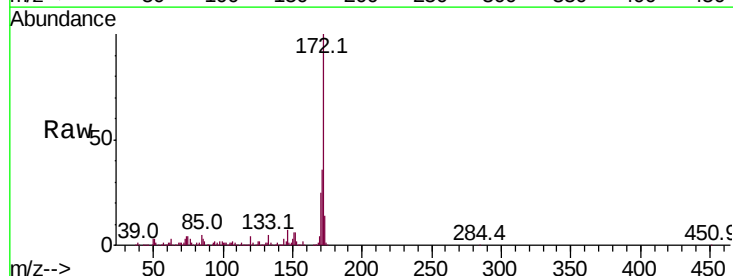




#50
Dimethylphthalate
Concen: 5.361 ng
RT: 14.08 min Scan# 1870
Delta R.T. -0.01 min
Lab File: BG045226.D
Acq: 1 May 2020 21:38




Instrument :
BNA_G
ClientSampleId :
209


Tot Ion	Ratio	Lower	Upper
163	100		
194	3.8	3.5	5.3
164	10.1	8.2	12.4

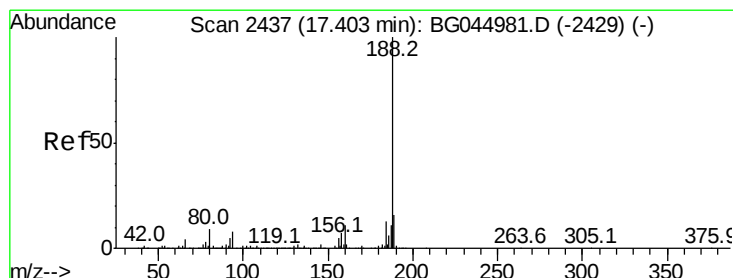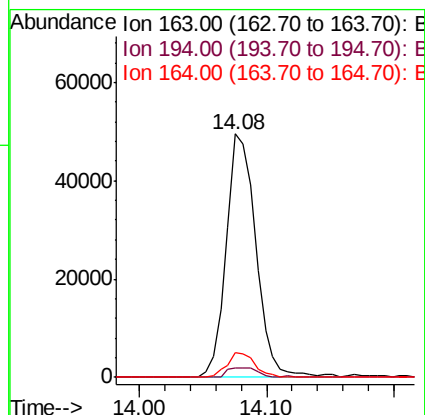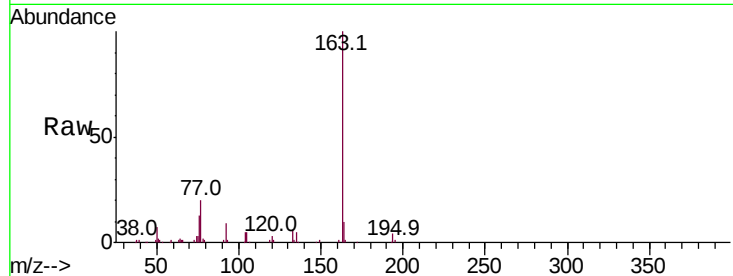

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.38 min Scan# 2432
Delta R.T. -0.00 min
Lab File: BG045226.D
Acq: 1 May 2020 21:38

Tgt Ion	Ratio	Lower	Upper
188	100		
94	6.8	6.2	9.4
80	8.1	7.0	10.6

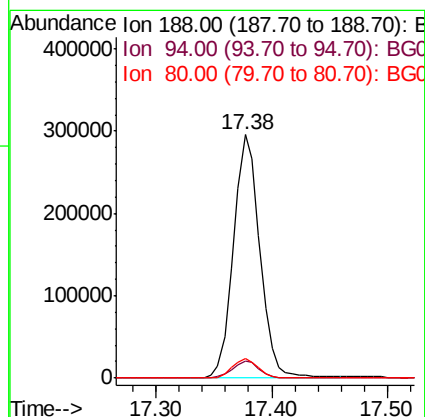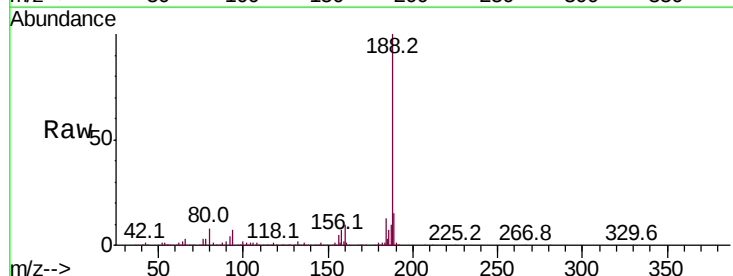



#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.64 min Scan# 3158

Delta R.T. -0.01 min

Lab File: BG045226.D

Acq: 1 May 2020 21:38

Instrument :

BNA_G

ClientSampleId :

209


Tot Ion:240 Resp: 482141

Ion Ratio Lower Upper

240 100

120 6.5 6.6 10.0#




236 26.0 22.2 33.2

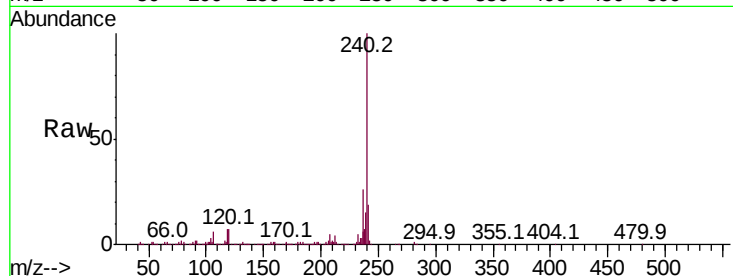

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

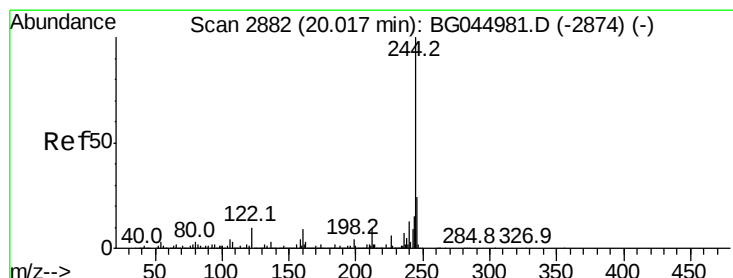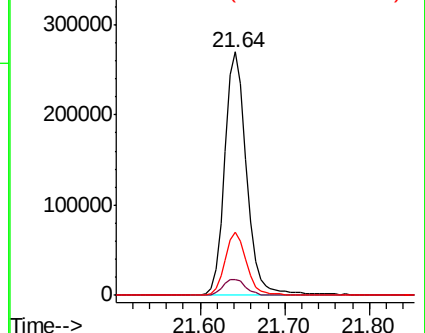

#79

Terphenyl-d14

Concen: 101.261 ng

RT: 20.00 min Scan# 2878

Delta R.T. 0.00 min

Lab File: BG045226.D

Acq: 1 May 2020 21:38


Tgt Ion:244 Resp: 2239994

Ion Ratio Lower Upper

244 100

212 10.0 7.9 11.9



122 8.7 7.7 11.5

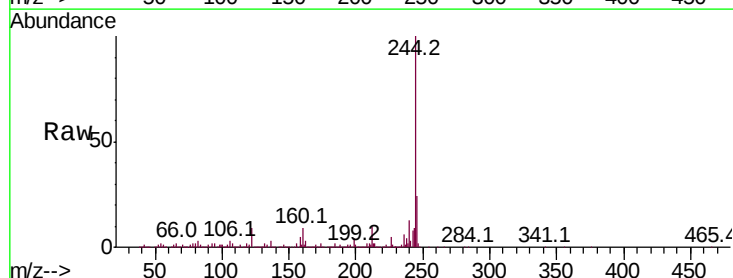


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

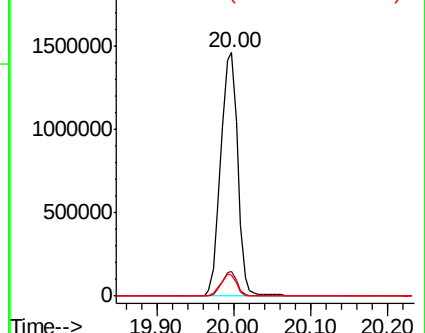



#87
Pervlene-d12
Concen: 20.000 ng
RT: 24.82 min Scan# 3699
Delta R.T. -0.01 min
Lab File: BG045226.D
Acq: 1 May 2020 21:38

Instrument :
BNA_G
ClientSampleId :
209

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.9	19.2	28.8
265	20.7	19.0	28.4

