


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG050120\
 Data File : BG045215.D
 Acq On : 1 May 2020 12:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 01 11:17:49 2020

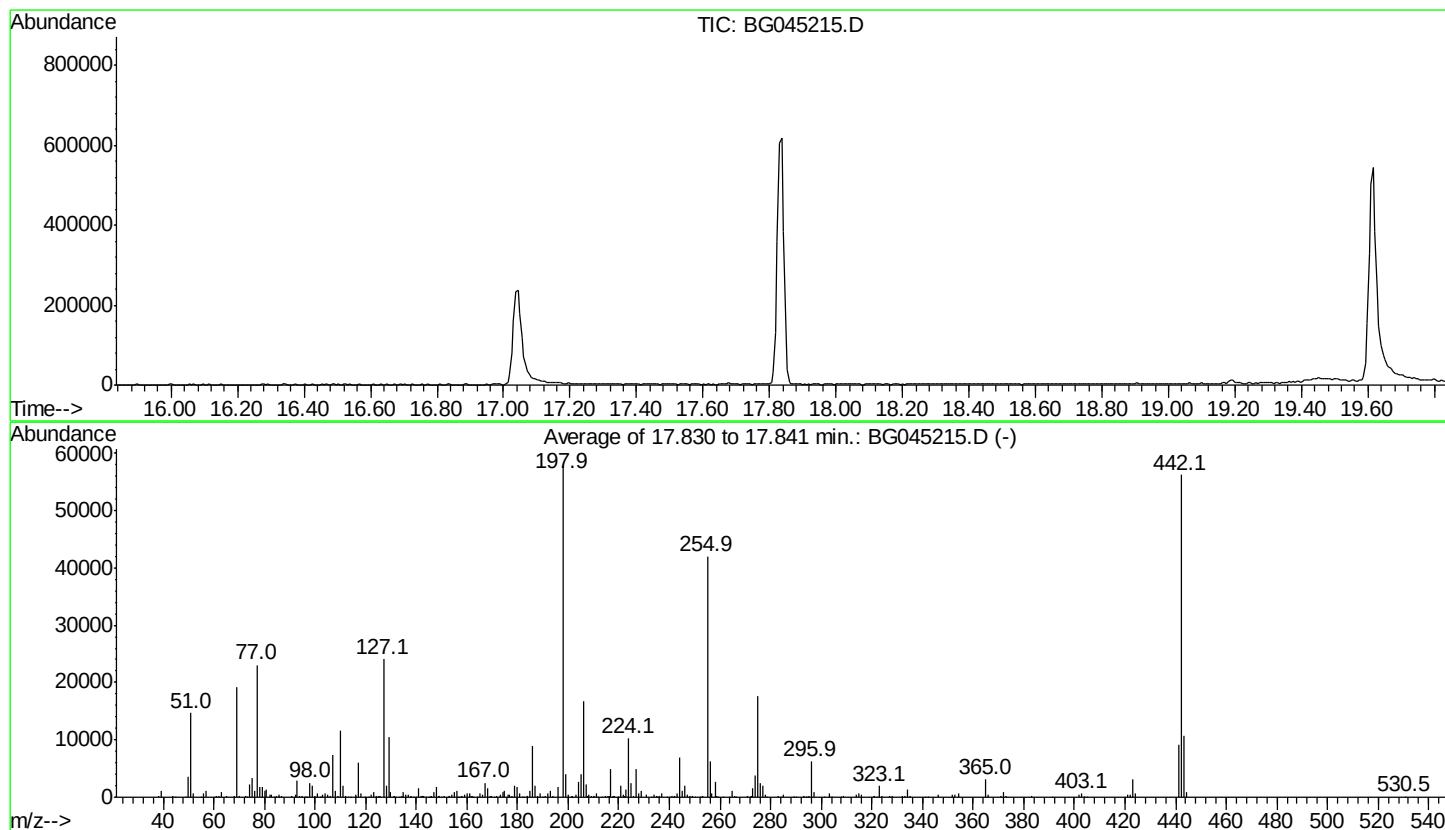

AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2502

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.3	14638	PASS
68	69	0.00	2	1.7	321	PASS
69	198	0.00	100	33.2	19170	PASS
70	69	0.00	2	0.7	133	PASS
127	198	10	80	41.6	24064	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	57816	PASS
199	198	5	9	7.1	4091	PASS
275	198	10	60	30.5	17619	PASS
365	198	1	100	5.4	3112	PASS
441	198	0.01	100	15.7	9055	PASS
442	198	50	100	97.2	56221	PASS
443	442	15	24	19.2	10793	PASS