




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
Data File : BG057247.D
Acq On : 1 May 2023 11:20
Operator : CG/JU
Sample : PB152344BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK344

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/02/2023
Supervised By :Jagrut Upadhyay 05/02/2023

Quant Time: May 01 22:28:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 01 12:45:38 2023
Response via : Initial Calibration

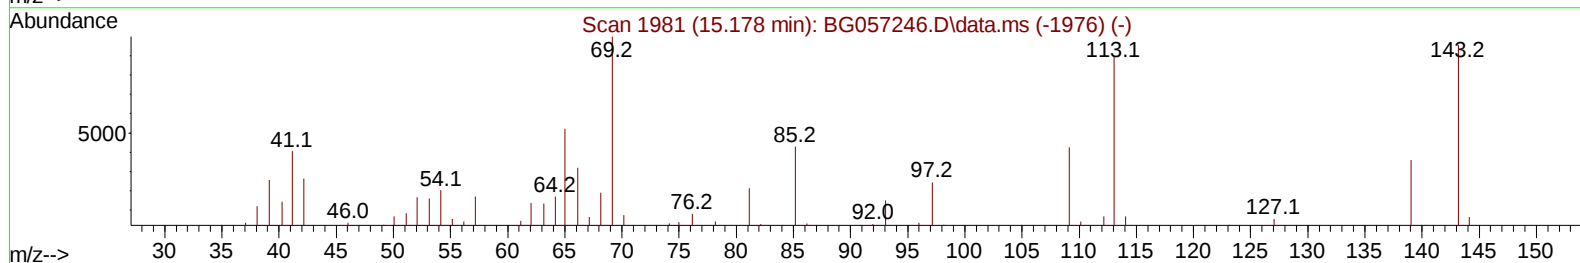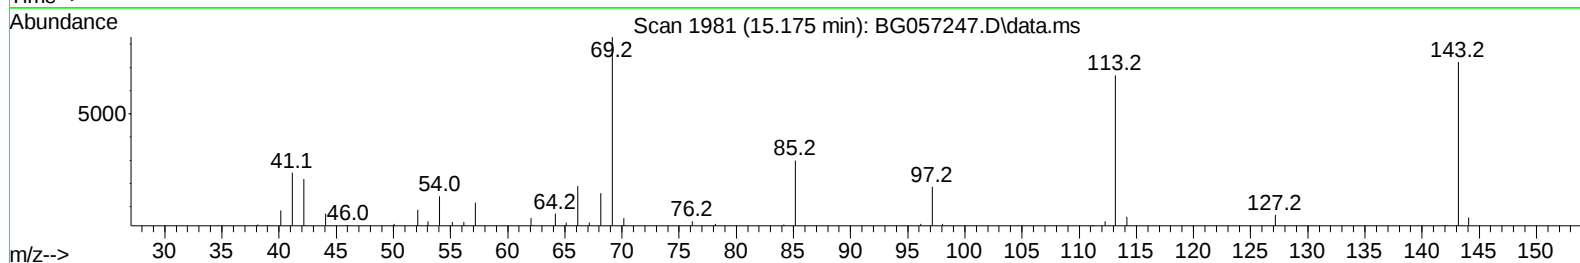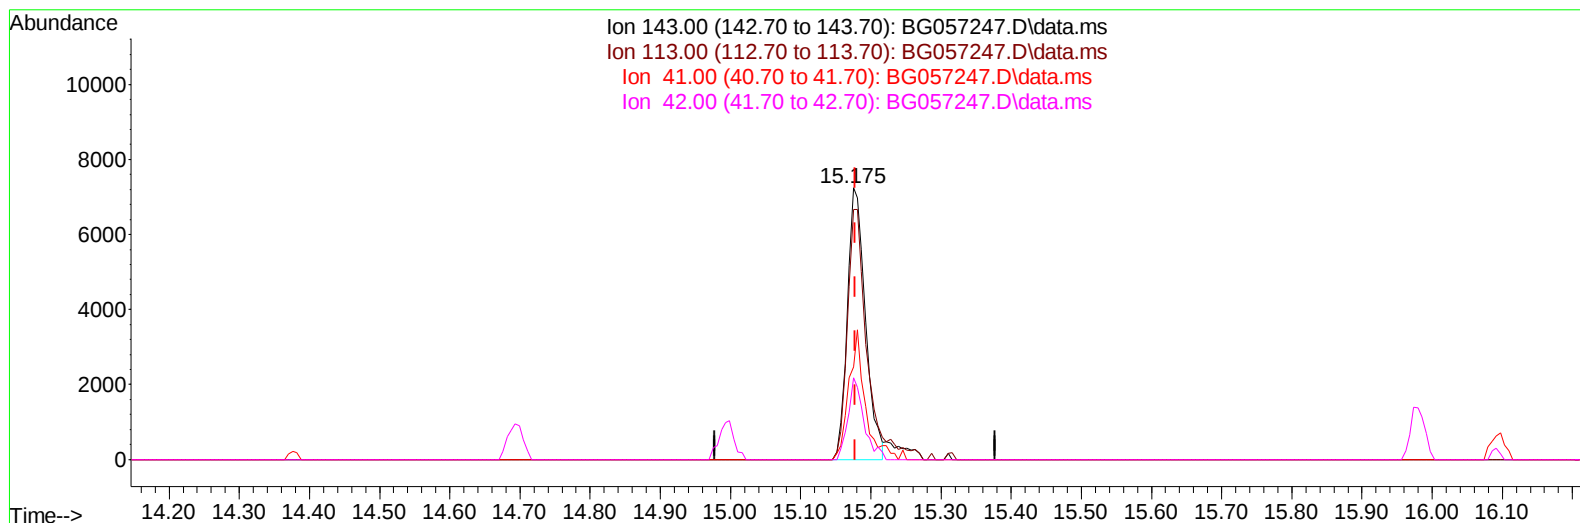

TIC: BG057247.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.175min (-0.003) 23.21 ng/u1

response 13032

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	95.60	92.03
41.00	44.40	34.13#
42.00	28.40	30.15




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
Data File : BG057247.D
Acq On : 1 May 2023 11:20
Operator : CG/JU
Sample : PB152344BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK344

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/02/2023
Supervised By :Jagrut Upadhyay 05/02/2023

Quant Time: May 01 22:28:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 01 12:45:38 2023
Response via : Initial Calibration

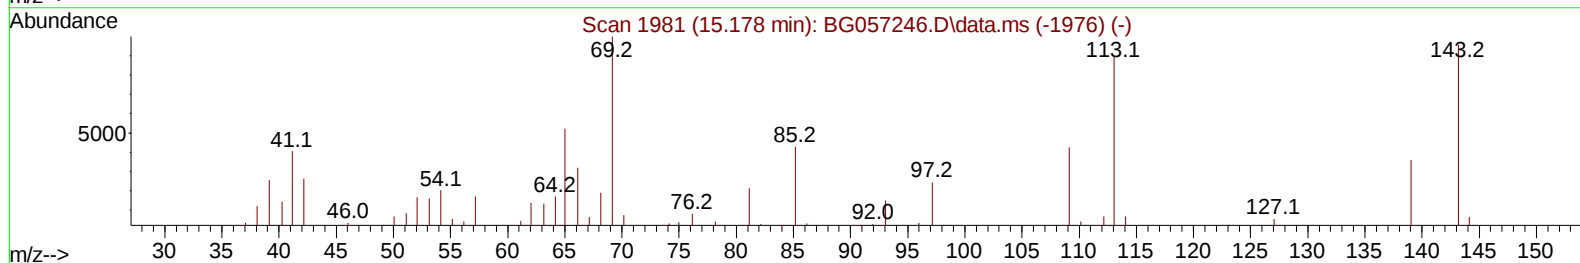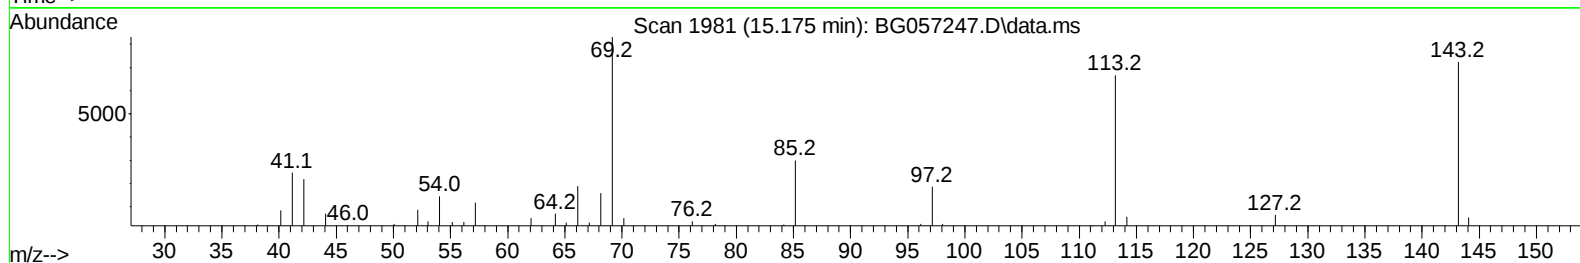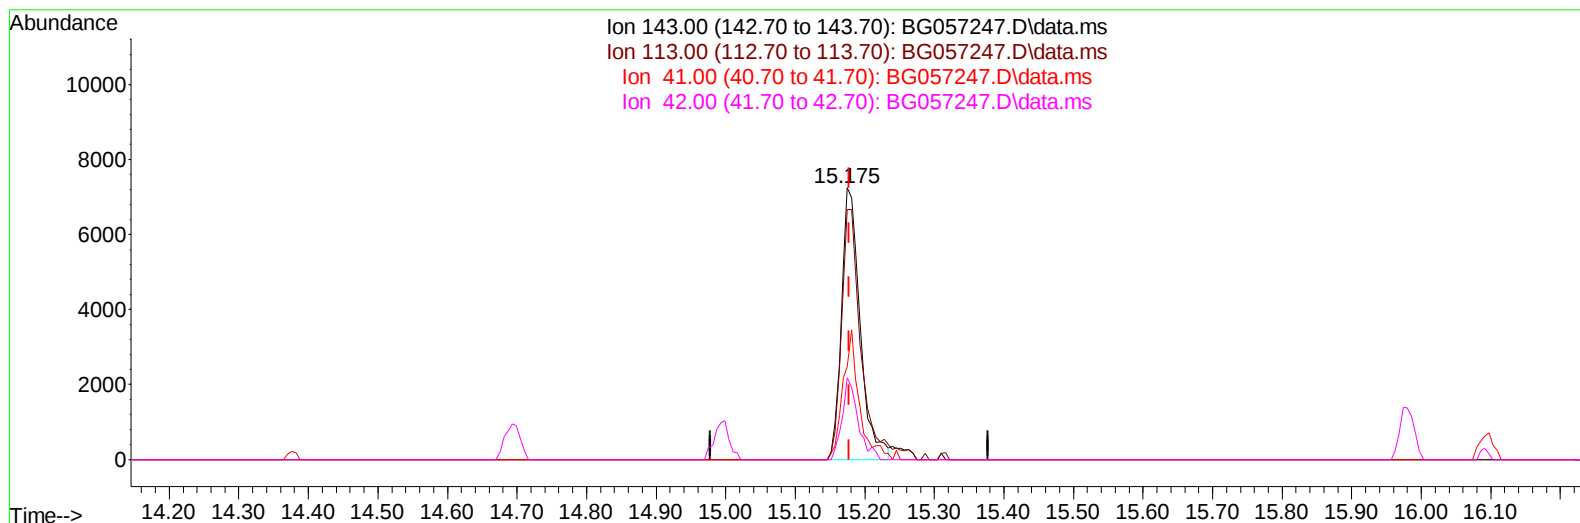

TIC: BG057247.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.175min (-0.003) 23.97 ng/ul m

response 13460

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	95.60	92.03
41.00	44.40	34.13#
42.00	28.40	30.15

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
 Data File : BG057247.D
 Acq On : 1 May 2023 11:20
 Operator : CG/JU
 Sample : PB152344BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK344

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/02/2023
 Supervised By :Jagrut Upadhyay 05/02/2023

Quant Time: May 01 22:36:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 01 12:45:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.378	152	14138	20.000	ng/ul	0.00
20) Naphthalene-d8	11.222	136	60475	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.993	164	48692	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.736	188	119544	20.000	ng/ul	0.00
79) Chrysene-d12	22.048	240	109107	20.000	ng/ul	0.00
88) Perylene-d12	25.567	264	112436	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.655	96	1610	5.011	ng/uL	0.00
4) Pyridine-d5	4.096	84	21606	21.331	ng/ul	0.00
7) Phenol-d5	7.515	99	32771	24.510	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.685	67	20341	25.866	ng/ul	0.00
11) 2-Chlorophenol-d4	7.902	132	23791	27.001	ng/ul	0.00
15) 4-Methylphenol-d8	9.077	113	26103	25.687	ng/ul	0.00
21) Nitrobenzene-d5	9.559	128	13333	27.685	ng/ul	0.00
24) 2-Nitrophenol-d4	10.288	143	15666	27.873	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.834	165	28733	26.498	ng/ul	0.00
31) 4-Chloroaniline-d4	11.345	131	34363	23.910	ng/ul	0.00
46) Dimethylphthalate-d6	14.382	166	106003	27.475	ng/ul	0.00
49) Acenaphthylene-d8	14.693	160	120829	27.864	ng/ul	0.00
54) 4-Nitrophenol-d4	15.175	143	13460m	23.967	ng/ul	0.00
60) Fluorene-d10	15.980	176	95483	26.566	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.091	200	16298	23.011	ng/ul	0.00
73) Anthracene-d10	17.836	188	160677	29.446	ng/ul	0.00
81) Pyrene-d10	20.098	212	187645	28.975	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.326	264	169334	29.561	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
Data File : BG057247.D
Acq On : 1 May 2023 11:20
Operator : CG/JU
Sample : PB152344BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK344

Manual IntegrationsAPPROVED

Quant Time: May 01 22:36:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 01 12:45:38 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 05/02/2023
Supervised By :Jagrut Upadhyay 05/02/2023

