




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
Data File : BG057271.D
Acq On : 2 May 2023 9:36
Operator : CG/JU
Sample : 02418-08
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW8Z4

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/03/2023
Supervised By :Jagrut Upadhyay 05/03/2023

Quant Time: May 03 01:04:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 01 12:45:38 2023
Response via : Initial Calibration

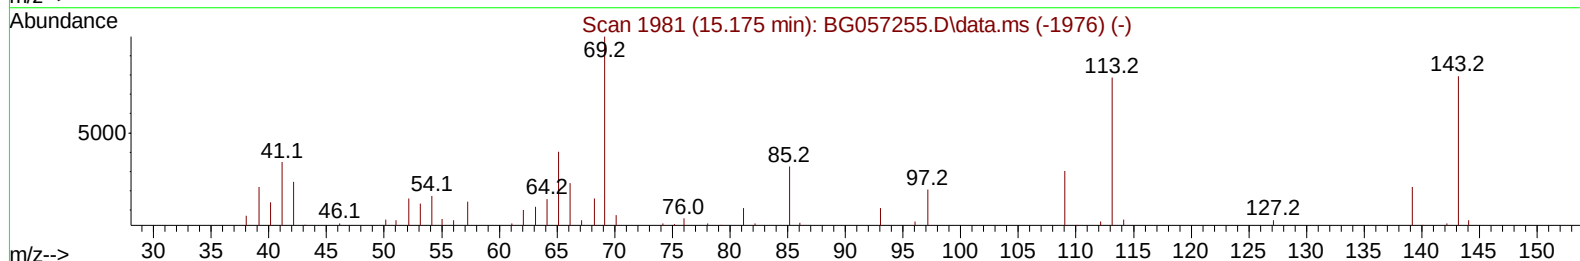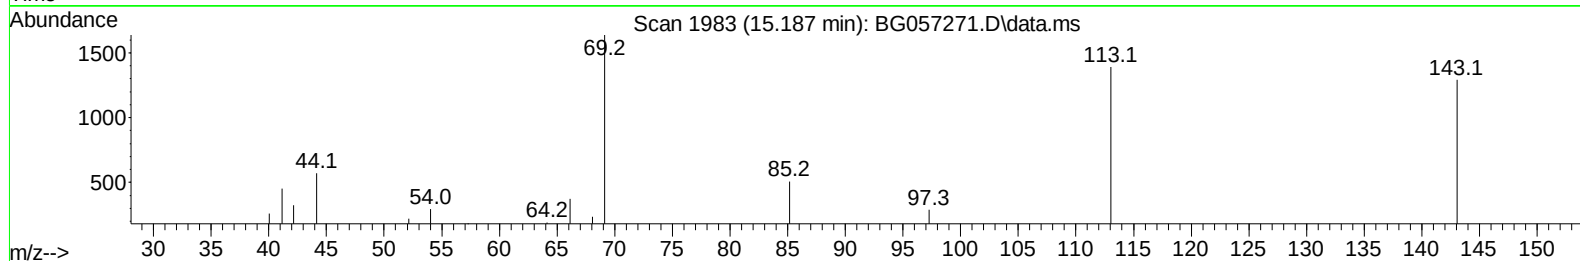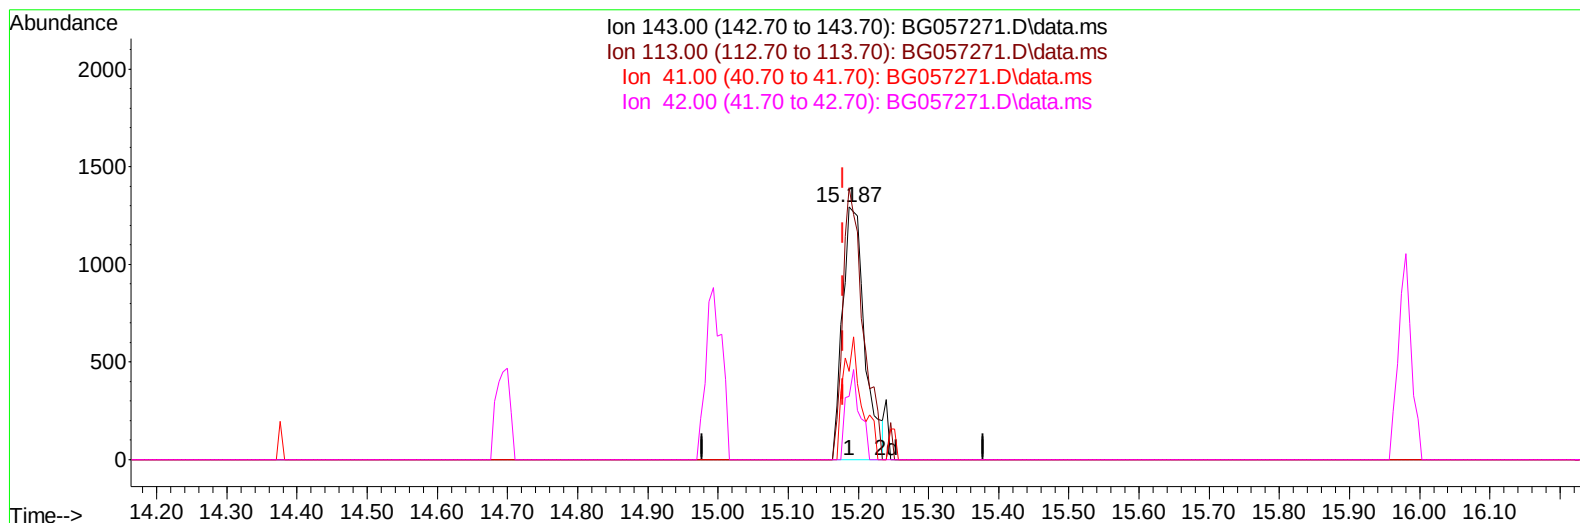

TIC: BG057271.D\data.ms

(54) 4-Nitrophenol-d4 (S)**15.187min (+ 0.009) 4.89 ng/ul****response 2833**

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	95.60	107.58
41.00	44.40	34.88#
42.00	28.40	25.06




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
Data File : BG057271.D
Acq On : 2 May 2023 9:36
Operator : CG/JU
Sample : 02418-08
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW8Z4

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/03/2023
Supervised By :Jagrut Upadhyay 05/03/2023

Quant Time: May 03 01:04:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 01 12:45:38 2023
Response via : Initial Calibration

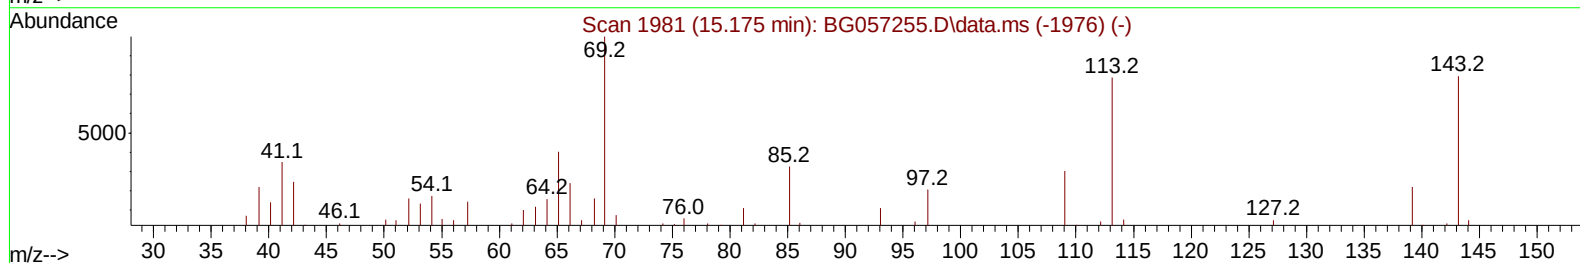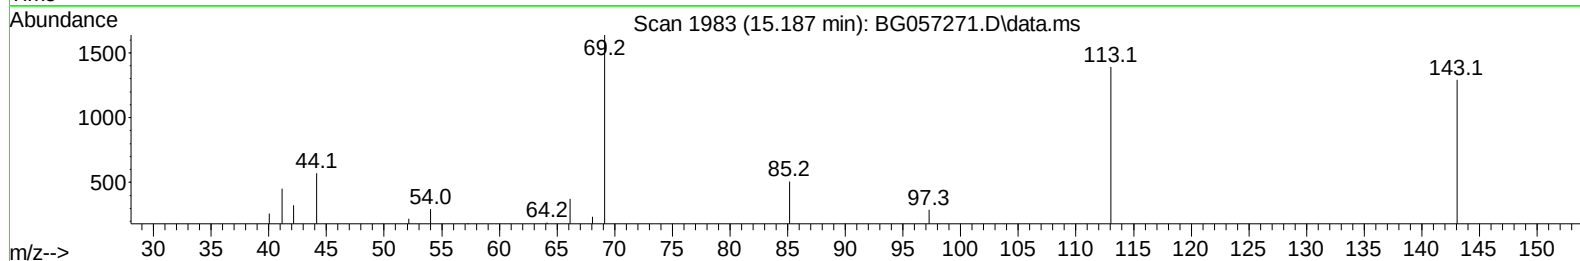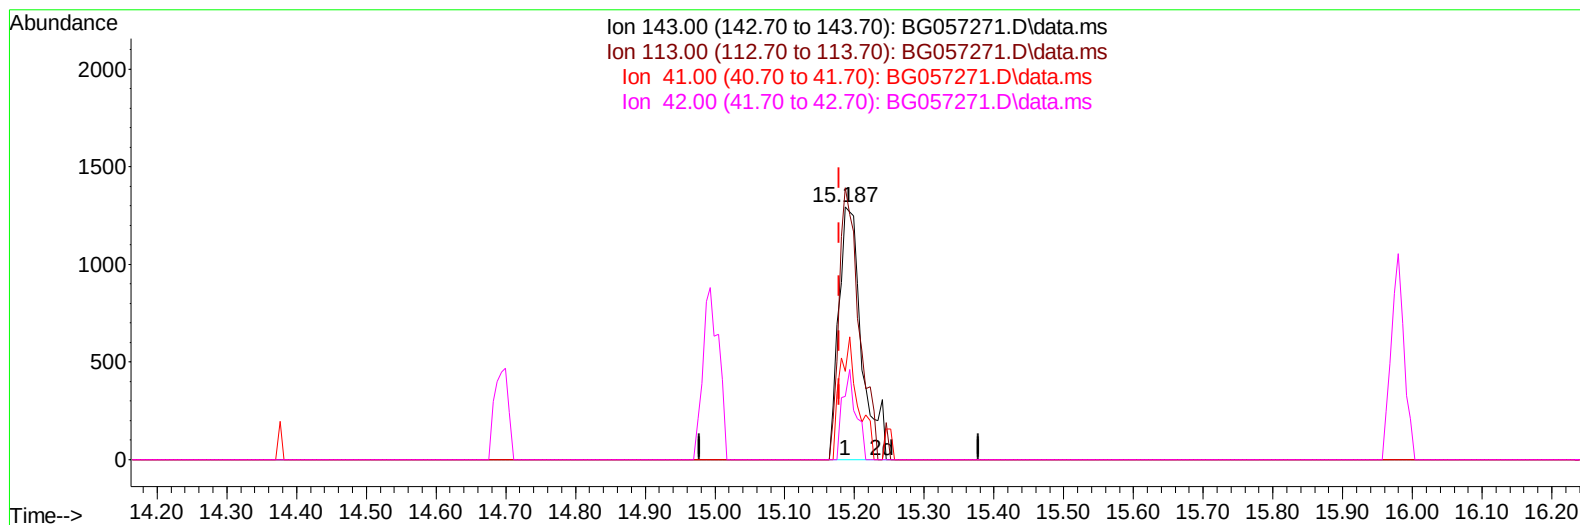

TIC: BG057271.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.187min (+ 0.009) 5.08 ng/ul m

response 2942

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	95.60	107.58
41.00	44.40	34.88#
42.00	28.40	25.06

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
 Data File : BG057271.D
 Acq On : 2 May 2023 9:36
 Operator : CG/JU
 Sample : 02418-08
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW8Z4

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/03/2023
 Supervised By :Jagrut Upadhyay 05/03/2023

Quant Time: May 03 01:19:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 01 12:45:38 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.378	152		15952	20.000	ng/ul	0.00
20) Naphthalene-d8	11.222	136		66310	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.993	164		50236	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.736	188		114211	20.000	ng/ul	0.00
79) Chrysene-d12	22.048	240		97822	20.000	ng/ul	0.00
88) Perylene-d12	25.567	264		102008	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.661	96		340	0.938	ng/uL	0.00
4) Pyridine-d5	0.000	84		0d	0.000	ng/ul	
7) Phenol-d5	7.521	99		17259	11.440	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.685	67		12348	13.916	ng/ul	0.00
11) 2-Chlorophenol-d4	7.909	132		13949	14.031	ng/ul	0.00
15) 4-Methylphenol-d8	9.078	113		15143	13.207	ng/ul	0.00
21) Nitrobenzene-d5	9.553	128		8572	16.233	ng/ul	0.00
24) 2-Nitrophenol-d4	10.288	143		8534	13.848	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.834	165		15854	13.334	ng/ul	0.00
31) 4-Chloroaniline-d4	11.345	131		14268	9.054	ng/ul	0.00
46) Dimethylphthalate-d6	14.376	166		57508	14.447	ng/ul	0.00
49) Acenaphthylene-d8	14.693	160		66610	14.889	ng/ul	0.00
54) 4-Nitrophenol-d4	15.187	143		2942m	5.078	ng/ul	0.00
60) Fluorene-d10	15.980	176		56405	15.211	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.097	200		2261	3.341	ng/ul	0.00
73) Anthracene-d10	17.830	188		84120	16.136	ng/ul	0.00
81) Pyrene-d10	20.098	212		51781	8.918	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.326	264		36108	6.948	ng/ul	0.00
Target Compounds							
16) Acetophenone	9.207	105		3082	1.562	ng/ul	Qvalue 88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
Data File : BG057271.D
Acq On : 2 May 2023 9:36
Operator : CG/JU
Sample : 02418-08
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW8Z4

Manual IntegrationsAPPROVED

Quant Time: May 03 01:19:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 01 12:45:38 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 05/03/2023
Supervised By :Jagrut Upadhyay 05/03/2023

