

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
 Data File : BG057247.D
 Acq On : 1 May 2023 11:20
 Operator : CG/JU
 Sample : PB152344BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK344

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG057247.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.655	16	20	25	rVB2	3109	5005	1.13%	0.112%
2	3.902	60	62	64	rBV2	947	876	0.20%	0.020%
3	4.096	92	95	109	rVV	36312	61404	13.86%	1.379%
4	5.095	262	265	267	rBV	567	652	0.15%	0.015%
5	7.515	671	677	685	rBV2	55221	95470	21.55%	2.144%
6	7.685	700	706	715	rVV	42104	69297	15.64%	1.556%
7	7.903	737	743	752	rVB	51881	90315	20.39%	2.029%
8	8.378	818	824	835	rBV	49494	83383	18.82%	1.873%
9	9.077	936	943	951	rBV	68528	118812	26.82%	2.669%
10	9.559	1018	1025	1034	rVB	56746	102148	23.06%	2.294%
11	10.288	1141	1149	1157	rBV2	48621	85154	19.22%	1.913%
12	10.616	1203	1205	1208	rBV	508	707	0.16%	0.016%
13	10.834	1235	1242	1252	rBV	71205	126577	28.57%	2.843%
14	11.222	1301	1308	1315	rVV	69896	127164	28.70%	2.856%
15	11.345	1322	1329	1338	rBV	64596	117565	26.54%	2.641%
16	12.778	1570	1573	1576	rBV	819	1008	0.23%	0.023%
17	13.859	1754	1757	1760	rVB	1023	1226	0.28%	0.028%
18	14.382	1840	1846	1858	rVB	159388	223843	50.53%	5.028%
19	14.693	1892	1899	1906	rBV	173743	267725	60.43%	6.013%
20	14.993	1944	1950	1957	rBV	129751	204761	46.22%	4.599%
21	15.181	1976	1982	1999	rBV	48752	89559	20.22%	2.012%
22	15.980	2111	2118	2126	rVB	226144	337277	76.13%	7.575%
23	16.091	2132	2137	2146	rVV	56378	86160	19.45%	1.935%
24	16.973	2284	2287	2292	rBV	379	689	0.16%	0.015%
25	17.519	2378	2380	2383	rBV2	641	726	0.16%	0.016%
26	17.736	2409	2417	2424	rBV	182568	267207	60.31%	6.002%
27	17.836	2427	2434	2441	rVV2	244442	381163	86.04%	8.561%
28	18.782	2593	2595	2599	rBV2	535	650	0.15%	0.015%
29	18.817	2599	2601	2606	rBV2	480	908	0.20%	0.020%
30	19.217	2666	2669	2670	rVB	681	625	0.14%	0.014%
31	19.316	2685	2686	2689	rBV2	557	607	0.14%	0.014%
32	19.457	2705	2710	2712	rBV3	601	1175	0.27%	0.026%
33	19.475	2712	2713	2716	rVV	844	768	0.17%	0.017%
34	19.610	2734	2736	2739	rVB2	684	605	0.14%	0.014%
35	19.669	2739	2746	2751	rBV3	3306	5794	1.31%	0.130%
36	19.739	2751	2758	2762	rBV3	3221	5036	1.14%	0.113%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
 Data File : BG057247.D
 Acq On : 1 May 2023 11:20
 Operator : CG/JU
 Sample : PB152344BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK344

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

37	19.786	2763	2766	2769	rVB2	910	844	0.19%	0.019%
38	19.822	2769	2772	2773	rBV	600	747	0.17%	0.017%
39	19.951	2791	2794	2797	rBV3	1283	1748	0.39%	0.039%
40	20.098	2813	2819	2829	rVB	308436	443024	100.00%	9.951%
41	20.321	2855	2857	2861	rBV4	658	837	0.19%	0.019%
42	20.397	2868	2870	2873	rVB3	1035	1042	0.24%	0.023%
43	20.433	2873	2876	2877	rBV2	967	1034	0.23%	0.023%
44	20.503	2886	2888	2889	rBV2	1249	653	0.15%	0.015%
45	20.585	2900	2902	2904	rBV3	788	660	0.15%	0.015%
46	20.662	2914	2915	2917	rBV2	1401	1034	0.23%	0.023%
47	20.903	2953	2956	2959	rBV5	1584	2342	0.53%	0.053%
48	21.002	2971	2973	2977	rBV5	1775	2424	0.55%	0.054%
49	21.396	3039	3040	3041	rBV	1845	702	0.16%	0.016%
50	21.525	3061	3062	3063	rBV	1983	895	0.20%	0.020%
51	21.666	3083	3086	3087	rBV2	1699	1883	0.43%	0.042%
52	22.048	3144	3151	3159	rVB	164287	277229	62.58%	6.227%
53	22.142	3165	3167	3168	rBV2	1655	1155	0.26%	0.026%
54	22.594	3242	3244	3249	rVB5	2150	3132	0.71%	0.070%
55	22.641	3249	3252	3254	rBV4	1719	2494	0.56%	0.056%
56	22.735	3266	3268	3269	rBV2	2360	1231	0.28%	0.028%
57	22.835	3283	3285	3286	rBV2	1617	1173	0.26%	0.026%
58	23.299	3362	3364	3367	rBV4	1585	1557	0.35%	0.035%
59	23.593	3407	3414	3418	rBV7	4038	8592	1.94%	0.193%
60	23.681	3427	3429	3434	rVB5	1708	2665	0.60%	0.060%
61	23.716	3434	3435	3437	rBV2	1856	1115	0.25%	0.025%
62	23.846	3456	3457	3460	rBV3	1813	1847	0.42%	0.041%
63	24.304	3534	3535	3536	rBV	1705	913	0.21%	0.021%
64	24.457	3558	3561	3562	rBV3	2980	3110	0.70%	0.070%
65	24.615	3586	3588	3589	rBV	1985	1081	0.24%	0.024%
66	24.633	3589	3591	3593	rVB2	1239	850	0.19%	0.019%
67	24.709	3602	3604	3609	rBV3	1855	1872	0.42%	0.042%
68	25.021	3655	3657	3658	rVB2	1801	1215	0.27%	0.027%
69	25.244	3693	3695	3696	rBV2	1352	1191	0.27%	0.027%
70	25.326	3698	3709	3722	rVB	140072	405268	91.48%	9.103%
71	25.449	3729	3730	3731	rBV	1384	747	0.17%	0.017%
72	25.467	3731	3733	3734	rVV2	2296	1865	0.42%	0.042%
73	25.567	3734	3750	3762	rVB3	88718	274780	62.02%	6.172%
74	25.778	3784	3786	3787	rVB2	1276	805	0.18%	0.018%
75	25.919	3807	3810	3811	rBV3	2353	2283	0.52%	0.051%
76	26.236	3861	3864	3865	rBV3	1317	1385	0.31%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
 Data File : BG057247.D
 Acq On : 1 May 2023 11:20
 Operator : CG/JU
 Sample : PB152344BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK344

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

77	26.513	3909	3911	3914	rBV4	1809	1600	0.36%	0.036%
78	26.718	3944	3946	3947	rBV	2757	2284	0.52%	0.051%
79	27.059	4003	4004	4005	rBV	1408	744	0.17%	0.017%
80	27.306	4044	4046	4047	rBV2	1649	1003	0.23%	0.023%
81	27.652	4104	4105	4109	rVB4	2115	1690	0.38%	0.038%
82	27.687	4109	4111	4114	rBV4	1676	2115	0.48%	0.048%
83	27.834	4134	4136	4137	rVB2	1536	765	0.17%	0.017%
84	27.881	4141	4144	4145	rBV2	1483	1574	0.36%	0.035%
85	28.334	4219	4221	4222	rBV2	1247	731	0.17%	0.016%
86	28.428	4235	4237	4239	rBV2	1434	959	0.22%	0.022%
87	28.739	4289	4290	4292	rVB2	1839	752	0.17%	0.017%
88	28.997	4332	4334	4337	rBV4	1292	1005	0.23%	0.023%
89	29.044	4340	4342	4346	rBV3	1182	1033	0.23%	0.023%
90	29.074	4346	4347	4349	rBV2	1409	835	0.19%	0.019%
91	29.379	4397	4399	4400	rBV2	1400	914	0.21%	0.021%
92	29.585	4432	4434	4436	rBV3	1763	1650	0.37%	0.037%
93	30.090	4518	4520	4523	rVB4	1526	1290	0.29%	0.029%
94	30.707	4623	4625	4626	rVB2	1948	985	0.22%	0.022%
95	30.824	4643	4645	4649	rBV4	1910	2467	0.56%	0.055%
96	31.670	4787	4789	4790	rBV2	1266	934	0.21%	0.021%
97	31.811	4811	4813	4815	rBV3	1937	1280	0.29%	0.029%
98	32.152	4869	4871	4873	rBV3	1997	2187	0.49%	0.049%
99	32.516	4932	4933	4934	rBV	2022	968	0.22%	0.022%
100	32.628	4950	4952	4953	rVB2	1645	1030	0.23%	0.023%




Sum of corrected areas: 4452260

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
Data File : BG057247.D
Acq On : 1 May 2023 11:20
Operator : CG/JU
Sample : PB152344BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK344

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

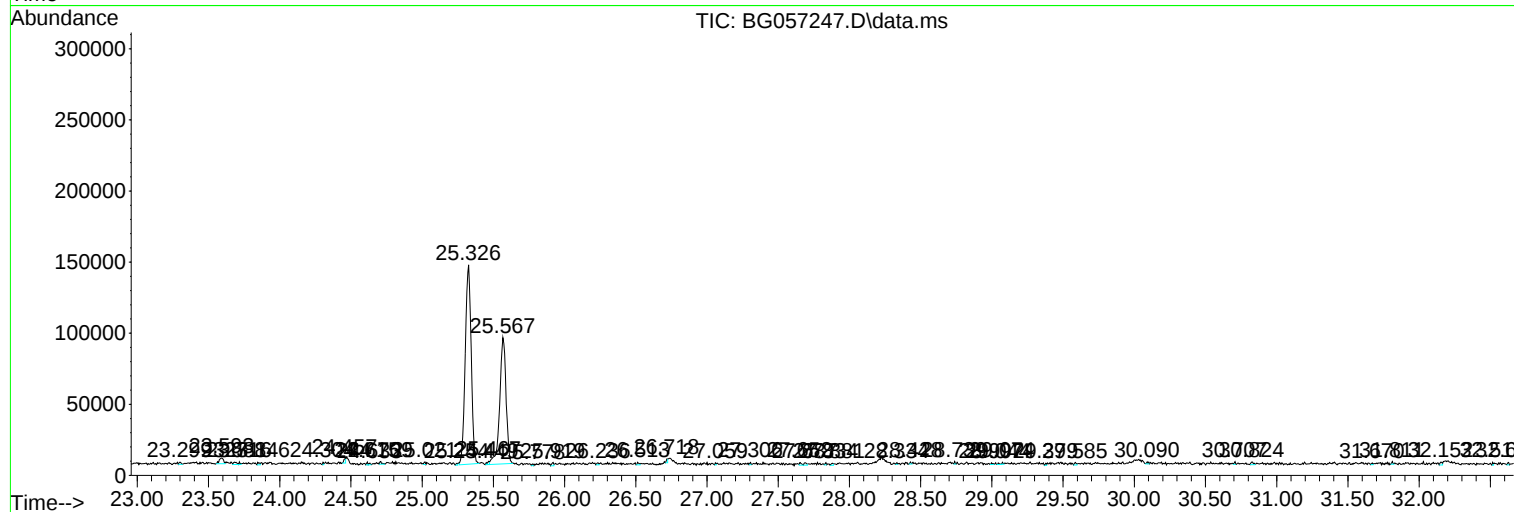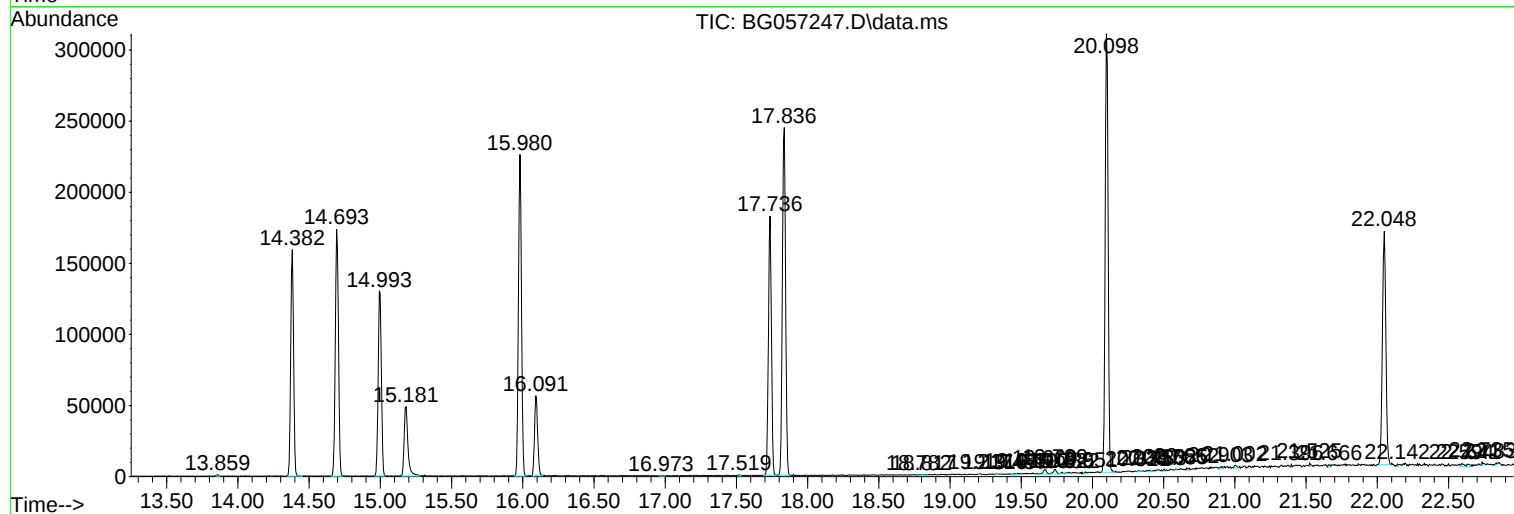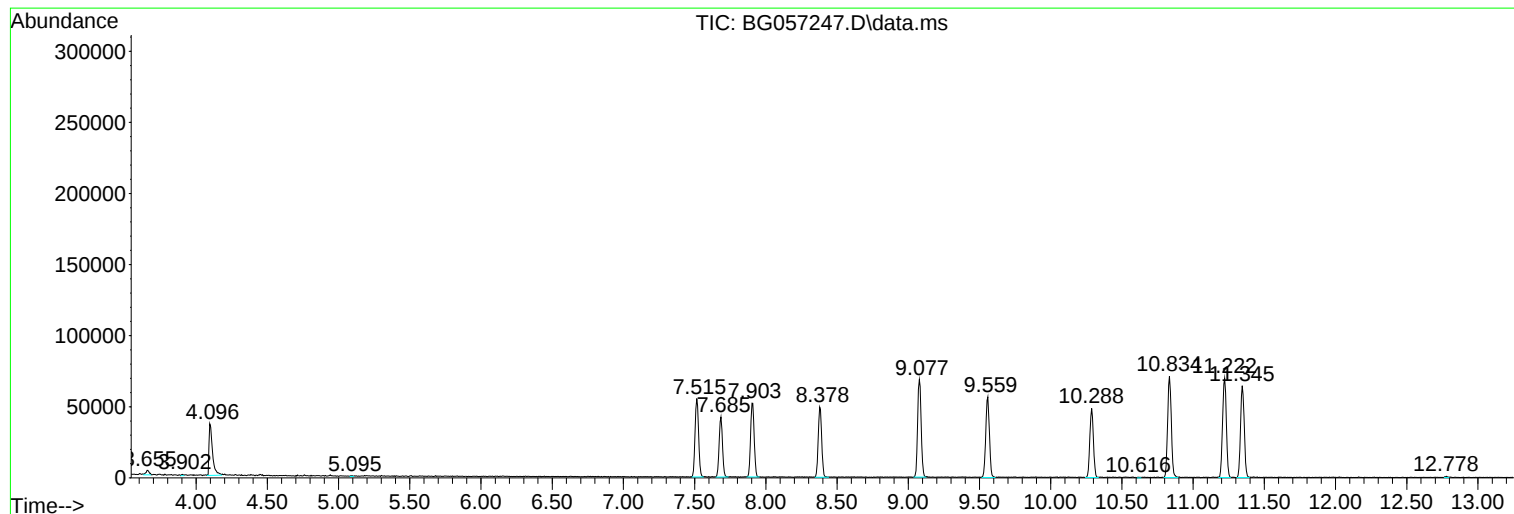

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
Data File : BG057247.D
Acq On : 1 May 2023 11:20
Operator : CG/JU
Sample : PB152344BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK344

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
Data File : BG057247.D
Acq On : 1 May 2023 11:20
Operator : CG/JU
Sample : PB152344BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK344

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc