

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
 Data File : BG057263.D
 Acq On : 1 May 2023 23:58
 Operator : CG/JU
 Sample : 02418-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW8Y9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG057263.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.652	18	19	21	rBV2	1218	960	0.37%	0.038%
2	3.864	53	55	58	rBV3	720	690	0.26%	0.027%
3	4.463	155	157	162	rVB	1212	820	0.31%	0.033%
4	4.563	172	174	176	rVB	559	405	0.16%	0.016%
5	4.604	179	181	182	rBV2	549	443	0.17%	0.018%
6	4.992	246	247	251	rVB2	592	672	0.26%	0.027%
7	5.133	269	271	273	rBV	517	435	0.17%	0.017%
8	5.174	276	278	282	rVB2	683	659	0.25%	0.026%
9	5.286	295	297	298	rBV2	418	353	0.14%	0.014%
10	5.344	306	307	309	rBV2	799	670	0.26%	0.027%
11	5.403	312	317	321	rVB3	1565	2728	1.05%	0.108%
12	5.626	354	355	356	rBV	701	341	0.13%	0.014%
13	5.896	399	401	404	rVB2	738	645	0.25%	0.026%
14	6.161	444	446	447	rVB	556	352	0.13%	0.014%
15	6.754	546	547	549	rBV	549	402	0.15%	0.016%
16	6.813	555	557	560	rVB	469	381	0.15%	0.015%
17	7.253	629	632	633	rBV2	369	448	0.17%	0.018%
18	7.518	672	677	686	rBB	23381	40283	15.44%	1.598%
19	7.682	700	705	714	rVB	23605	39021	14.96%	1.548%
20	7.835	729	731	733	rVB	486	347	0.13%	0.014%
21	7.864	733	736	738	rBV	448	546	0.21%	0.022%
22	7.911	738	744	752	rVV2	26464	44684	17.13%	1.773%
23	8.170	781	788	790	rBV2	459	764	0.29%	0.030%
24	8.381	817	824	831	rBV	60662	99786	38.25%	3.958%
25	8.669	871	873	875	rVB	405	344	0.13%	0.014%
26	8.757	885	888	890	rBV2	485	475	0.18%	0.019%
27	8.840	899	902	905	rVB2	347	382	0.15%	0.015%
28	8.951	919	921	924	rVB	516	434	0.17%	0.017%
29	9.080	937	943	950	rBV	16757	28379	10.88%	1.126%
30	9.210	960	965	973	rVB2	5013	8727	3.35%	0.346%
31	9.280	976	977	980	rBV2	382	395	0.15%	0.016%
32	9.456	1006	1007	1009	rBV	419	374	0.14%	0.015%
33	9.556	1017	1024	1033	rBV	32338	58804	22.54%	2.333%
34	9.680	1041	1045	1046	rBV2	336	361	0.14%	0.014%
35	9.744	1053	1056	1060	rVB2	350	523	0.20%	0.021%
36	10.285	1143	1148	1156	rVB2	23715	41099	15.76%	1.630%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
 Data File : BG057263.D
 Acq On : 1 May 2023 23:58
 Operator : CG/JU
 Sample : 02418-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW8Y9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

37	10.602	1199	1202	1205	rBV2	373	435	0.17%	0.017%
38	10.649	1205	1210	1212	rVB2	631	807	0.31%	0.032%
39	10.672	1212	1214	1216	rBV	350	420	0.16%	0.017%
40	10.837	1236	1242	1250	rBV	35523	61180	23.45%	2.427%
41	11.142	1291	1294	1297	rVB2	361	435	0.17%	0.017%
42	11.219	1300	1307	1315	rVV	83602	147222	56.44%	5.840%
43	11.307	1320	1322	1323	rBV	403	371	0.14%	0.015%
44	11.348	1323	1329	1341	rVB2	21513	36654	14.05%	1.454%
45	11.636	1376	1378	1383	rVB	340	496	0.19%	0.020%
46	11.742	1392	1396	1397	rVB	371	350	0.13%	0.014%
47	11.941	1428	1430	1432	rBV	458	492	0.19%	0.020%
48	12.200	1471	1474	1480	rVB2	314	416	0.16%	0.017%
49	12.781	1569	1573	1575	rBV2	670	741	0.28%	0.029%
50	12.811	1576	1578	1582	rVB	505	582	0.22%	0.023%
51	12.846	1582	1584	1585	rBV	660	587	0.23%	0.023%
52	14.379	1839	1845	1853	rVB	83053	114535	43.91%	4.543%
53	14.690	1892	1898	1905	rBV	89286	141138	54.11%	5.599%
54	14.996	1943	1950	1956	rVB	143557	217508	83.38%	8.628%
55	15.196	1980	1984	1992	rBV2	2700	4941	1.89%	0.196%
56	15.325	2004	2006	2010	rVB	515	647	0.25%	0.026%
57	15.648	2057	2061	2064	rBV	209	371	0.14%	0.015%
58	15.977	2110	2117	2124	rBV	113427	171694	65.82%	6.811%
59	16.094	2135	2137	2145	rVB2	2014	2546	0.98%	0.101%
60	16.329	2172	2177	2181	rVB	6954	9629	3.69%	0.382%
61	16.494	2202	2205	2208	rBV	281	425	0.16%	0.017%
62	16.670	2231	2235	2237	rVB3	1116	1236	0.47%	0.049%
63	16.805	2254	2258	2262	rBV	299	396	0.15%	0.016%
64	17.240	2330	2332	2333	rBV	374	357	0.14%	0.014%
65	17.387	2355	2357	2359	rBV	714	465	0.18%	0.018%
66	17.434	2363	2365	2369	rBV	1077	995	0.38%	0.039%
67	17.481	2372	2373	2378	rBV	526	612	0.23%	0.024%
68	17.522	2378	2380	2383	rBV	527	526	0.20%	0.021%
69	17.592	2388	2392	2394	rBV2	2050	2865	1.10%	0.114%
70	17.657	2400	2403	2405	rBV	1125	1368	0.52%	0.054%
71	17.733	2410	2416	2422	rBV	176157	260848	100.00%	10.347%
72	17.833	2427	2433	2441	rVB	112533	161383	61.87%	6.402%
73	17.968	2454	2456	2459	rVB	705	773	0.30%	0.031%
74	18.127	2482	2483	2486	rVB2	502	369	0.14%	0.015%
75	18.174	2486	2491	2493	rVB2	1323	1426	0.55%	0.057%
76	18.221	2497	2499	2501	rBV2	377	385	0.15%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
 Data File : BG057263.D
 Acq On : 1 May 2023 23:58
 Operator : CG/JU
 Sample : 02418-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW8Y9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

77	18.403	2527	2530	2534	rBV	868	1235	0.47%	0.049%
78	18.468	2538	2541	2545	rVV3	2660	4001	1.53%	0.159%
79	18.526	2548	2551	2554	rVV3	1311	1914	0.73%	0.076%
80	18.573	2556	2559	2568	rVV4	9543	16617	6.37%	0.659%
81	18.644	2568	2571	2575	rVB4	2328	3156	1.21%	0.125%
82	18.744	2587	2588	2590	rVB	1168	416	0.16%	0.017%
83	18.791	2590	2596	2601	rBV5	1258	2821	1.08%	0.112%
84	18.850	2605	2606	2608	rBV	1807	1322	0.51%	0.052%
85	18.885	2610	2612	2614	rVB2	1003	867	0.33%	0.034%
86	18.908	2614	2616	2617	rBV2	843	496	0.19%	0.020%
87	18.949	2620	2623	2626	rBV3	1984	2814	1.08%	0.112%
88	19.079	2643	2645	2646	rBV	1106	972	0.37%	0.039%
89	19.149	2655	2657	2658	rBV	1478	1394	0.53%	0.055%
90	19.208	2665	2667	2669	rBV3	634	421	0.16%	0.017%
91	19.249	2671	2674	2676	rBV3	945	1023	0.39%	0.041%
92	19.290	2680	2681	2685	rBV2	1001	1562	0.60%	0.062%
93	19.361	2691	2693	2694	rBV2	1042	589	0.23%	0.023%
94	19.437	2704	2706	2707	rBV2	1403	797	0.31%	0.032%
95	19.766	2759	2762	2768	rVB	12287	15751	6.04%	0.625%
96	19.813	2768	2770	2771	rBV2	2273	1655	0.63%	0.066%
97	20.101	2813	2819	2828	rBV	132720	204160	78.27%	8.099%
98	20.418	2869	2873	2880	rVB2	27701	37431	14.35%	1.485%
99	22.045	3144	3150	3157	rVB2	142210	254006	97.38%	10.076%
100	25.576	3743	3751	3763	rVB2	79577	239741	91.91%	9.510%




Sum of corrected areas: 2520919

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
Data File : BG057263.D
Acq On : 1 May 2023 23:58
Operator : CG/JU
Sample : 02418-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW8Y9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

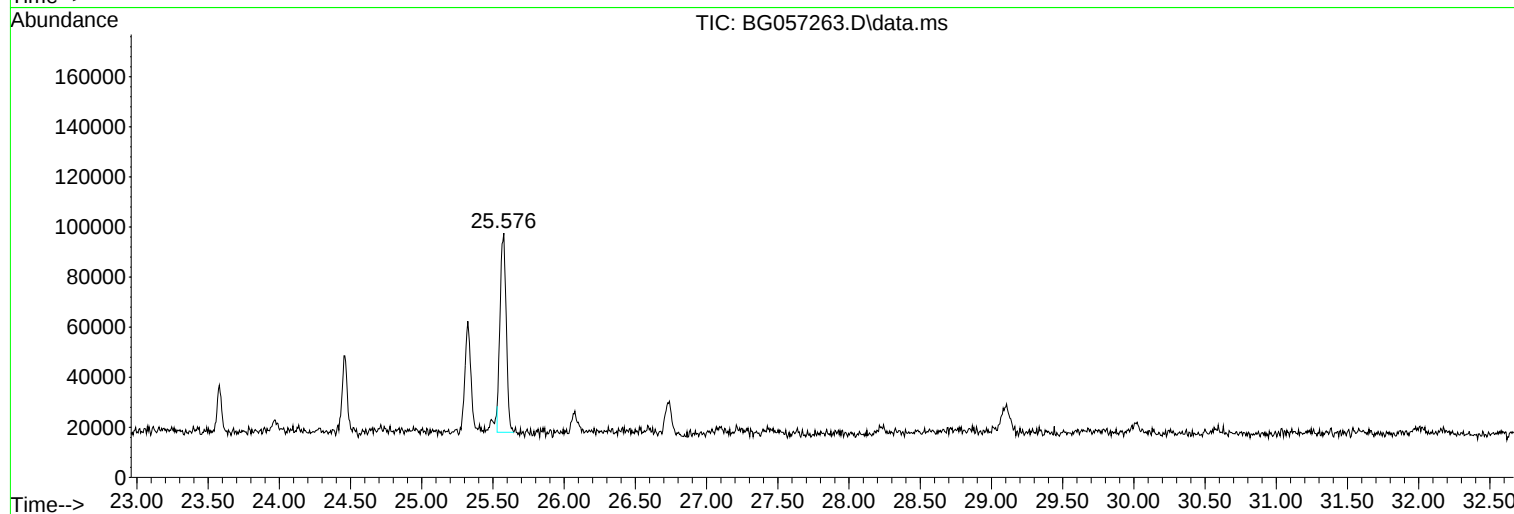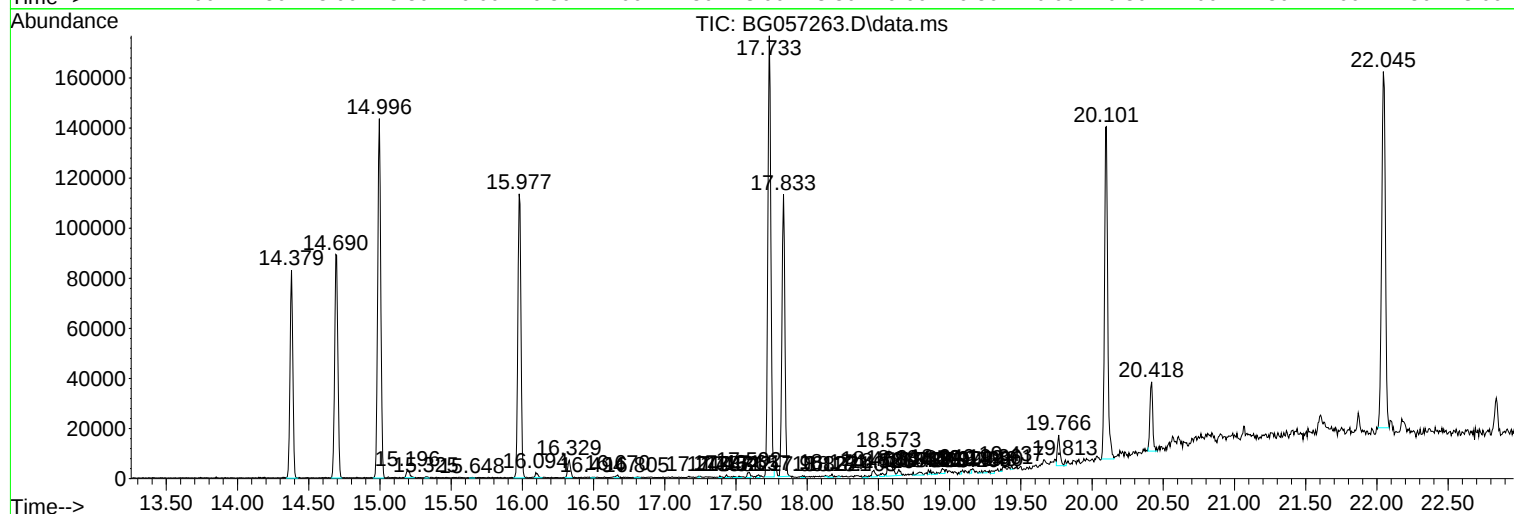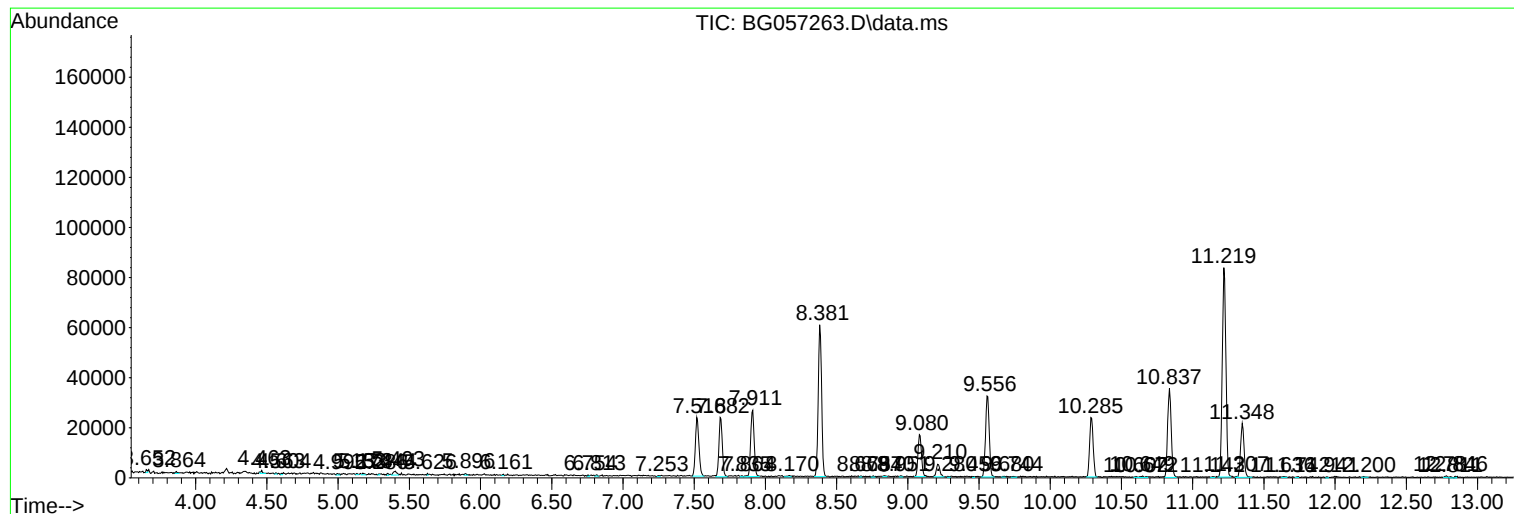

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
Data File : BG057263.D
Acq On : 1 May 2023 23:58
Operator : CG/JU
Sample : 02418-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW8Y9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
Data File : BG057263.D
Acq On : 1 May 2023 23:58
Operator : CG/JU
Sample : 02418-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW8Y9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc