

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
 Data File : BG057264.D
 Acq On : 2 May 2023 00:40
 Operator : CG/JU
 Sample : 02418-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW8Z4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG057264.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.819	46	48	49	rBV	548	384	0.13%	0.017%
2	4.812	215	217	220	rBV2	756	975	0.34%	0.044%
3	5.405	313	318	324	rVB3	1392	2673	0.92%	0.120%
4	5.599	349	351	353	rBV2	482	510	0.18%	0.023%
5	5.798	383	385	388	rBV2	448	504	0.17%	0.023%
6	6.139	442	443	445	rBV	547	394	0.14%	0.018%
7	6.791	553	554	557	rBV	412	442	0.15%	0.020%
8	6.985	583	587	589	rBV2	474	779	0.27%	0.035%
9	7.108	605	608	609	rBV	477	611	0.21%	0.027%
10	7.361	650	651	654	rBV	650	753	0.26%	0.034%
11	7.520	673	678	687	rVB2	16701	30034	10.37%	1.346%
12	7.684	701	706	713	rVB	18999	29061	10.03%	1.303%
13	7.907	738	744	752	rVB	21085	35217	12.16%	1.579%
14	8.313	809	813	816	rBV2	266	469	0.16%	0.021%
15	8.383	818	825	831	rVB	65076	109422	37.78%	4.905%
16	8.683	871	876	877	rBV2	435	686	0.24%	0.031%
17	8.700	877	879	882	rVB2	485	546	0.19%	0.024%
18	9.029	931	935	938	rBV	449	643	0.22%	0.029%
19	9.082	938	944	954	rVV2	25565	43981	15.19%	1.972%
20	9.211	962	966	976	rVB2	5457	9821	3.39%	0.440%
21	9.311	982	983	986	rBV	438	447	0.15%	0.020%
22	9.417	998	1001	1004	rBV2	356	491	0.17%	0.022%
23	9.558	1018	1025	1032	rBV2	25586	45326	15.65%	2.032%
24	9.781	1061	1063	1066	rVB2	352	404	0.14%	0.018%
25	10.116	1117	1120	1122	rVB2	356	413	0.14%	0.019%
26	10.134	1122	1123	1125	rBV2	414	381	0.13%	0.017%
27	10.292	1144	1150	1156	rVB2	16418	28154	9.72%	1.262%
28	10.521	1185	1189	1190	rBV2	290	396	0.14%	0.018%
29	10.639	1206	1209	1212	rVB2	639	680	0.23%	0.030%
30	10.839	1237	1243	1255	rVB	24305	43111	14.88%	1.933%
31	10.944	1258	1261	1262	rVB	466	472	0.16%	0.021%
32	10.962	1262	1264	1266	rBV	463	552	0.19%	0.025%
33	11.220	1301	1308	1315	rVB	92161	162572	56.13%	7.288%
34	11.273	1315	1317	1321	rBV2	596	658	0.23%	0.029%
35	11.350	1324	1330	1335	rBV2	12694	21491	7.42%	0.963%
36	11.438	1343	1345	1352	rBV2	362	580	0.20%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
 Data File : BG057264.D
 Acq On : 2 May 2023 00:40
 Operator : CG/JU
 Sample : 02418-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW8Z4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

37	11.726	1393	1394	1400	rVB2	308	445	0.15%	0.020%
38	11.996	1438	1440	1446	rBV	391	611	0.21%	0.027%
39	12.848	1583	1585	1588	rBV2	581	701	0.24%	0.031%
40	13.071	1620	1623	1625	rVB	413	400	0.14%	0.018%
41	13.788	1741	1745	1747	rVB	351	371	0.13%	0.017%
42	14.310	1831	1834	1838	rBV	427	486	0.17%	0.022%
43	14.381	1840	1846	1852	rVV	59398	82989	28.65%	3.720%
44	14.557	1872	1876	1877	rBV	457	390	0.13%	0.017%
45	14.692	1893	1899	1905	rBV	65090	97950	33.82%	4.391%
46	14.998	1944	1951	1959	rVB	158832	242086	83.58%	10.852%
47	15.197	1983	1985	1987	rBV	1155	1201	0.41%	0.054%
48	15.891	2100	2103	2106	rBV	245	388	0.13%	0.017%
49	15.979	2111	2118	2126	rVB	98832	145559	50.26%	6.525%
50	16.220	2157	2159	2162	rVB	362	402	0.14%	0.018%
51	16.331	2173	2178	2182	rBV2	6743	9634	3.33%	0.432%
52	16.466	2198	2201	2203	rBV	348	449	0.16%	0.020%
53	16.666	2228	2235	2238	rVB3	1577	2537	0.88%	0.114%
54	16.895	2272	2274	2278	rVB	570	462	0.16%	0.021%
55	17.001	2288	2292	2294	rBV2	620	788	0.27%	0.035%
56	17.430	2364	2365	2369	rVB	966	821	0.28%	0.037%
57	17.483	2371	2374	2377	rBV	752	773	0.27%	0.035%
58	17.518	2377	2380	2381	rBV	554	522	0.18%	0.023%
59	17.594	2390	2393	2396	rVB	1672	1626	0.56%	0.073%
60	17.735	2410	2417	2423	rBV	189543	289632	100.00%	12.983%
61	17.835	2428	2434	2443	rVB	91928	137941	47.63%	6.183%
62	17.970	2455	2457	2460	rVB2	725	852	0.29%	0.038%
63	18.000	2460	2462	2463	rBV	719	514	0.18%	0.023%
64	18.170	2486	2491	2496	rBV3	1348	2205	0.76%	0.099%
65	18.281	2507	2510	2511	rBV	557	472	0.16%	0.021%
66	18.464	2539	2541	2543	rBV	535	396	0.14%	0.018%
67	18.581	2558	2561	2564	rVB2	1515	2027	0.70%	0.091%
68	18.652	2569	2573	2577	rVB2	1158	1657	0.57%	0.074%
69	18.704	2581	2582	2585	rVB	867	425	0.15%	0.019%
70	18.787	2594	2596	2597	rBV	810	781	0.27%	0.035%
71	18.845	2604	2606	2607	rVV2	894	494	0.17%	0.022%
72	18.881	2610	2612	2613	rBV2	552	412	0.14%	0.018%
73	18.986	2628	2630	2631	rBV	892	711	0.25%	0.032%
74	19.022	2633	2636	2637	rBV2	943	939	0.32%	0.042%
75	19.039	2637	2639	2642	rBV3	1031	1275	0.44%	0.057%
76	19.080	2642	2646	2652	rVV3	5477	6960	2.40%	0.312%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
 Data File : BG057264.D
 Acq On : 2 May 2023 00:40
 Operator : CG/JU
 Sample : 02418-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW8Z4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

77	19.122	2652	2653	2654	rVV3	1477	665	0.23%	0.030%
78	19.139	2654	2656	2658	rVV2	1331	1273	0.44%	0.057%
79	19.169	2660	2661	2665	rVV4	1422	1341	0.46%	0.060%
80	19.221	2669	2670	2672	rBV2	1092	611	0.21%	0.027%
81	19.292	2678	2682	2684	rBV3	1744	2513	0.87%	0.113%
82	19.351	2690	2692	2693	rVV2	1041	539	0.19%	0.024%
83	19.380	2695	2697	2700	rVB4	1962	1662	0.57%	0.075%
84	19.468	2710	2712	2715	rVB2	2170	1899	0.66%	0.085%
85	19.533	2721	2723	2726	rBV4	1219	1061	0.37%	0.048%
86	19.603	2733	2735	2737	rBV3	1735	1899	0.66%	0.085%
87	19.774	2760	2764	2766	rBV2	3084	3924	1.35%	0.176%
88	20.097	2814	2819	2825	rBV2	29404	42213	14.57%	1.892%
89	22.047	3145	3151	3158	rBV2	169114	281814	97.30%	12.633%
90	25.572	3743	3751	3763	rVB2	93162	276096	95.33%	12.376%




Sum of corrected areas: 2230827

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
Data File : BG057264.D
Acq On : 2 May 2023 00:40
Operator : CG/JU
Sample : 02418-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW8Z4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

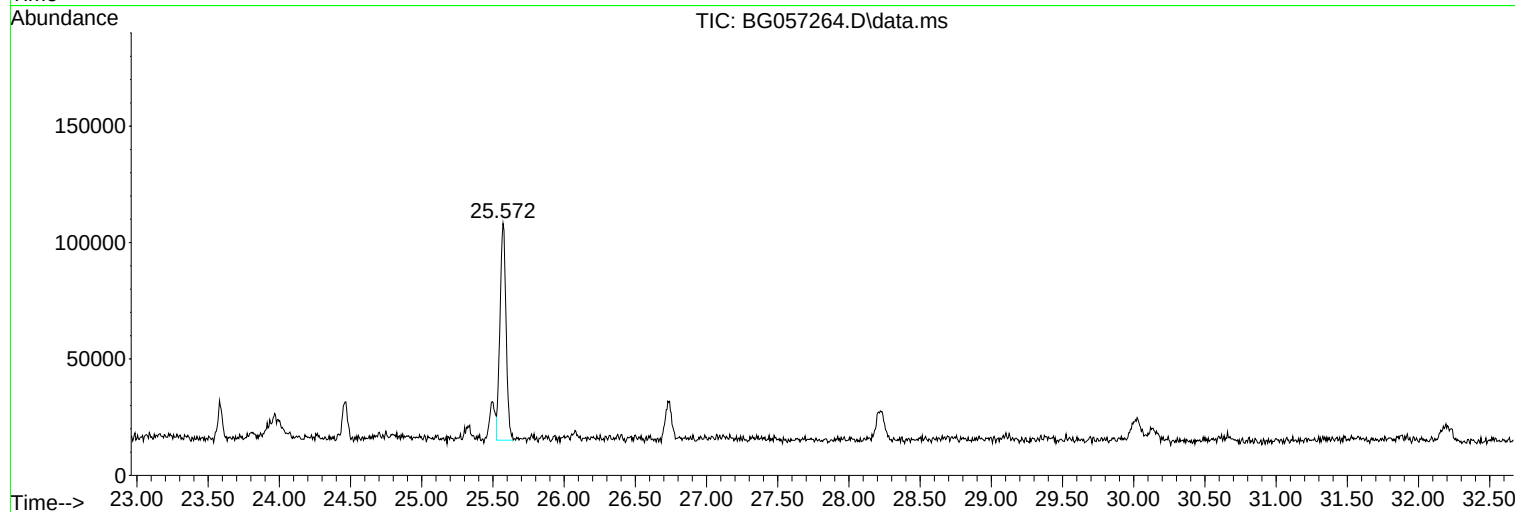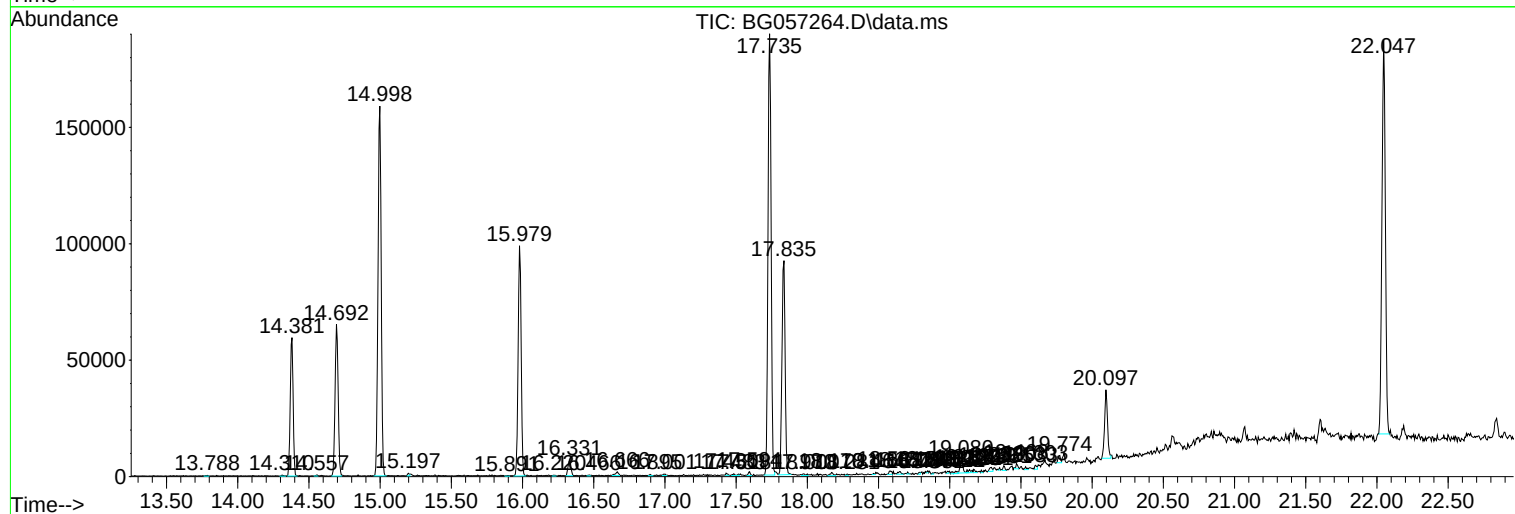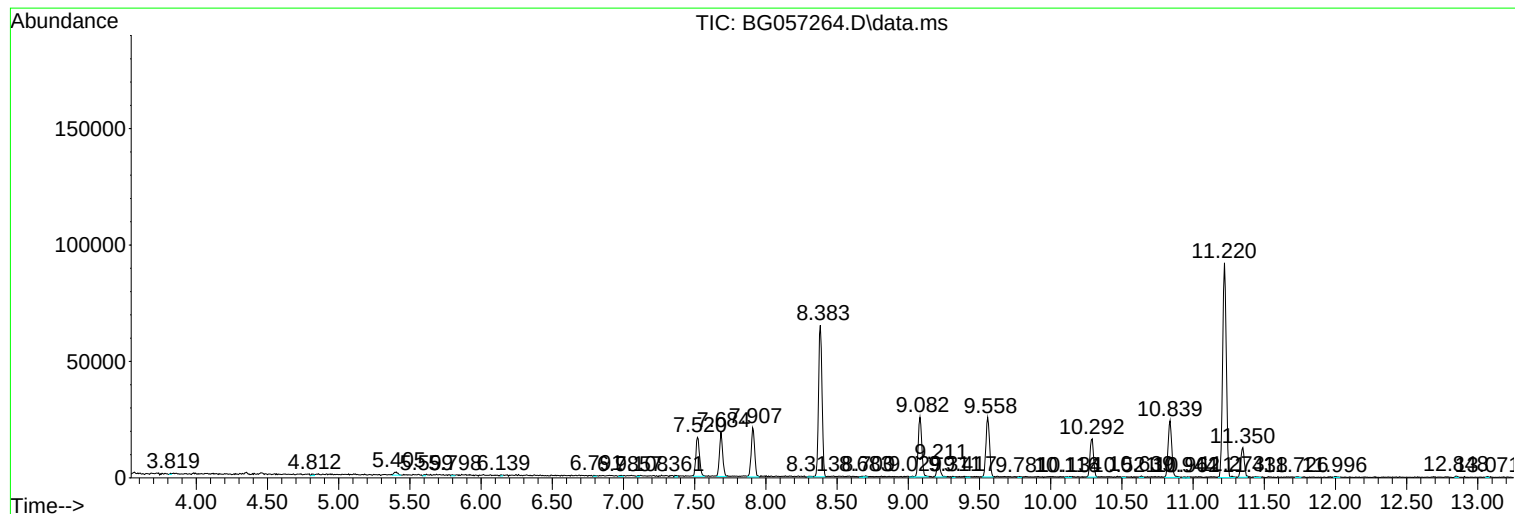

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
Data File : BG057264.D
Acq On : 2 May 2023 00:40
Operator : CG/JU
Sample : 02418-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW8Z4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
Data File : BG057264.D
Acq On : 2 May 2023 00:40
Operator : CG/JU
Sample : 02418-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW8Z4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc