

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
 Data File : BG057270.D
 Acq On : 2 May 2023 8:46
 Operator : CG/JU
 Sample : PB152413BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK413

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG057270.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.655	17	20	27	rVV4	3594	4871	1.03%	0.097%
2	3.966	72	73	77	rBV2	818	1060	0.22%	0.021%
3	4.049	85	87	90	rVB2	771	617	0.13%	0.012%
4	4.096	92	95	108	rBV	44536	76393	16.17%	1.526%
5	4.331	134	135	137	rVB	876	614	0.13%	0.012%
6	4.460	153	157	159	rVV2	1063	1478	0.31%	0.030%
7	4.513	163	166	168	rBV3	708	723	0.15%	0.014%
8	4.660	188	191	192	rVB2	777	629	0.13%	0.013%
9	5.652	358	360	364	rVB2	667	851	0.18%	0.017%
10	6.252	459	462	465	rBV	709	910	0.19%	0.018%
11	7.520	671	678	685	rBV	74648	130819	27.69%	2.613%
12	7.685	699	706	715	rVB	54280	90121	19.07%	1.800%
13	7.908	737	744	754	rVV	74187	124851	26.42%	2.494%
14	8.378	819	824	835	rVB	60719	104408	22.10%	2.086%
15	8.760	885	889	892	rVB	563	768	0.16%	0.015%
16	8.919	911	916	922	rVB2	394	903	0.19%	0.018%
17	9.077	937	943	953	rBV	90905	161706	34.23%	3.230%
18	9.236	967	970	972	rBV2	410	559	0.12%	0.011%
19	9.295	976	980	983	rBV2	386	706	0.15%	0.014%
20	9.371	989	993	997	rVB2	314	562	0.12%	0.011%
21	9.559	1017	1025	1032	rBV	76527	134216	28.41%	2.681%
22	9.741	1053	1056	1058	rBV2	368	576	0.12%	0.012%
23	10.164	1124	1128	1131	rBV2	452	652	0.14%	0.013%
24	10.287	1143	1149	1158	rBV2	65488	118612	25.10%	2.369%
25	10.834	1235	1242	1251	rBV	96974	169953	35.97%	3.395%
26	11.221	1300	1308	1316	rVB	88178	155169	32.84%	3.100%
27	11.345	1322	1329	1337	rBV	81582	149257	31.59%	2.982%
28	11.456	1345	1348	1351	rVB	500	658	0.14%	0.013%
29	11.486	1351	1353	1357	rBV2	517	894	0.19%	0.018%
30	11.544	1361	1363	1366	rBV	471	667	0.14%	0.013%
31	12.778	1568	1573	1579	rBV2	1724	2879	0.61%	0.058%
32	13.859	1754	1757	1761	rBV2	1357	1824	0.39%	0.036%
33	14.382	1840	1846	1854	rVB	179267	259689	54.96%	5.188%
34	14.699	1893	1900	1909	rVB2	197616	312139	66.06%	6.235%
35	14.999	1944	1951	1958	rBV	149561	224885	47.60%	4.492%
36	15.181	1977	1982	1992	rBV	54022	99906	21.15%	1.996%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
 Data File : BG057270.D
 Acq On : 2 May 2023 8:46
 Operator : CG/JU
 Sample : PB152413BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK413

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

37	15.251	1992	1994	1999	rVV2	1534	2303	0.49%	0.046%
38	15.985	2111	2119	2126	rVB	243251	378960	80.21%	7.570%
39	16.097	2133	2138	2148	rVB	56506	86073	18.22%	1.719%
40	16.220	2156	2159	2163	rBV	474	603	0.13%	0.012%

41	17.513	2378	2379	2382	rBV	689	558	0.12%	0.011%
42	17.619	2392	2397	2399	rBV	508	566	0.12%	0.011%
43	17.736	2411	2417	2424	rBV	186286	272327	57.64%	5.440%
44	17.836	2428	2434	2443	rVV	274872	407878	86.33%	8.148%
45	18.159	2485	2489	2492	rVB2	375	616	0.13%	0.012%

46	18.412	2530	2532	2534	rBV2	525	614	0.13%	0.012%
47	19.252	2673	2675	2678	rVB	634	572	0.12%	0.011%
48	19.398	2698	2700	2701	rBV	796	570	0.12%	0.011%
49	19.498	2715	2717	2718	rBV	629	561	0.12%	0.011%
50	19.669	2742	2746	2750	rVB5	3636	5140	1.09%	0.103%

51	19.739	2754	2758	2762	rVB	3312	4515	0.96%	0.090%
52	19.857	2777	2778	2781	rBV2	871	667	0.14%	0.013%
53	19.939	2791	2792	2794	rBV	922	560	0.12%	0.011%
54	19.968	2794	2797	2803	rVB2	1420	2969	0.63%	0.059%
55	20.021	2803	2806	2807	rBV2	898	1047	0.22%	0.021%

56	20.103	2814	2820	2827	rBV	338444	472475	100.00%	9.438%
57	20.174	2830	2832	2833	rBV2	1305	808	0.17%	0.016%
58	20.244	2841	2844	2846	rBV3	1102	1251	0.26%	0.025%
59	20.368	2863	2865	2868	rVB2	1195	1068	0.23%	0.021%
60	20.515	2887	2890	2893	rBV5	1102	1523	0.32%	0.030%

61	20.567	2897	2899	2901	rVB3	2174	1482	0.31%	0.030%
62	20.814	2939	2941	2942	rVB2	2426	1411	0.30%	0.028%
63	20.832	2942	2944	2947	rBV4	1277	1814	0.38%	0.036%
64	21.290	3020	3022	3023	rVB2	1684	1092	0.23%	0.022%
65	21.308	3023	3025	3028	rBV4	1585	2206	0.47%	0.044%

66	21.736	3097	3098	3099	rVB	2567	905	0.19%	0.018%
67	21.842	3114	3116	3118	rBV2	1701	1171	0.25%	0.023%
68	22.054	3145	3152	3159	rVB2	159144	272953	57.77%	5.452%
69	22.183	3172	3174	3178	rBV5	2595	3835	0.81%	0.077%
70	22.524	3230	3232	3234	rBV2	1872	1318	0.28%	0.026%

71	22.806	3278	3280	3283	rBV4	1782	1853	0.39%	0.037%
72	23.399	3379	3381	3382	rBV2	3008	2316	0.49%	0.046%
73	23.593	3410	3414	3417	rBV5	3300	4240	0.90%	0.085%
74	23.810	3449	3451	3454	rBV4	2316	2699	0.57%	0.054%
75	24.022	3486	3487	3488	rVB	1782	627	0.13%	0.013%

76	24.462	3559	3562	3564	rBV4	3864	4350	0.92%	0.087%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
 Data File : BG057270.D
 Acq On : 2 May 2023 8:46
 Operator : CG/JU
 Sample : PB152413BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK413

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

77	24.580	3581	3582	3583	rBV	1988	801	0.17%	0.016%
78	25.338	3699	3711	3722	rBV2	147024	419982	88.89%	8.389%
79	25.514	3734	3741	3742	rBV7	5010	8814	1.87%	0.176%
80	25.578	3742	3752	3765	rVB2	85012	257918	54.59%	5.152%
81	25.784	3786	3787	3788	rBV	1831	787	0.17%	0.016%
82	26.835	3964	3966	3969	rVB3	2148	1958	0.41%	0.039%
83	27.023	3996	3998	4000	rBV3	1556	939	0.20%	0.019%
84	27.670	4106	4108	4113	rBV6	1627	2190	0.46%	0.044%
85	28.615	4267	4269	4270	rBV2	2008	903	0.19%	0.018%
86	29.132	4355	4357	4360	rBV4	1866	2255	0.48%	0.045%
87	29.667	4446	4448	4449	rBV2	1611	860	0.18%	0.017%
88	30.196	4536	4538	4543	rVB5	2273	2413	0.51%	0.048%
89	30.354	4563	4565	4566	rBV3	2042	873	0.18%	0.017%
90	30.595	4604	4606	4607	rBV2	1943	852	0.18%	0.017%
91	31.347	4730	4734	4736	rBV5	2179	3371	0.71%	0.067%
92	31.582	4773	4774	4776	rBV2	2324	1652	0.35%	0.033%
93	31.788	4805	4809	4812	rBV5	2132	3710	0.79%	0.074%
94	31.846	4817	4819	4822	rVB4	2110	1897	0.40%	0.038%
95	31.923	4830	4832	4835	rVB4	2006	1571	0.33%	0.031%
96	32.087	4858	4860	4861	rBV2	1643	1263	0.27%	0.025%
97	32.240	4884	4886	4889	rVB4	2277	2111	0.45%	0.042%
98	32.381	4907	4910	4911	rBV3	2225	2403	0.51%	0.048%
99	32.493	4927	4929	4930	rVB2	2425	1249	0.26%	0.025%
100	32.510	4930	4932	4933	rBV2	1734	1259	0.27%	0.025%




Sum of corrected areas: 5006052

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
Data File : BG057270.D
Acq On : 2 May 2023 8:46
Operator : CG/JU
Sample : PB152413BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK413

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

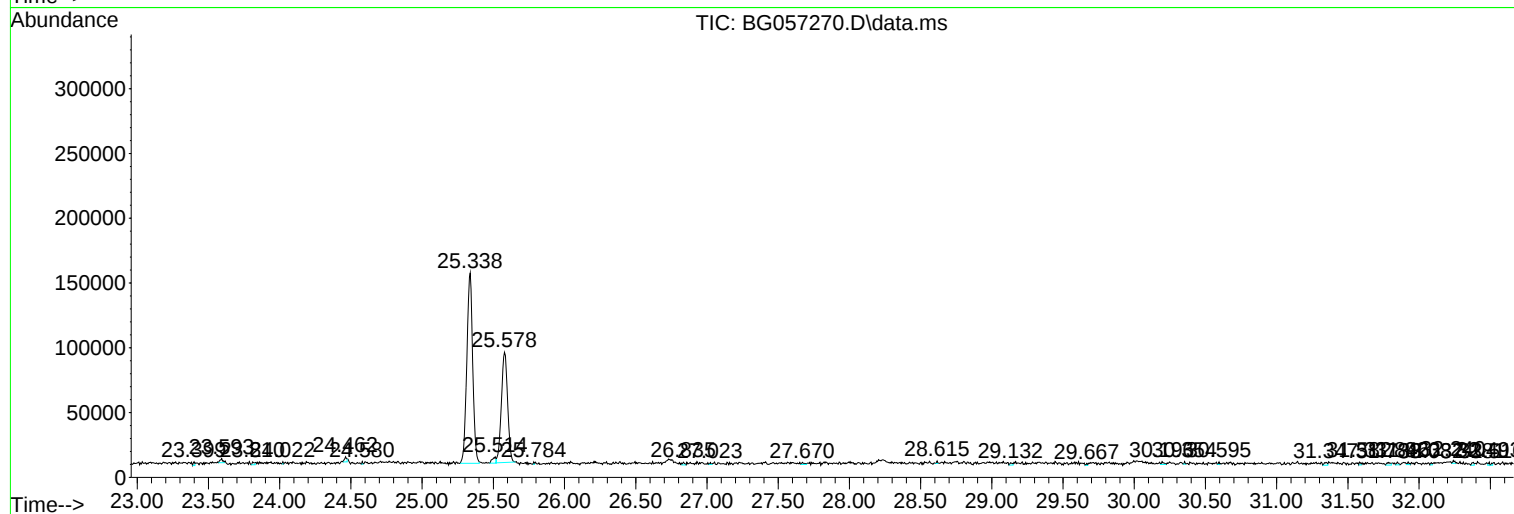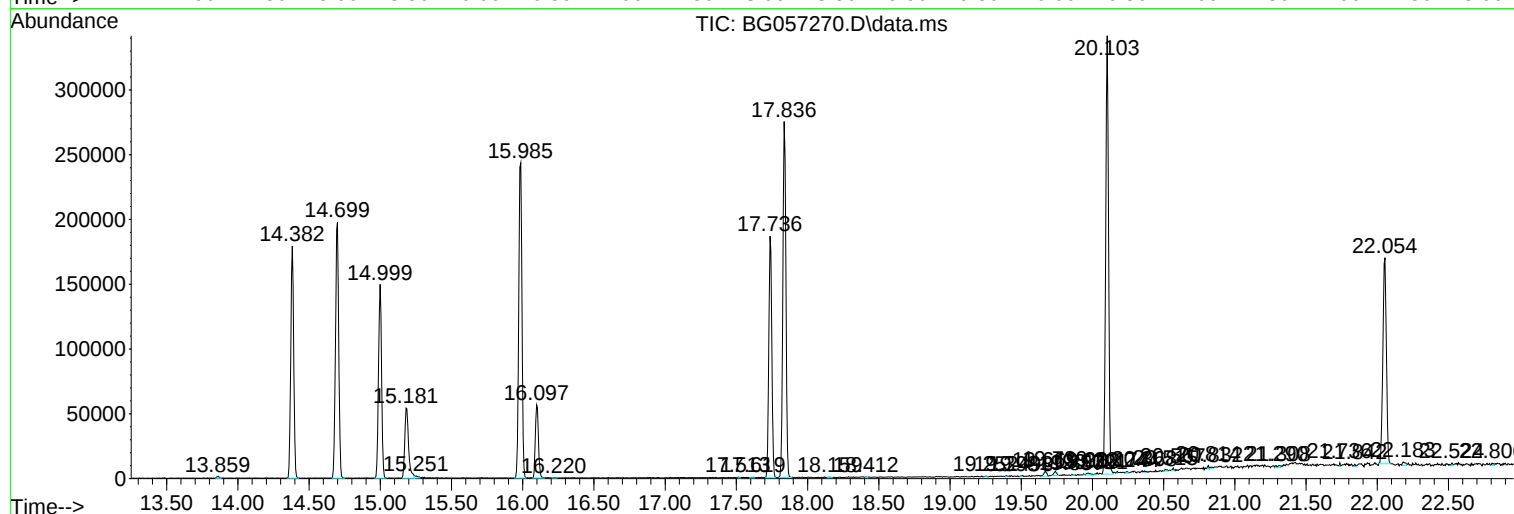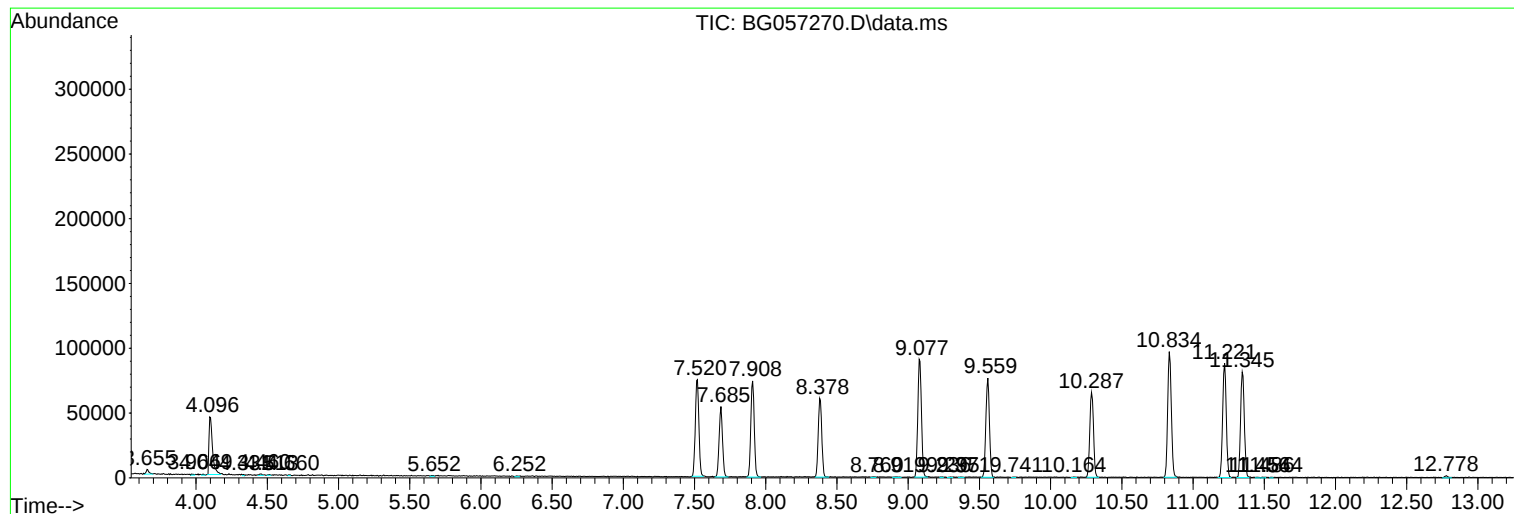

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
Data File : BG057270.D
Acq On : 2 May 2023 8:46
Operator : CG/JU
Sample : PB152413BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK413

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
Data File : BG057270.D
Acq On : 2 May 2023 8:46
Operator : CG/JU
Sample : PB152413BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK413

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc