

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
 Data File : BG057271.D
 Acq On : 2 May 2023 9:36
 Operator : CG/JU
 Sample : 02418-08
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW8Z4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG057271.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.454	154	156	163	rVB2	922	1315	0.51%	0.050%
2	4.578	174	177	178	rBV	613	553	0.21%	0.021%
3	4.866	224	226	231	rVB	787	633	0.25%	0.024%
4	5.077	260	262	263	rVB	634	330	0.13%	0.013%
5	6.839	560	562	564	rBV2	430	494	0.19%	0.019%
6	7.521	672	678	686	rBV	29420	50460	19.54%	1.915%
7	7.685	699	706	713	rBV	24348	41783	16.18%	1.585%
8	7.809	725	727	730	rBV2	288	355	0.14%	0.013%
9	7.909	738	744	751	rVB	32413	52428	20.30%	1.989%
10	8.296	807	810	812	rBV	438	395	0.15%	0.015%
11	8.378	817	824	832	rVV	58401	95360	36.93%	3.618%
12	9.078	937	943	953	rBV	40501	68454	26.51%	2.597%
13	9.213	961	966	973	rBV2	4418	8248	3.19%	0.313%
14	9.559	1018	1025	1034	rVB	37415	66185	25.63%	2.511%
15	9.618	1034	1035	1039	rBV	437	507	0.20%	0.019%
16	9.918	1082	1086	1088	rBV2	260	415	0.16%	0.016%
17	9.994	1098	1099	1102	rBV	404	374	0.14%	0.014%
18	10.288	1143	1149	1156	rVB3	25995	46099	17.85%	1.749%
19	10.834	1234	1242	1252	rVB	40682	70395	27.26%	2.671%
20	10.904	1252	1254	1255	rBV	562	536	0.21%	0.020%
21	11.004	1268	1271	1274	rVB	332	378	0.15%	0.014%
22	11.040	1274	1277	1280	rBV2	331	468	0.18%	0.018%
23	11.092	1285	1286	1288	rBV2	376	357	0.14%	0.014%
24	11.222	1301	1308	1315	rVB	80487	141601	54.84%	5.373%
25	11.345	1322	1329	1338	rVB3	25773	46668	18.07%	1.771%
26	11.474	1349	1351	1356	rVB	405	463	0.18%	0.018%
27	11.510	1356	1357	1361	rBV	354	347	0.13%	0.013%
28	11.586	1367	1370	1374	rBV	380	589	0.23%	0.022%
29	11.645	1377	1380	1381	rBV	293	338	0.13%	0.013%
30	11.668	1381	1384	1388	rVB2	354	567	0.22%	0.022%
31	11.709	1388	1391	1394	rBV2	374	453	0.18%	0.017%
32	11.815	1407	1409	1413	rVB2	370	364	0.14%	0.014%
33	11.868	1415	1418	1421	rBV2	355	494	0.19%	0.019%
34	12.508	1524	1527	1530	rVB	308	359	0.14%	0.014%
35	12.778	1570	1573	1576	rVB	503	452	0.18%	0.017%
36	12.849	1583	1585	1589	rVB	558	558	0.22%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
 Data File : BG057271.D
 Acq On : 2 May 2023 9:36
 Operator : CG/JU
 Sample : 02418-08
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW8Z4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

37	13.859	1751	1757	1759	rBV3	1364	1886	0.73%	0.072%
38	14.312	1832	1834	1836	rBV	472	360	0.14%	0.014%
39	14.376	1840	1845	1852	rVB	87292	120965	46.84%	4.590%
40	14.693	1893	1899	1907	rVB	96676	145756	56.44%	5.530%
41	14.993	1944	1950	1957	rVB	132401	212848	82.43%	8.076%
42	15.193	1979	1984	1995	rBV4	8262	16085	6.23%	0.610%
43	15.387	2014	2017	2020	rBV	406	385	0.15%	0.015%
44	15.980	2112	2118	2125	rVB2	131832	197996	76.68%	7.512%
45	16.097	2135	2138	2148	rVB3	6612	8904	3.45%	0.338%
46	16.221	2156	2159	2160	rBV	442	414	0.16%	0.016%
47	16.327	2173	2177	2182	rBV	6317	8890	3.44%	0.337%
48	16.644	2227	2231	2233	rBV	707	703	0.27%	0.027%
49	16.667	2233	2235	2240	rVB3	1282	1550	0.60%	0.059%
50	16.896	2272	2274	2278	rBV	365	427	0.17%	0.016%
51	16.990	2289	2290	2295	rVB2	653	648	0.25%	0.025%
52	17.114	2308	2311	2313	rVB	365	366	0.14%	0.014%
53	17.184	2319	2323	2325	rBV	311	390	0.15%	0.015%
54	17.266	2332	2337	2339	rBV2	673	681	0.26%	0.026%
55	17.519	2379	2380	2382	rBV	477	378	0.15%	0.014%
56	17.595	2388	2393	2396	rBV3	993	1163	0.45%	0.044%
57	17.736	2409	2417	2423	rBV	172888	255934	99.11%	9.711%
58	17.830	2427	2433	2443	rVV2	131963	199116	77.11%	7.555%
59	18.054	2470	2471	2477	rVB	401	470	0.18%	0.018%
60	18.171	2489	2491	2493	rBV	942	802	0.31%	0.030%
61	18.283	2508	2510	2512	rBV	601	563	0.22%	0.021%
62	18.365	2523	2524	2527	rBV	542	612	0.24%	0.023%
63	18.477	2541	2543	2546	rVB	661	479	0.19%	0.018%
64	18.582	2559	2561	2562	rBV	654	427	0.17%	0.016%
65	18.653	2570	2573	2576	rVB3	1357	1558	0.60%	0.059%
66	18.682	2576	2578	2580	rBV2	561	571	0.22%	0.022%
67	18.735	2585	2587	2591	rVB	403	544	0.21%	0.021%
68	19.058	2638	2642	2643	rBV	492	508	0.20%	0.019%
69	19.088	2643	2647	2652	rVB4	3842	5291	2.05%	0.201%
70	19.134	2652	2655	2658	rBV3	843	1481	0.57%	0.056%
71	19.205	2665	2667	2670	rBV	539	514	0.20%	0.020%
72	19.234	2670	2672	2674	rVB2	669	511	0.20%	0.019%
73	19.311	2683	2685	2688	rVB	1412	1006	0.39%	0.038%
74	19.340	2688	2690	2691	rVB	664	401	0.16%	0.015%
75	19.358	2691	2693	2694	rBV2	898	853	0.33%	0.032%
76	19.469	2708	2712	2715	rBV2	2019	2730	1.06%	0.104%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
 Data File : BG057271.D
 Acq On : 2 May 2023 9:36
 Operator : CG/JU
 Sample : 02418-08
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW8Z4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

77	19.516	2718	2720	2723	rVB	845	990	0.38%	0.038%
78	19.546	2723	2725	2726	rBV	541	409	0.16%	0.016%
79	19.563	2726	2728	2729	rBV2	565	334	0.13%	0.013%
80	19.593	2731	2733	2734	rBV	941	471	0.18%	0.018%
81	19.763	2759	2762	2765	rBV2	3751	4609	1.78%	0.175%
82	19.792	2765	2767	2771	rVV2	2789	2768	1.07%	0.105%
83	19.881	2781	2782	2784	rVB2	1051	534	0.21%	0.020%
84	19.963	2794	2796	2799	rBV3	1117	1308	0.51%	0.050%
85	20.004	2801	2803	2805	rVB3	1673	1259	0.49%	0.048%
86	20.039	2805	2809	2812	rBV3	2729	4345	1.68%	0.165%
87	20.098	2812	2819	2827	rBV	87018	127821	49.50%	4.850%
88	20.262	2845	2847	2849	rBV3	2090	1656	0.64%	0.063%
89	20.568	2896	2899	2903	rBV4	3919	4953	1.92%	0.188%
90	21.073	2982	2985	2987	rBV3	4647	4689	1.82%	0.178%
91	21.608	3072	3076	3078	rBV5	6719	9455	3.66%	0.359%
92	22.048	3144	3151	3160	rBV2	148284	258227	100.00%	9.798%
93	25.320	3702	3708	3717	rVB2	28443	76277	29.54%	2.894%
94	25.573	3742	3751	3763	rVB3	77954	240509	93.14%	9.126%




Sum of corrected areas: 2635555

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
Data File : BG057271.D
Acq On : 2 May 2023 9:36
Operator : CG/JU
Sample : 02418-08
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW8Z4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

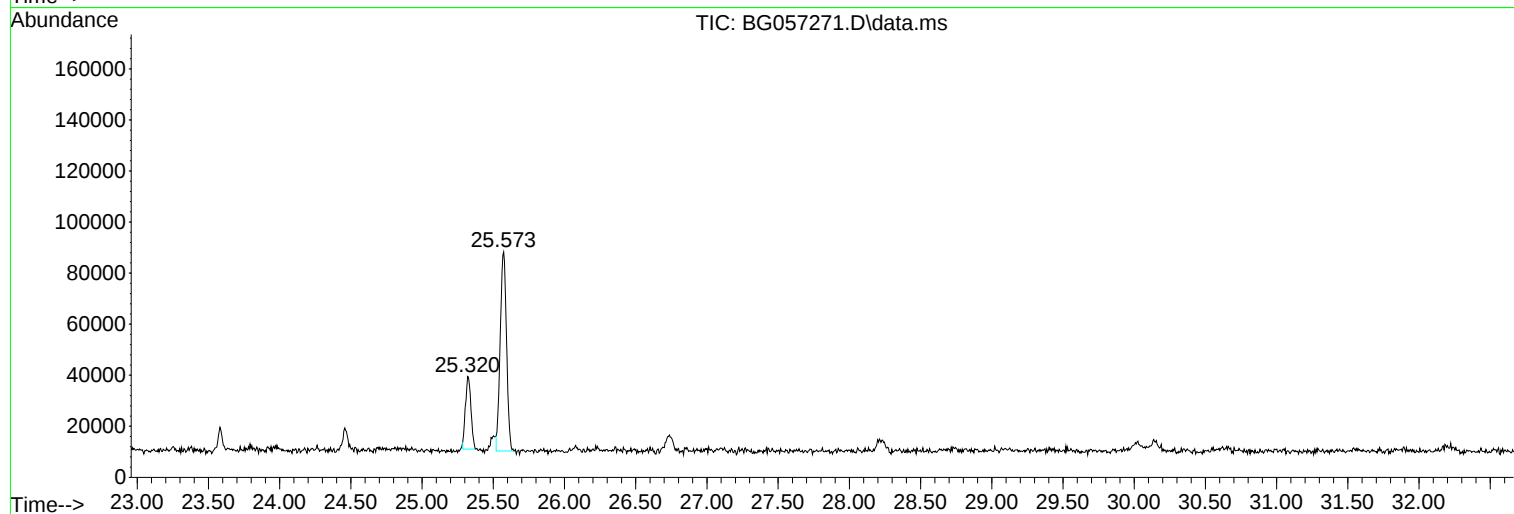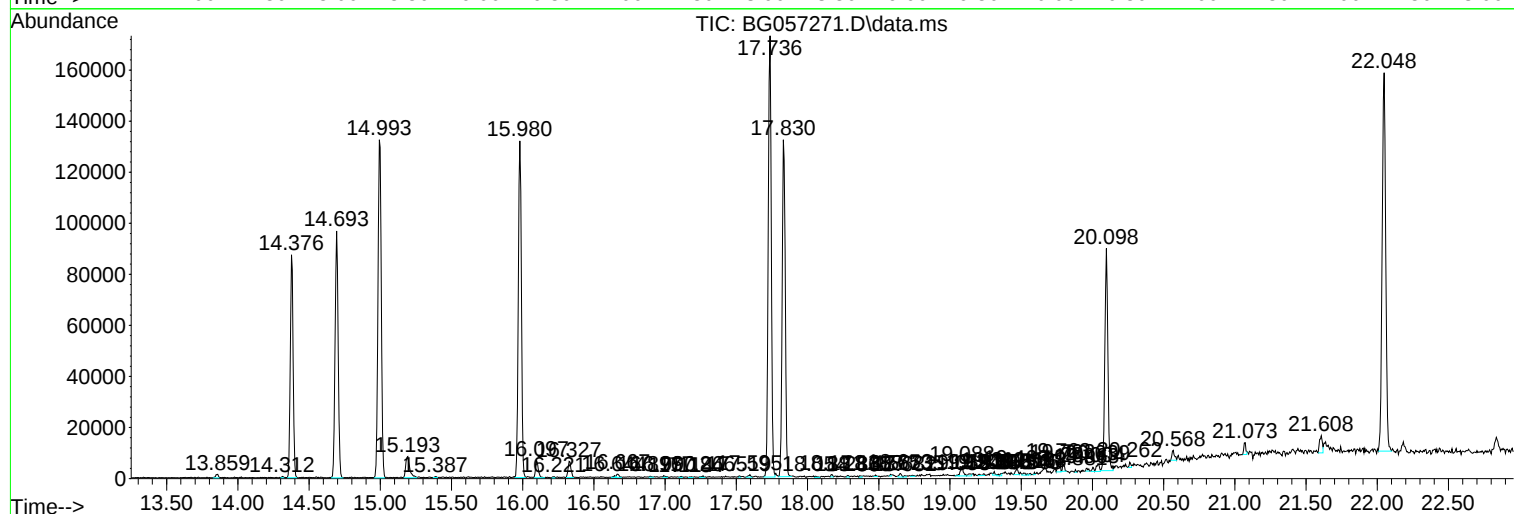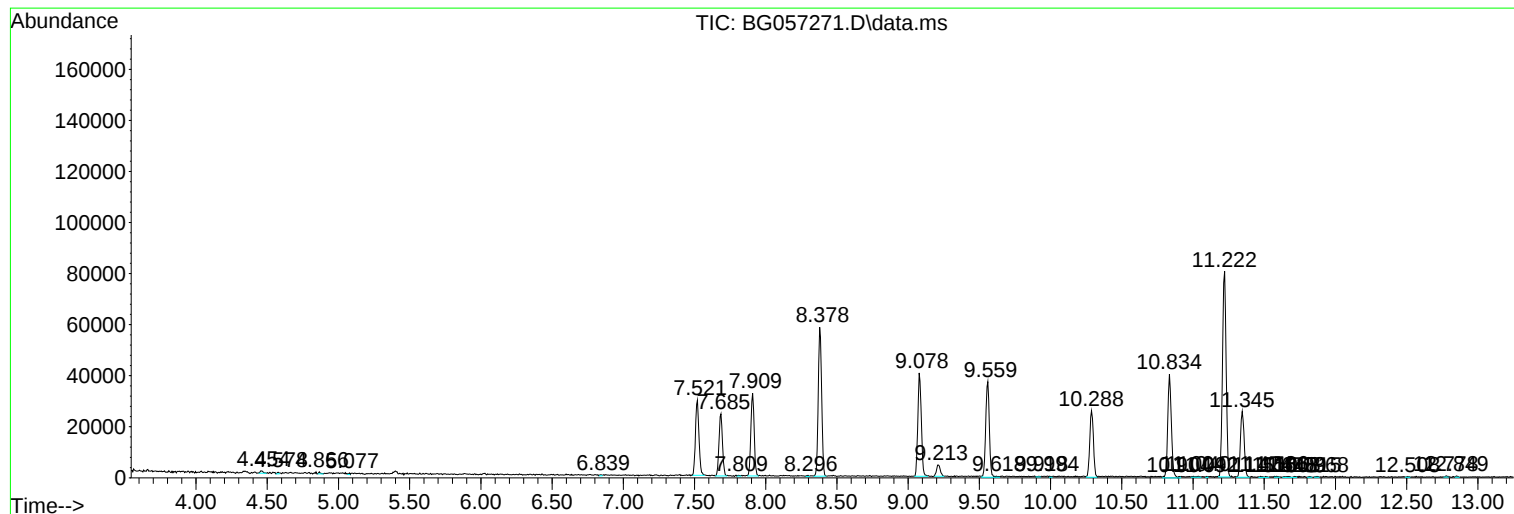

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
Data File : BG057271.D
Acq On : 2 May 2023 9:36
Operator : CG/JU
Sample : 02418-08
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW8Z4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050123\
Data File : BG057271.D
Acq On : 2 May 2023 9:36
Operator : CG/JU
Sample : 02418-08
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW8Z4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc