
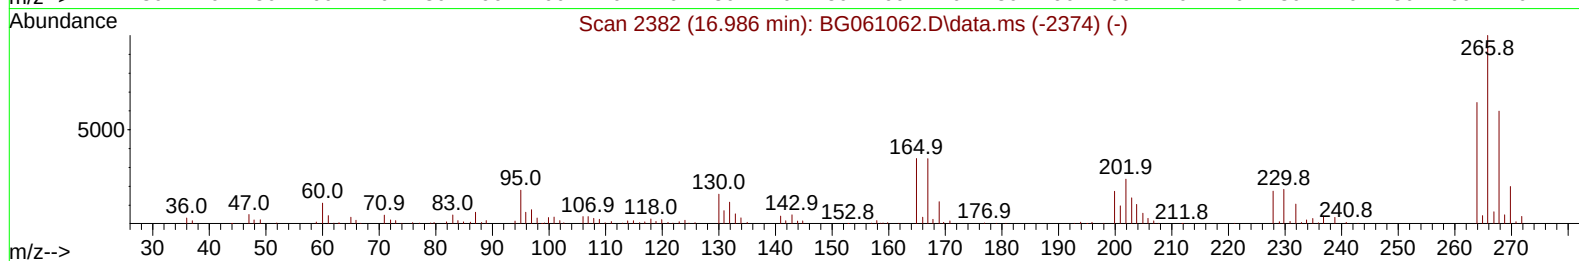
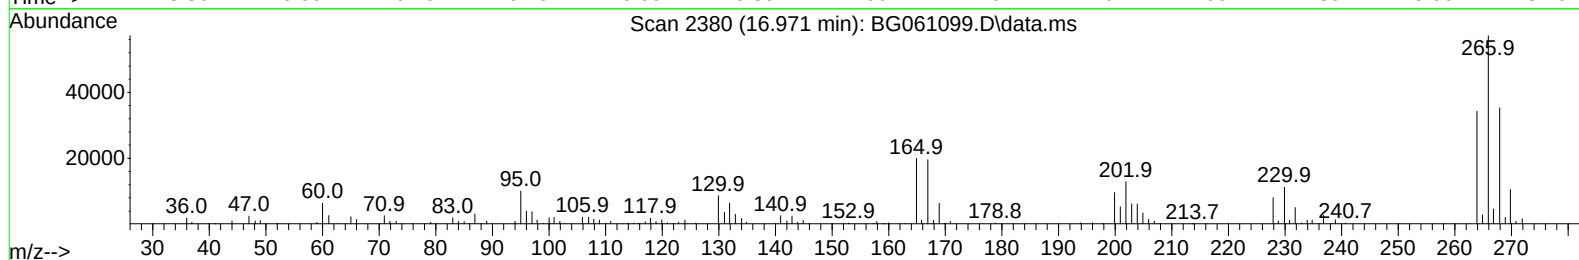


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050324\
Data File : BG061099.D
Acq On : 3 May 2024 9:39
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 03 11:29:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

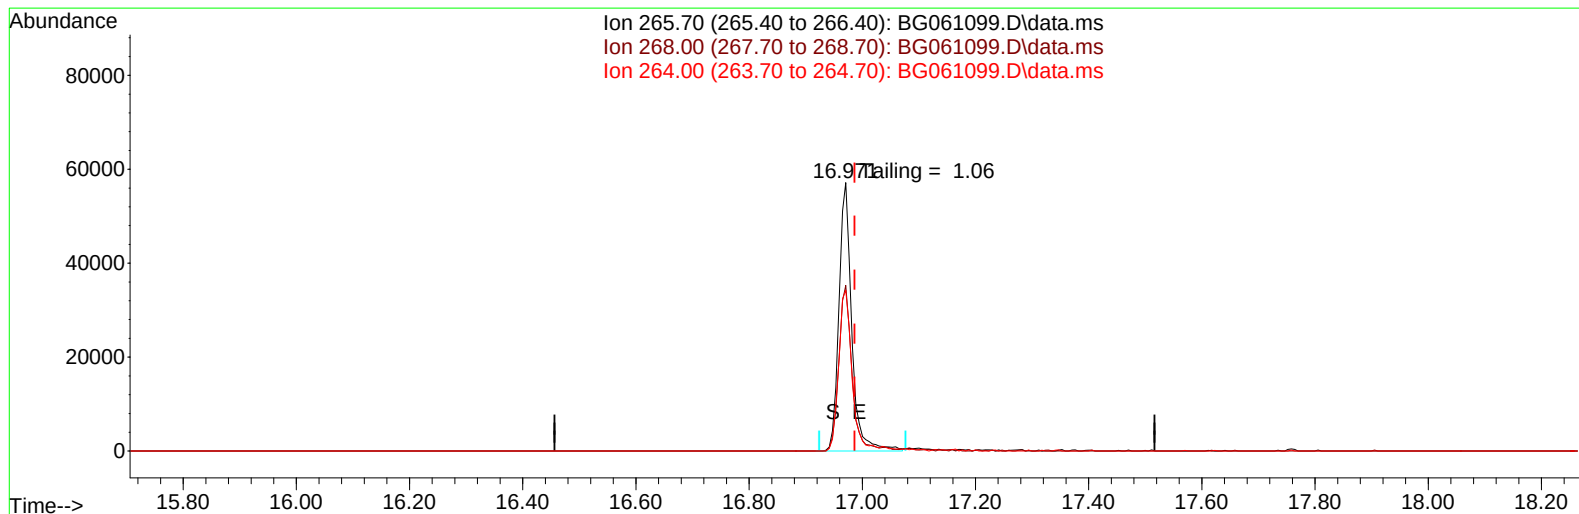

TIC: BG061099.D\data.ms

(70) Pentachlorophenol (C)




16.971min (-0.015) 17445.55 ng

response 90201

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.80	61.70
264.00	64.40	59.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050324\
Data File : BG061099.D
Acq On : 3 May 2024 9:39
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 03 11:29:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

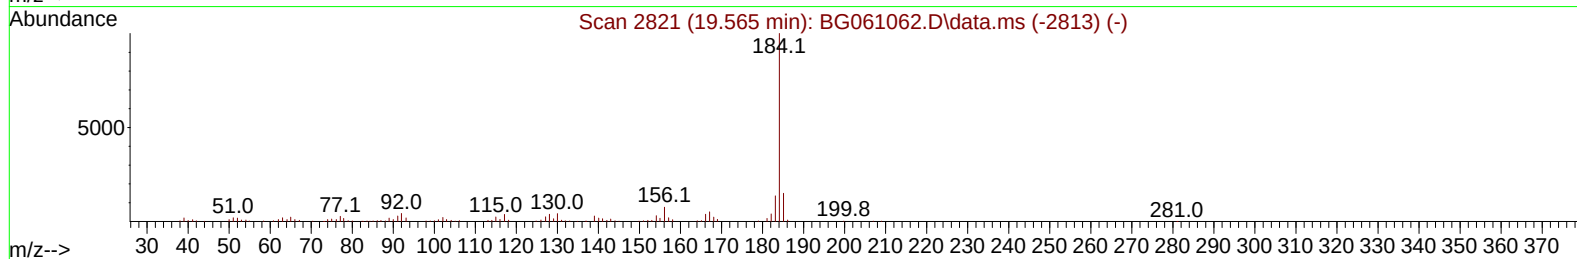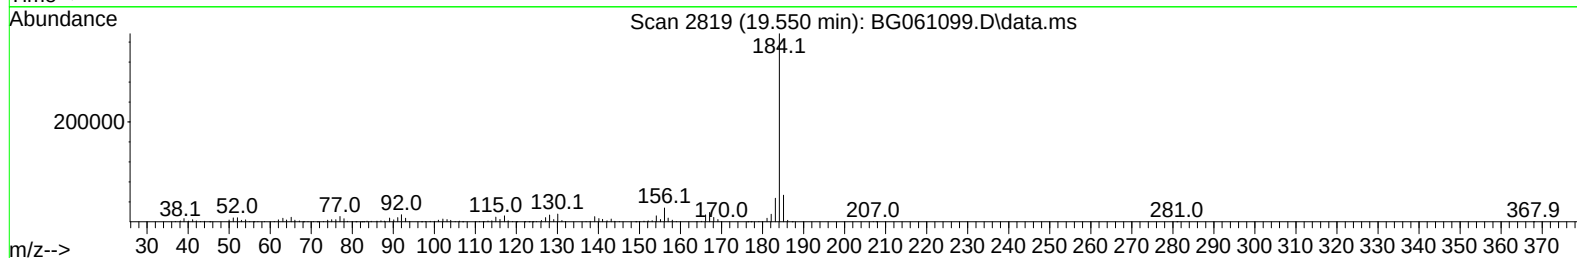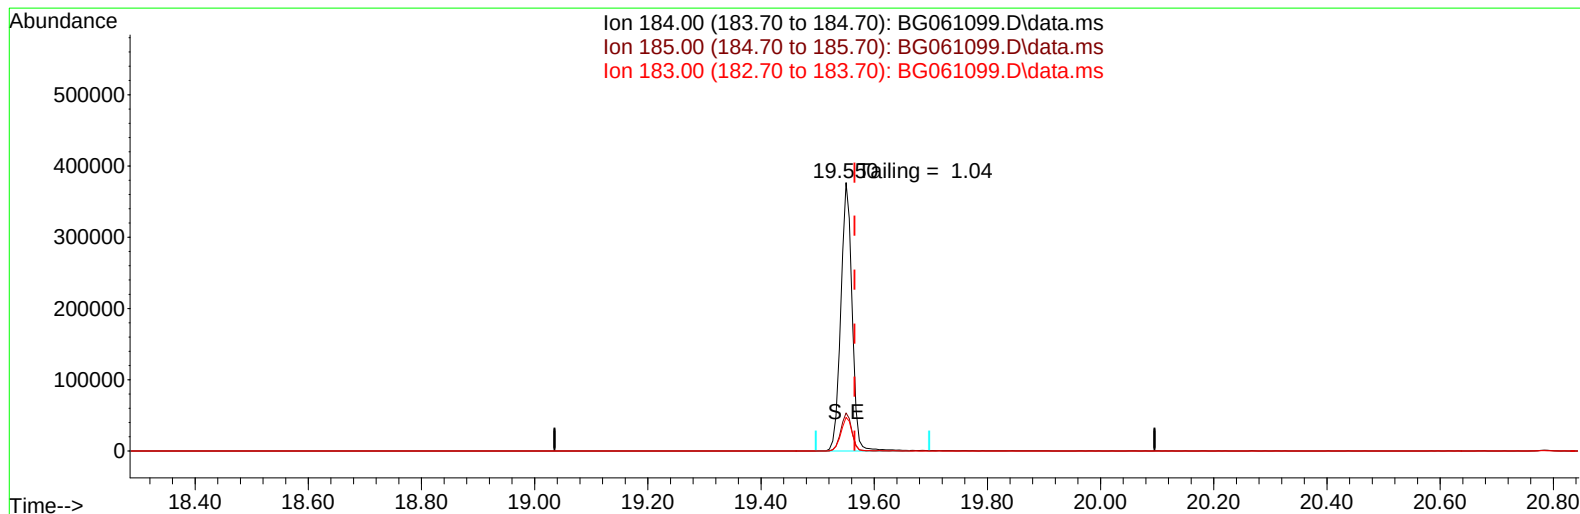

TIC: BG061099.D\data.ms

(77) Benzidine

19.550min (-0.015) 377801.49 ng m

response 519096

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.19
183.00	13.60	12.53
0.00	0.00	0.00