

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050324\
Data File : BG061101.D
Acq On : 3 May 2024 11:02
Operator : MA/JU
Sample : PB160665BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB160665BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG061101.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.533	426	433	442	rVB	387826	609363	23.08%	7.219%
2	7.114	694	702	712	rBV	400954	666707	25.25%	7.898%
3	7.937	837	842	848	rVB	70313	116530	4.41%	1.381%
4	9.094	1032	1039	1048	rVB	249243	428883	16.25%	5.081%
5	10.733	1308	1318	1326	rBV	90223	154334	5.85%	1.828%
6	13.189	1729	1736	1748	rBV	689208	1053438	39.90%	12.480%
7	14.564	1962	1970	1978	rBV	153606	242009	9.17%	2.867%
8	16.056	2216	2224	2240	rBV	734632	1133102	42.92%	13.424%
9	17.314	2432	2438	2445	rBV	246239	367857	13.93%	4.358%
10	19.934	2878	2884	2891	rVB	2076259	2639989	100.00%	31.276%
11	21.568	3155	3162	3168	rBV2	311386	520732	19.72%	6.169%
12	24.699	3686	3695	3706	rVB	178094	508068	19.25%	6.019%




Sum of corrected areas: 8441012

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050324\
Data File : BG061101.D
Acq On : 3 May 2024 11:02
Operator : MA/JU
Sample : PB160665BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB160665BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

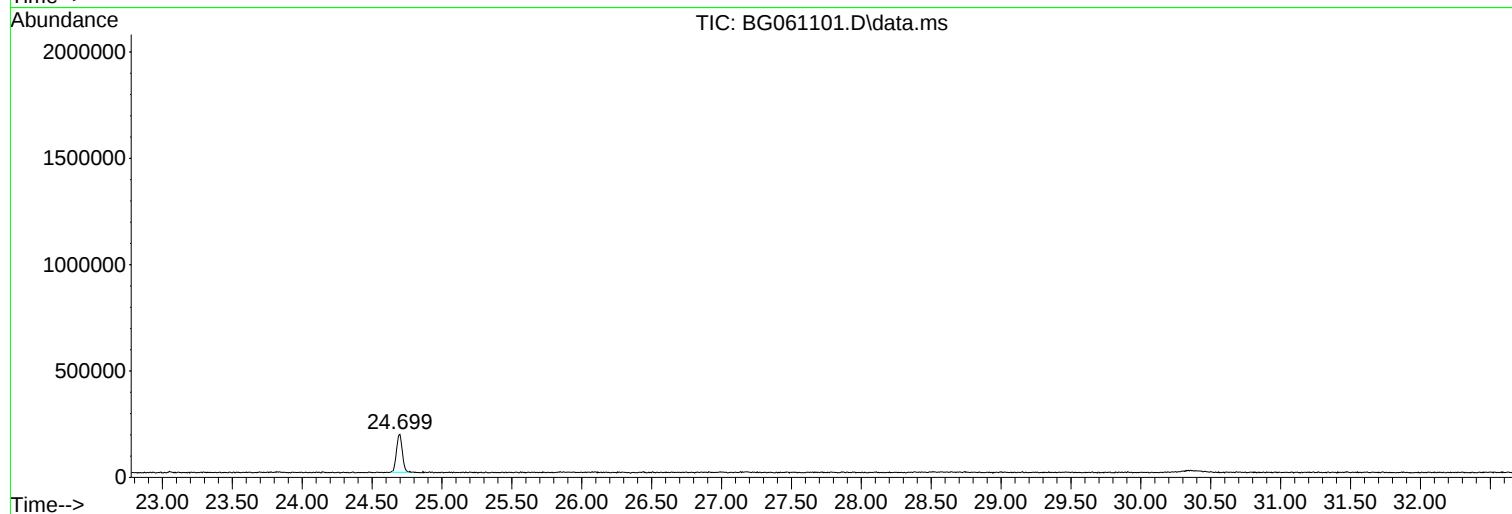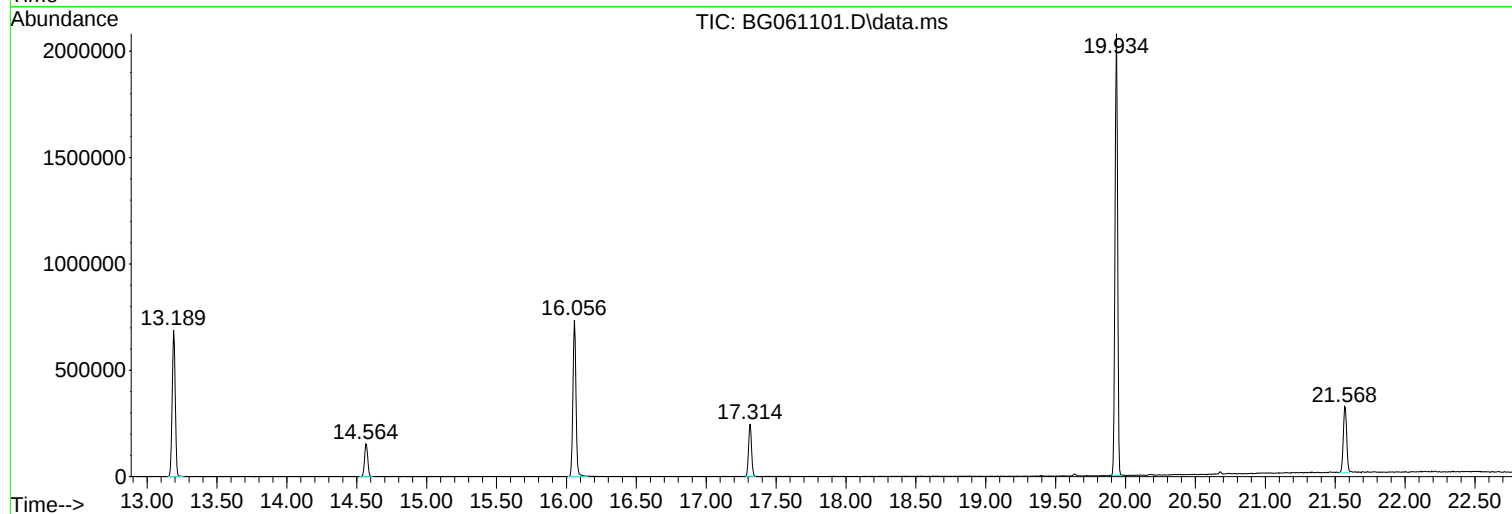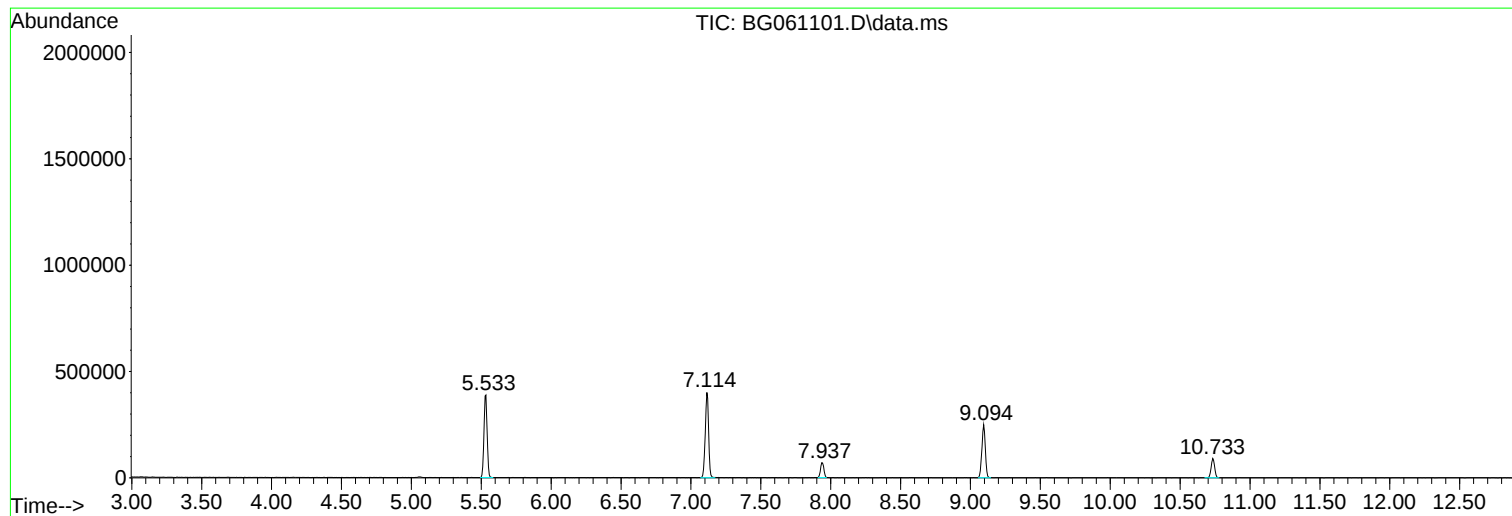

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050324\
Data File : BG061101.D
Acq On : 3 May 2024 11:02
Operator : MA/JU
Sample : PB160665BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB160665BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050324\
Data File : BG061101.D
Acq On : 3 May 2024 11:02
Operator : MA/JU
Sample : PB160665BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB160665BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------