


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050324\
Data File : BG061099.D
Acq On : 3 May 2024 9:39
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 01 05:11:25 2024

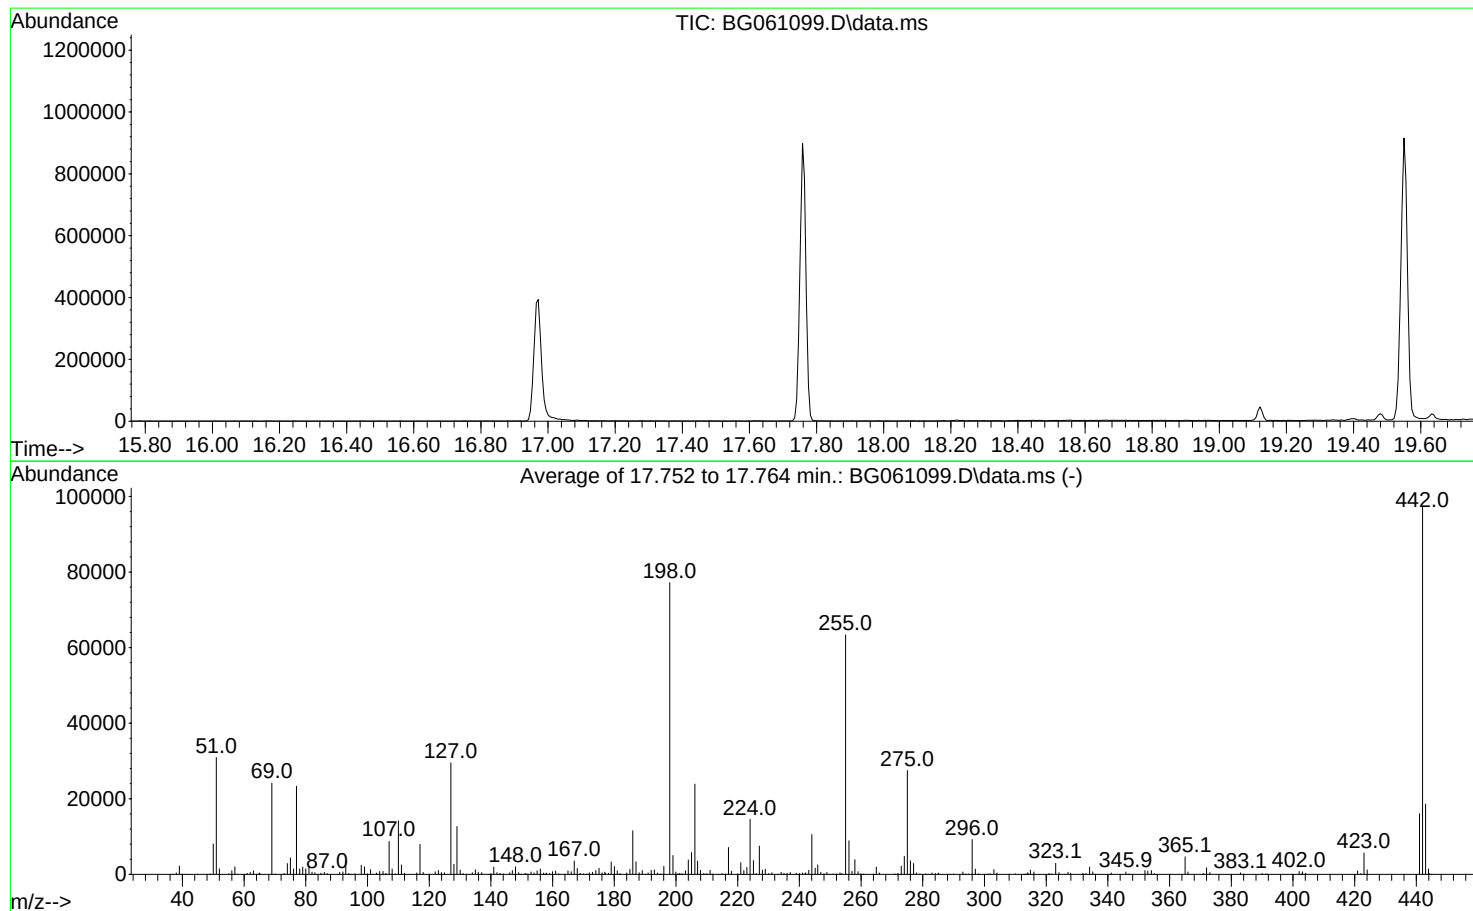

AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	30931	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.3	24120	PASS
70	69	0.00	2	0.5	114	PASS
127	198	10	80	38.3	29525	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	77176	PASS
199	198	5	9	6.5	4988	PASS
275	198	10	60	35.6	27499	PASS
365	198	1	100	6.1	4673	PASS
441	198	0.01	100	20.8	16050	PASS
442	442	50	100	100.0	97341	PASS
443	442	15	24	19.1	18571	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/3/2024	BNA_G	<u>BG061099.D</u>
Compound Name	Response	Retention Time
DDT	324072	20.784
DDD	8410	20.349
DDE	62	19.48
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8472	332544	2.55

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050324\
Data File : BG061099.D
Acq On : 3 May 2024 9:39
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 03 11:29:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

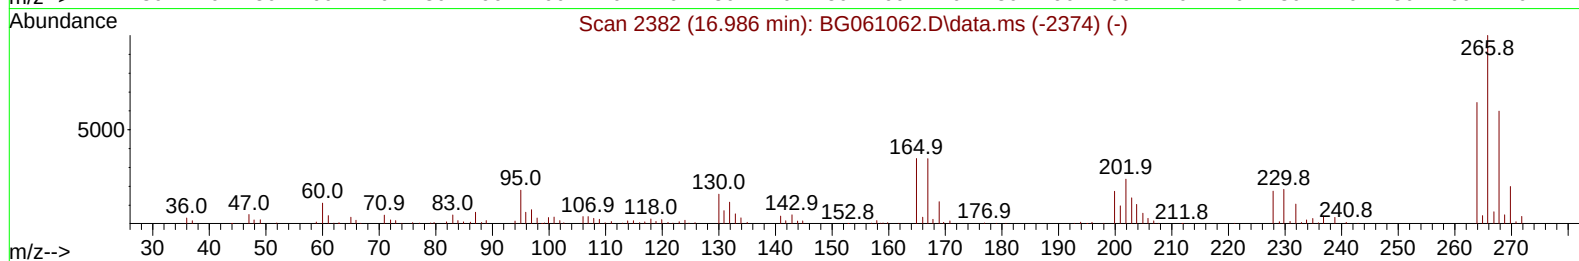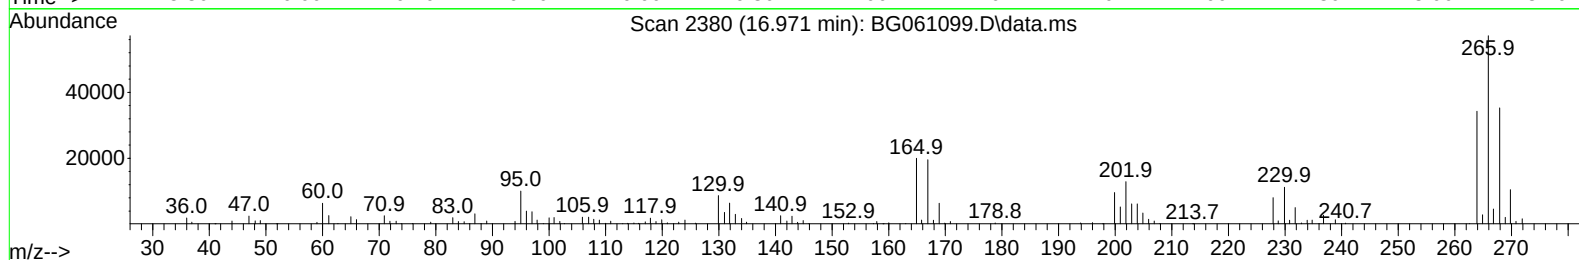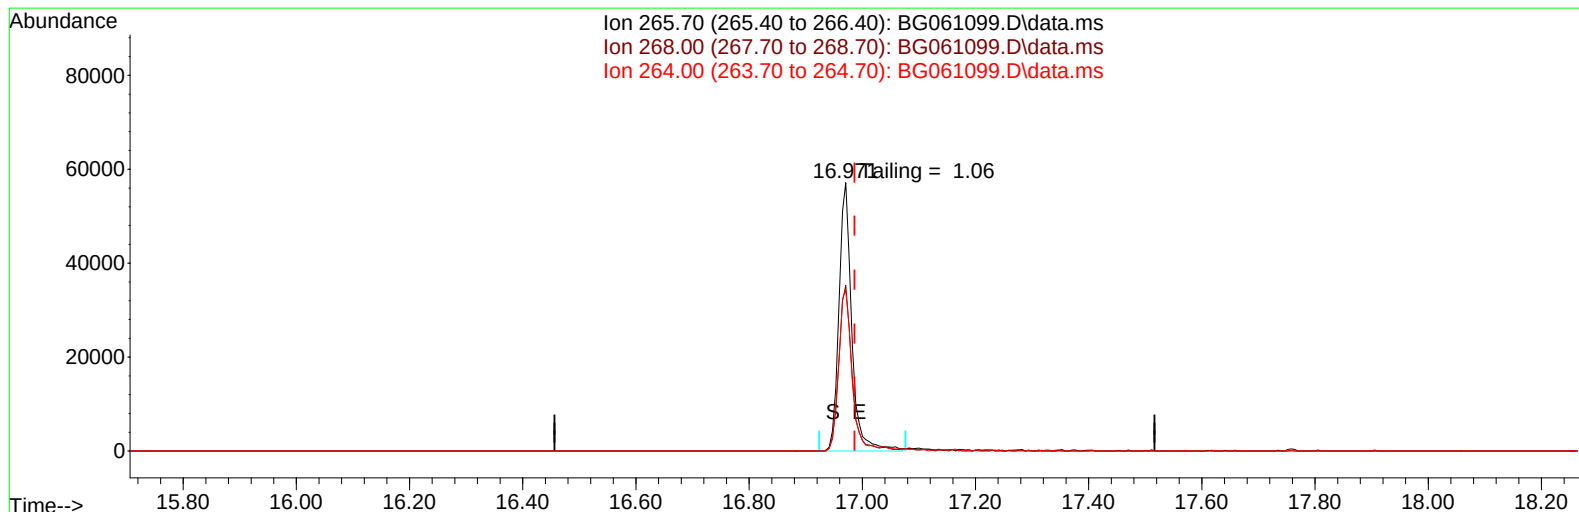

TIC: BG061099.D\data.ms

(70) Pentachlorophenol (C)

16.971min (-0.015) 17445.55 ng




response 90201

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.80	61.70
264.00	64.40	59.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050324\
Data File : BG061099.D
Acq On : 3 May 2024 9:39
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 03 11:29:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

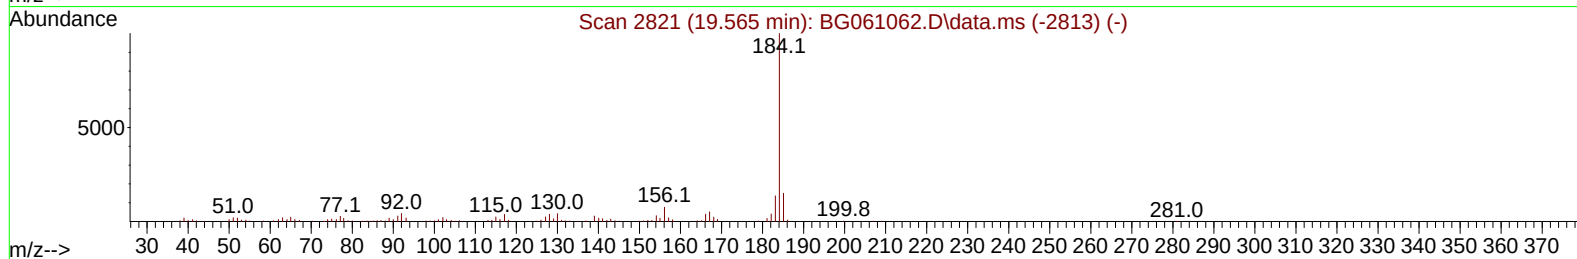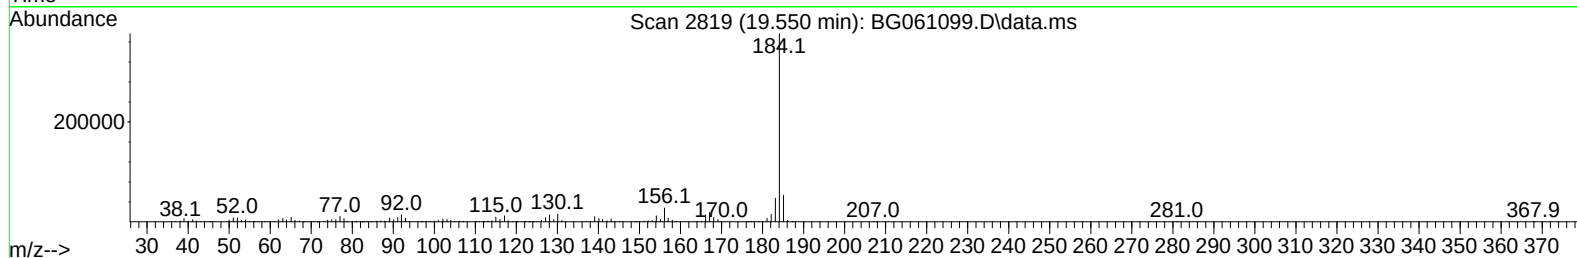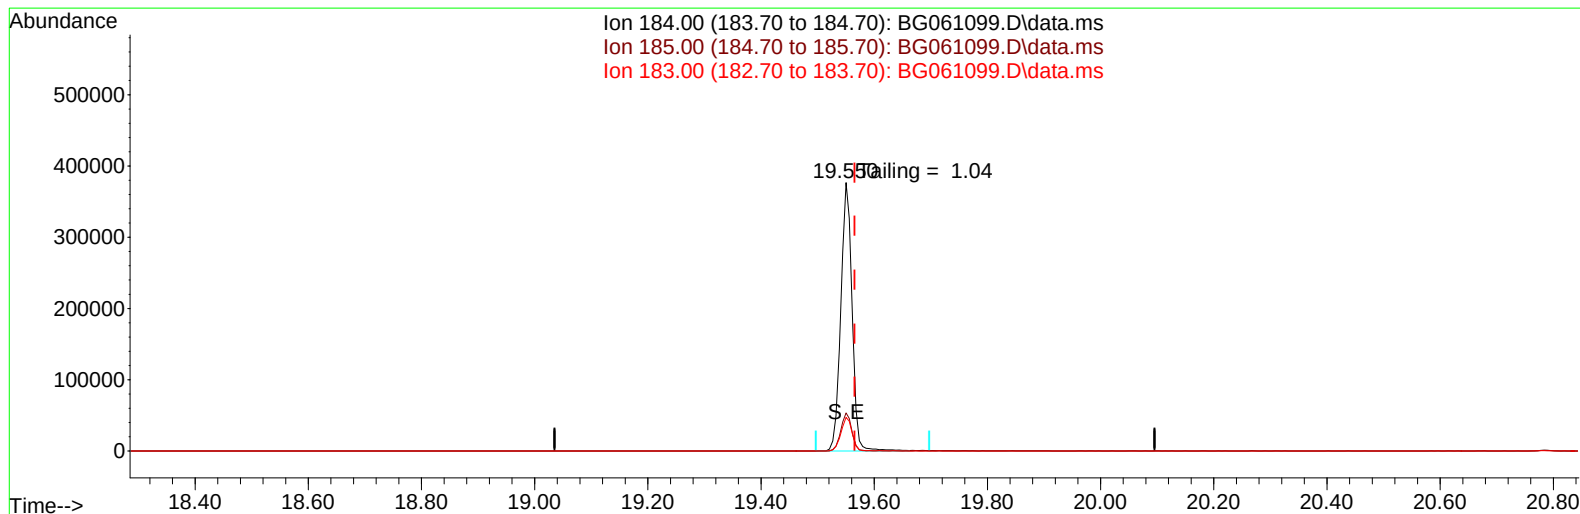

TIC: BG061099.D\data.ms

(77) Benzidine

19.550min (-0.015) 377801.49 ng m

response 519096

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.19
183.00	13.60	12.53
0.00	0.00	0.00