
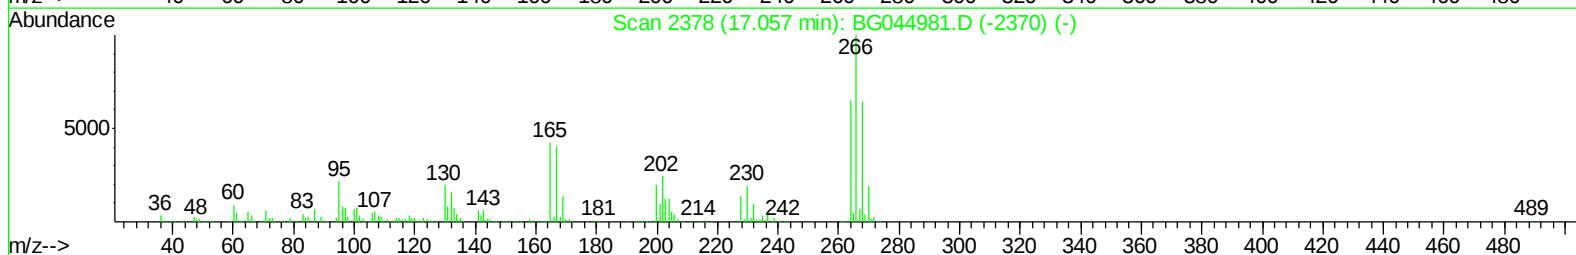
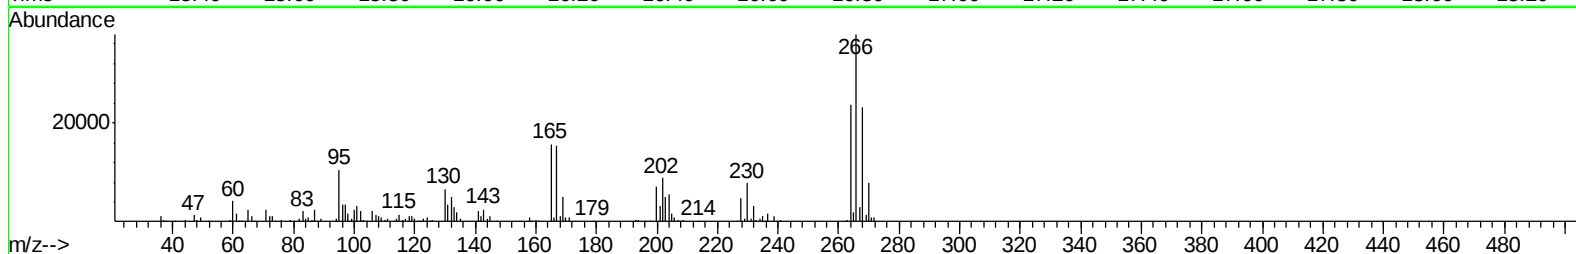


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG050420\
 Data File : BG045230.D
 Acq On : 4 May 2020 11:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 05 02:50:52 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 04 13:03:14 2020
 Response via : Initial Calibration

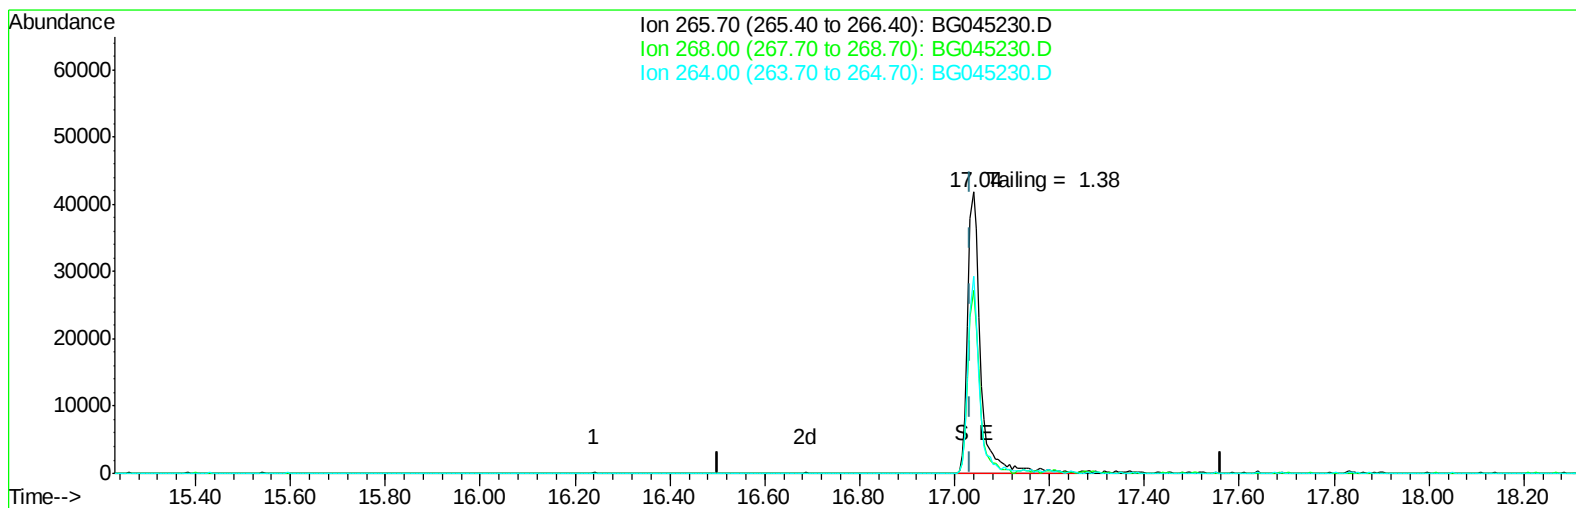




TIC: BG045230.D

(70) Pentachlorophenol (C)
 16.240min (-0.793) 110.31ng
 response 67

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	0.00#
264.00	65.30	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG050420\
 Data File : BG045230.D
 Acq On : 4 May 2020 11:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 05 02:50:52 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 04 13:03:14 2020
 Response via : Initial Calibration

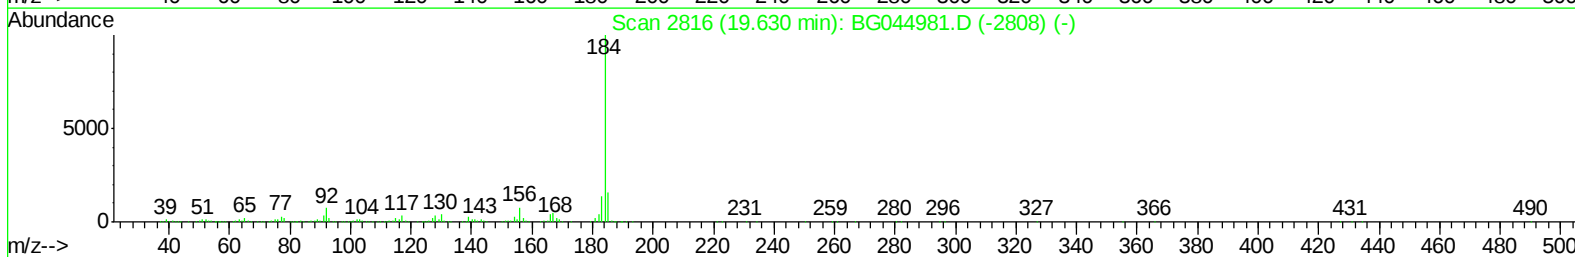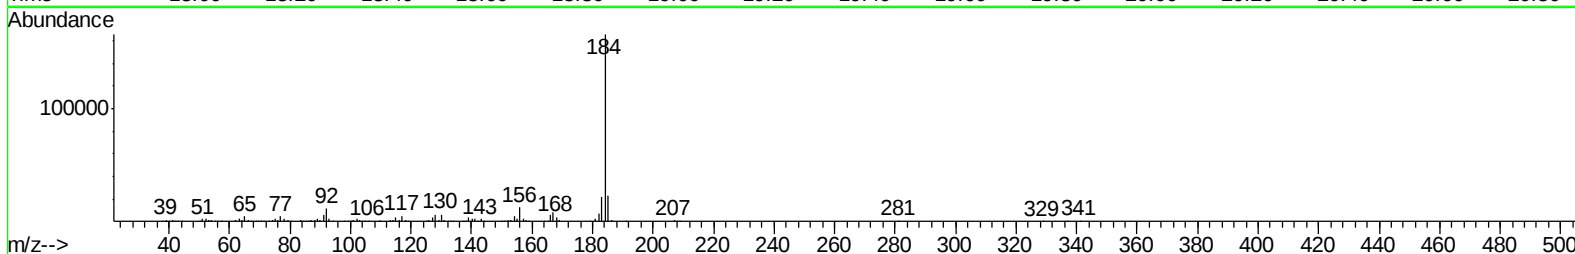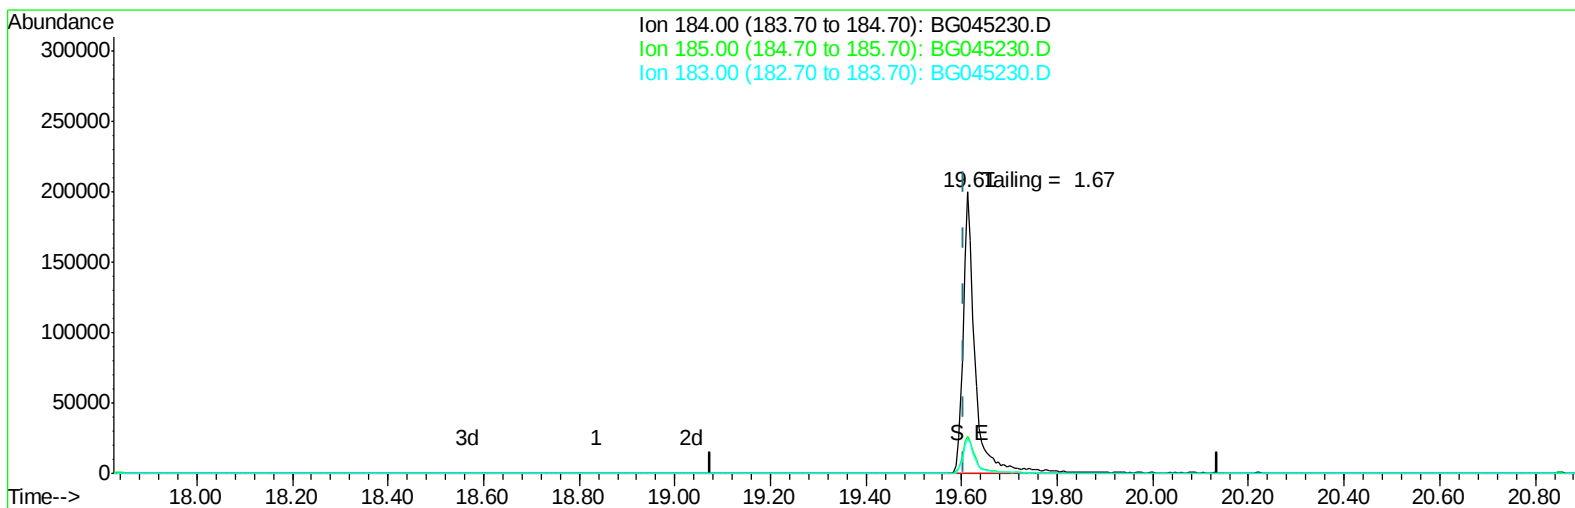

TIC: BG045230.D

(77) Benzidine

18.837min (-0.769) -6.19ng

response 56

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	0.00#
183.00	14.10	0.00#
0.00	0.00	0.00