


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG050420\
 Data File : BG045230.D
 Acq On : 4 May 2020 11:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 04 13:03:14 2020

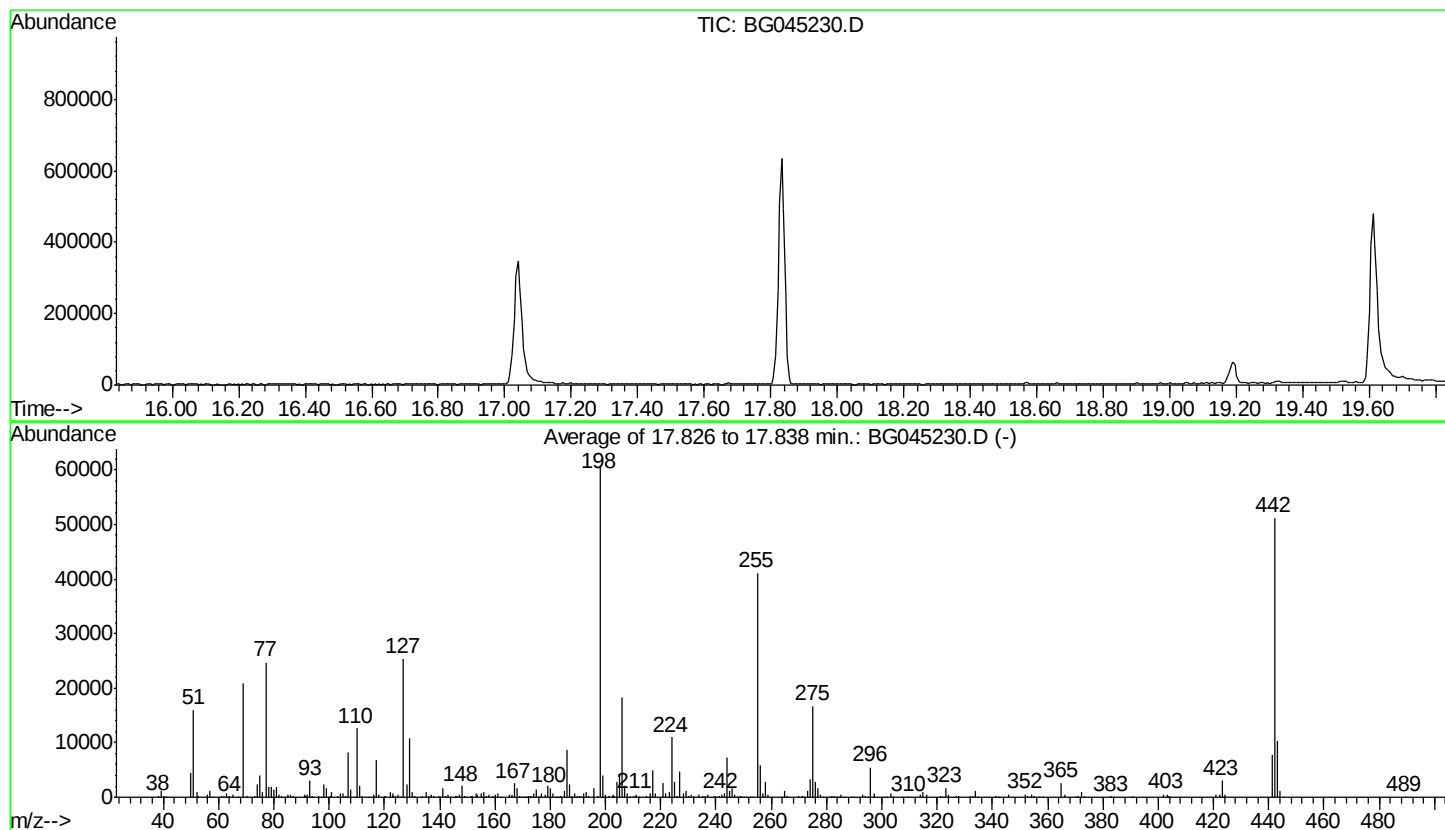

AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2502

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.4	16033	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.4	20910	PASS
70	69	0.00	2	0.7	150	PASS
127	198	10	80	41.9	25442	PASS
197	198	0.00	2	0.3	189	PASS
198	198	100	100	100.0	60776	PASS
199	198	5	9	6.5	3947	PASS
275	198	10	60	27.5	16710	PASS
365	198	1	100	4.3	2612	PASS
441	198	0.01	100	12.8	7800	PASS
442	198	50	100	84.2	51160	PASS
443	442	15	24	20.0	10239	PASS