
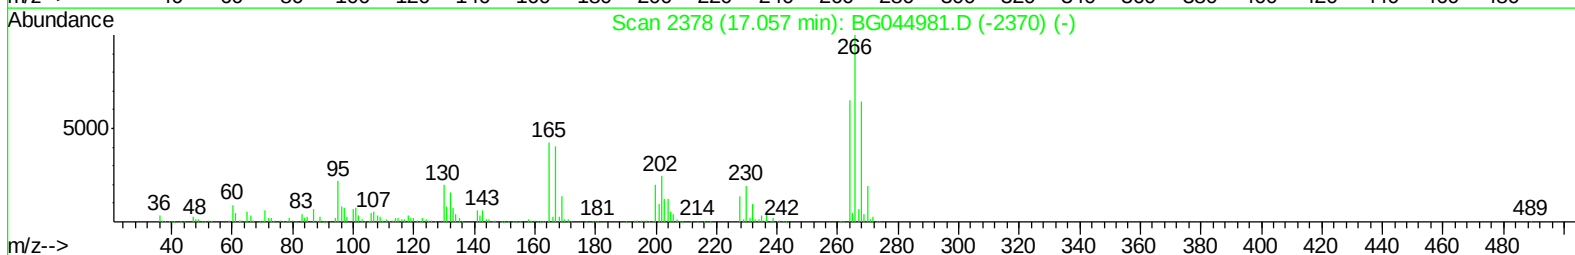
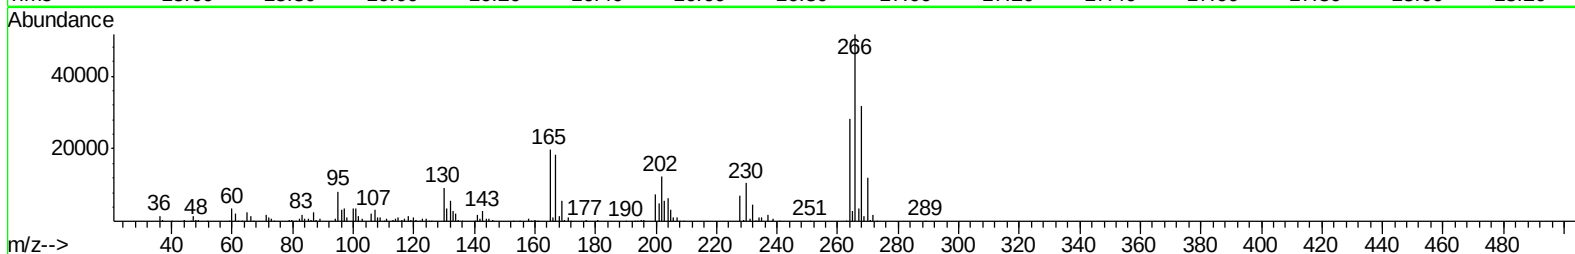


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG050620\
 Data File : BG045248.D
 Acq On : 6 May 2020 11:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 07 01:49:26 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 06 12:59:59 2020
 Response via : Initial Calibration

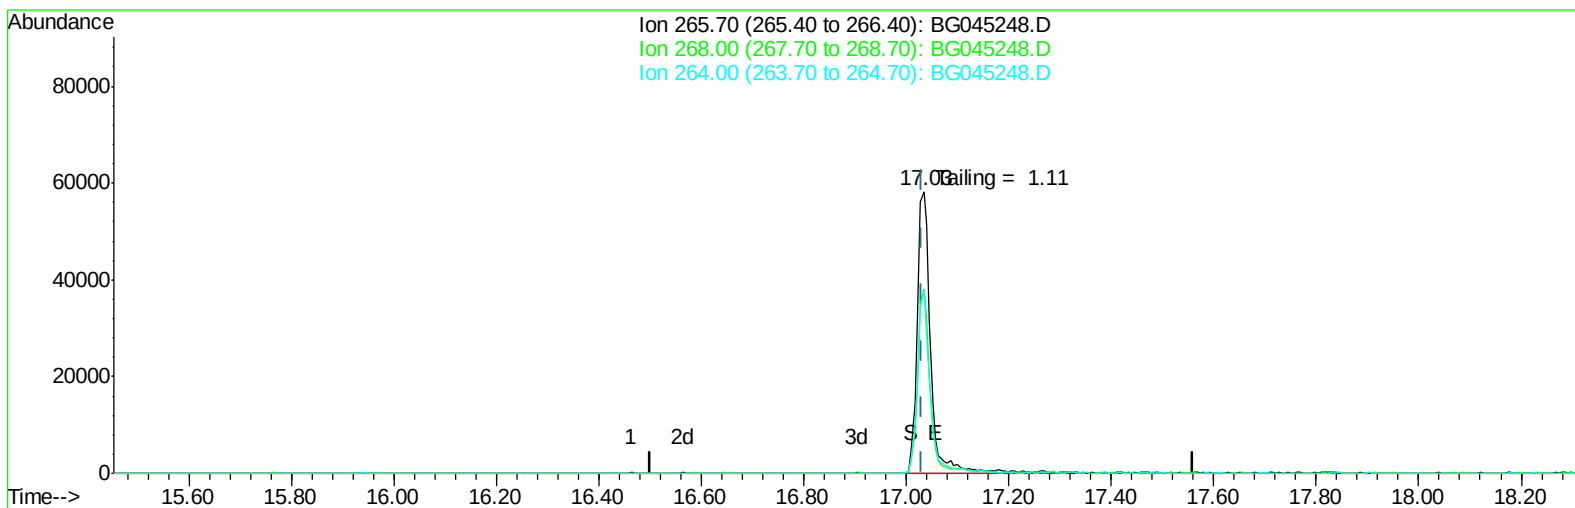

TIC: BG045248.D

(70) Pentachlorophenol (C)




16.464min (-0.567) 197.25ng

response 102

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	0.00#
264.00	65.30	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG050620\
 Data File : BG045248.D
 Acq On : 6 May 2020 11:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 07 01:49:26 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 06 12:59:59 2020
 Response via : Initial Calibration

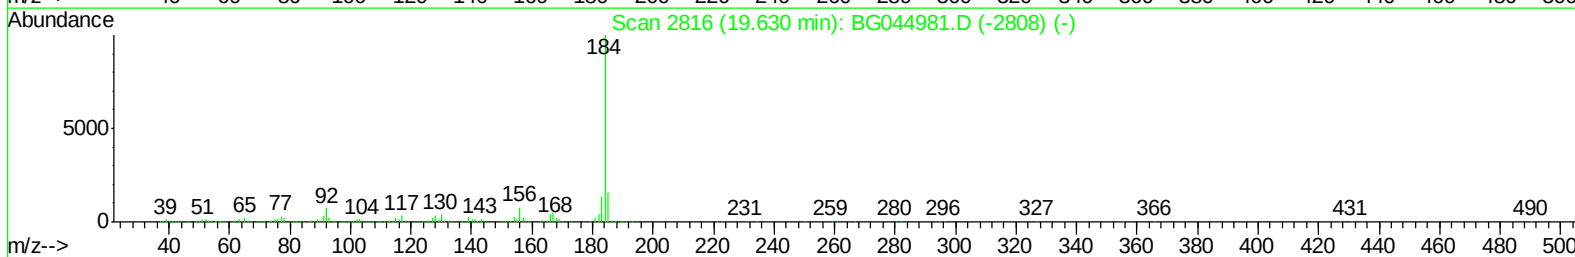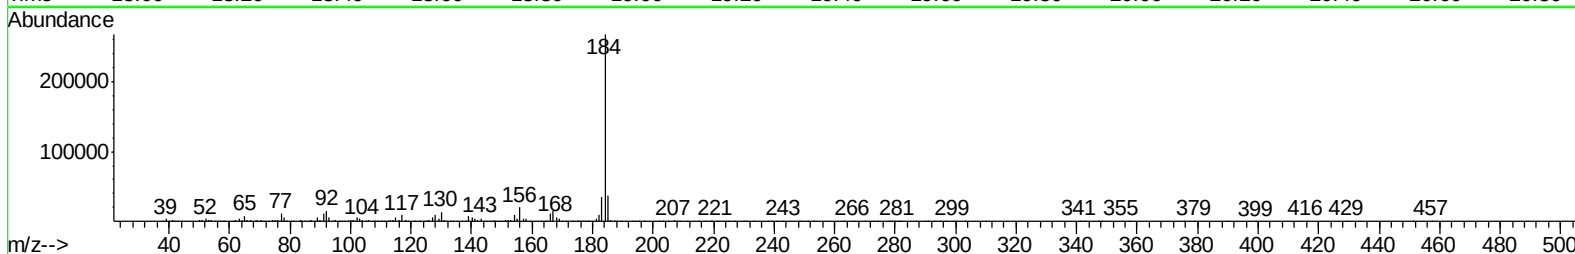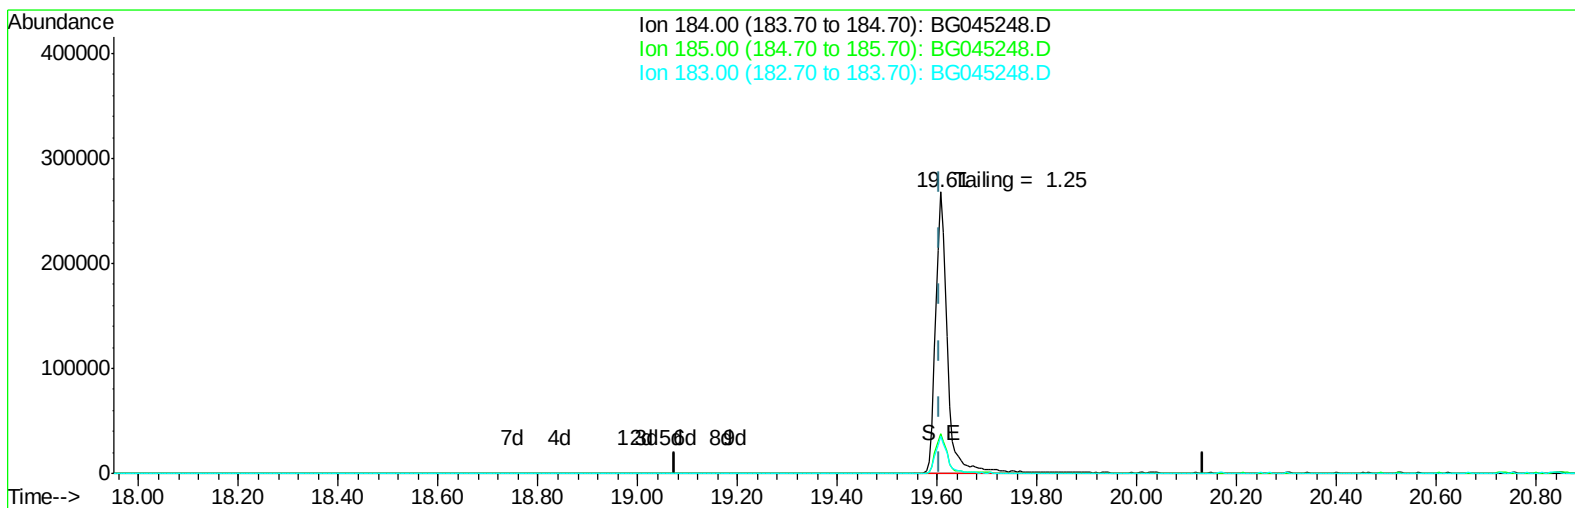

TIC: BG045248.D

(77) Benzidine

18.972min (-0.632) 1.34ng

response 115

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	0.00#
183.00	14.10	0.00#
0.00	0.00	0.00