

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG050620\
 Data File : BG045251.D
 Acq On : 6 May 2020 13:39
 Operator : CG/JU
 Sample : PB128675BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB128675BL

Quant Time: May 06 14:33:39 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 06 12:59:59 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.98	152	57058	20.00	ng	0.00
21) Naphthalene-d8	10.79	136	217880	20.00	ng	0.00
39) Acenaphthene-d10	14.63	164	157725	20.00	ng	0.00
64) Phenanthrene-d10	17.37	188	396988	20.00	ng	0.00
76) Chrysene-d12	21.64	240	390401	20.00	ng	0.00
87) Perylene-d12	24.81	264	402828	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.55	112	429579	124.30	ng	0.00
7) Phenol-d6	7.14	99	605328	117.89	ng	0.00
23) Nitrobenzene-d5	9.14	82	428857	89.81	ng	0.00
42) 2,4,6-Tribromophenol	16.11	330	339063	139.15	ng	0.00
45) 2-Fluorobiphenyl	13.25	172	1022424	95.05	ng	0.00
79) Terphenyl-d14	19.99	244	1887397	105.37	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG050620\
Data File : BG045251.D
Acq On : 6 May 2020 13:39
Operator : CG/JU
Sample : PB128675BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB128675BL

Quant Time: May 06 14:33:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 06 12:59:59 2020
Response via : Initial Calibration

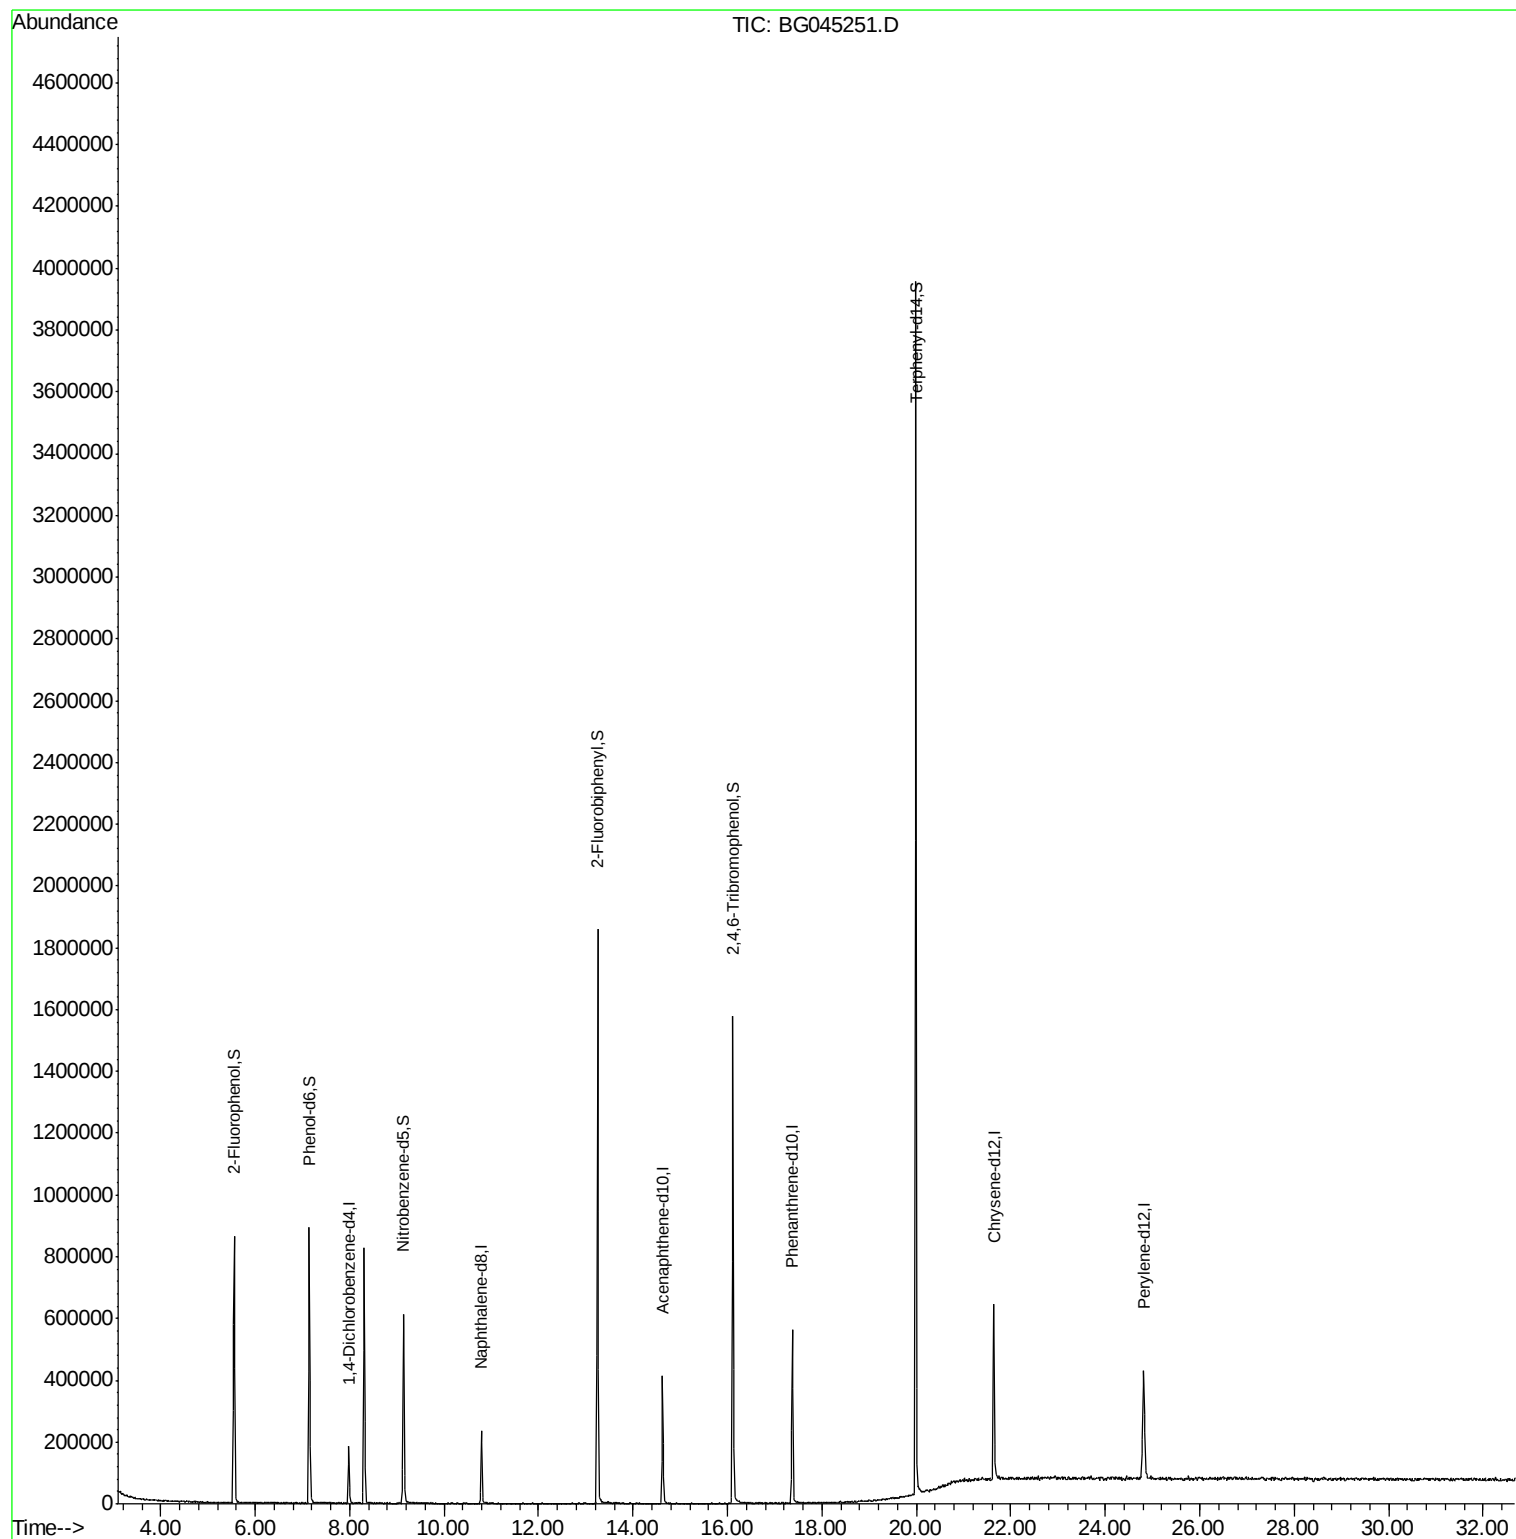

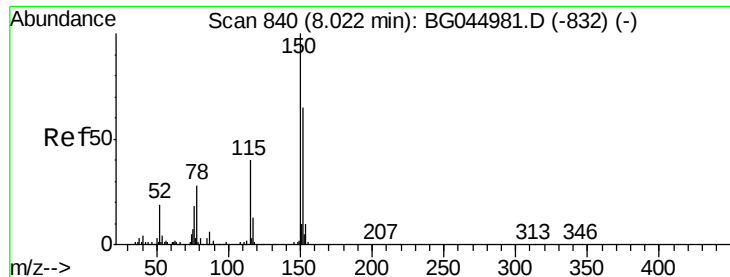


#1


1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.98 min Scan# 833
Delta R.T. -0.00 min
Lab File: BG045251.D
Acq: 6 May 2020 13:39

Instrument :
BNA_G
ClientSampleId :
PB128675BL



Tot Ion:152 Resp: 57058
Ion Ratio Lower Upper
152 100
150 157.7 123.6 185.4
115 55.7 49.1 73.7

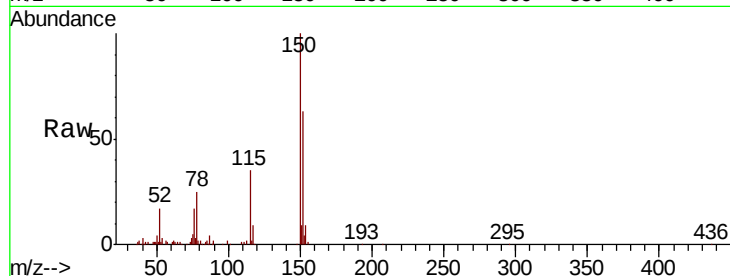

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

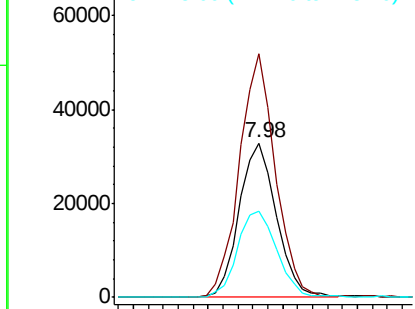


Time-->

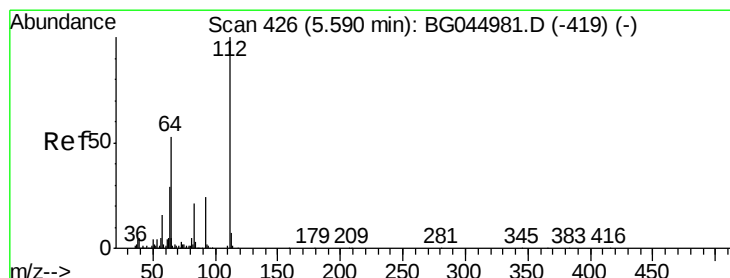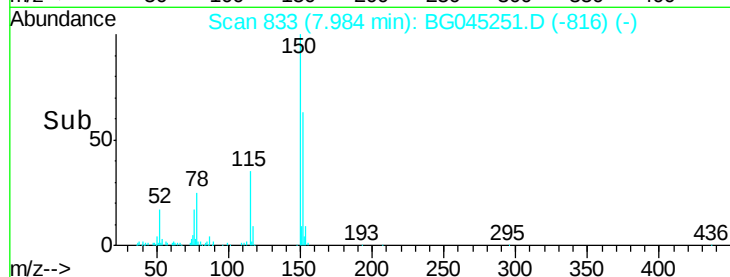


#5

2-Fluorophenol
Concen: 124.297 ng
RT: 5.55 min Scan# 419
Delta R.T. -0.00 min
Lab File: BG045251.D
Acq: 6 May 2020 13:39


Tgt Ion:112 Resp: 429579
Ion Ratio Lower Upper
112 100
64 57.0 42.4 63.6
63 31.4 23.1 34.7

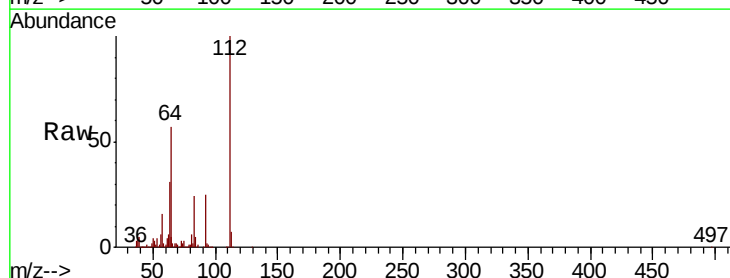

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

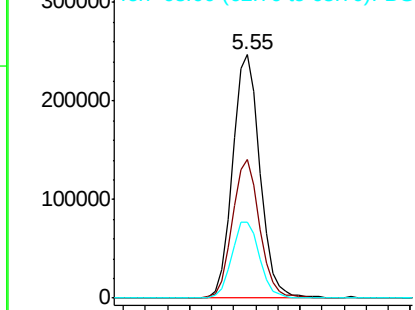

Time-->

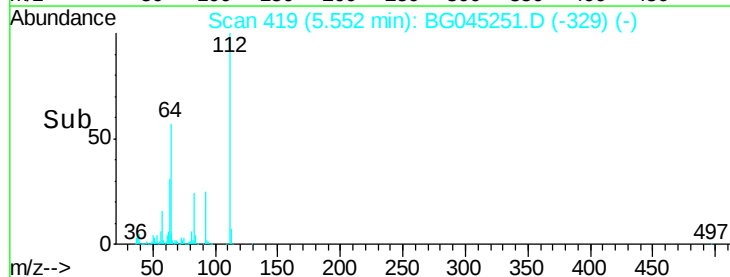



#7

Phenol-d6

Concen: 117.886 ng

RT: 7.14 min Scan# 690

Delta R.T. -0.01 min

Lab File: BG045251.D

Acq: 6 May 2020 13:39

Instrument :

BNA_G

ClientSampleId :

PB128675BL


Tot Ion: 99 Resp: 605328

Ion Ratio Lower Upper




99 100

42 14.0 11.3 16.9

71 37.4 28.3 42.5

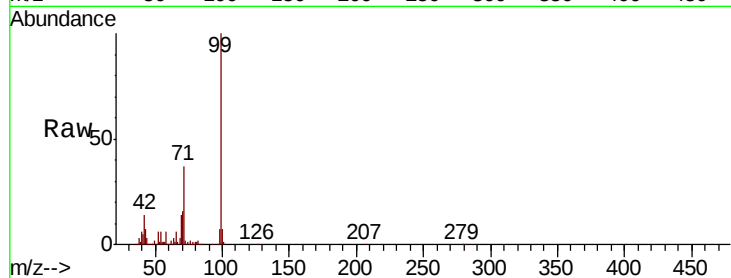

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

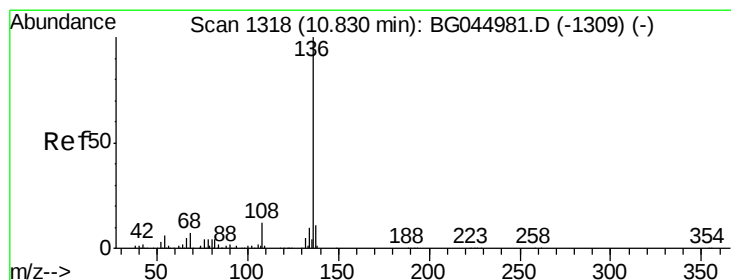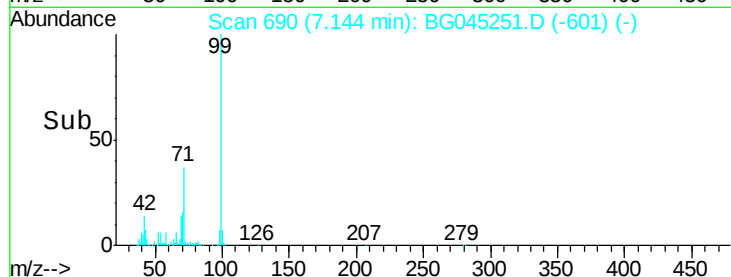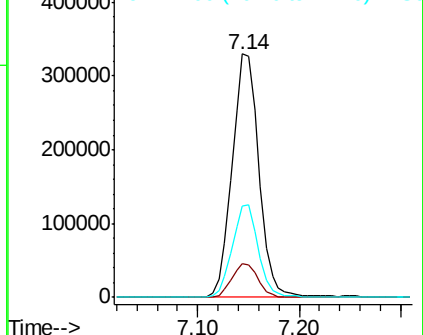

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.79 min Scan# 1311

Delta R.T. -0.00 min

Lab File: BG045251.D

Acq: 6 May 2020 13:39

Tgt Ion: 136 Resp: 217880


Ion Ratio Lower Upper

136 100



137 12.2 8.6 13.0

54 5.7 4.8 7.2

68 5.1 5.2 7.8#

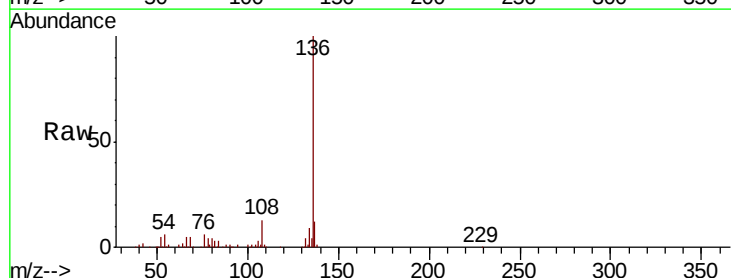

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

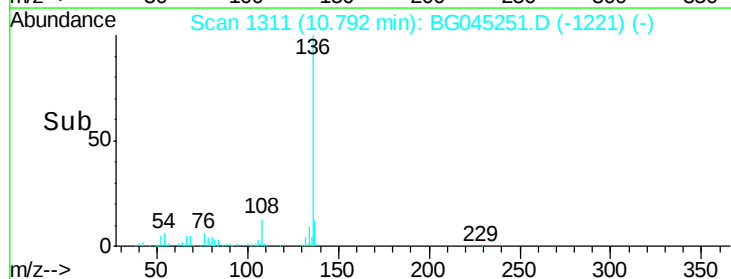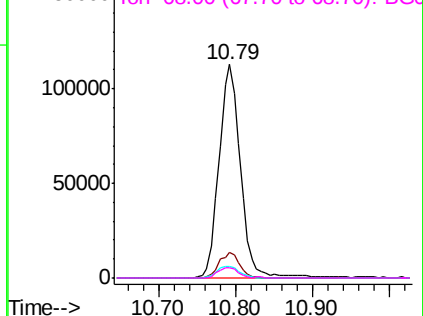




#23
 Nitrobenzene-d5
 Concen: 89.812 ng
 RT: 9.14 min Scan# 1030
 Delta R.T. -0.00 min
 Lab File: BG045251.D
 Acq: 6 May 2020 13:39

Instrument :
 BNA_G
 ClientSampleID :
 PB128675BL




Tot Ion	82	Resp	428857
Ion Ratio	Lower	Upper	
82	100		
128	40.9	33.0	49.4
54	39.0	30.4	45.6

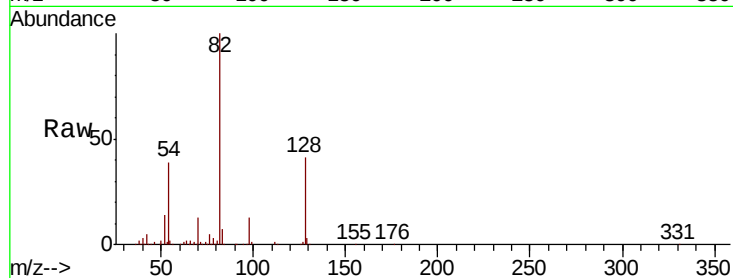

Abundance Ion 82.00 (81.70 to 82.70): BG044981.D (-1030) (-)


Ion 128.00 (127.70 to 128.70): BG044981.D (-1030) (-)

Ion 54.00 (53.70 to 54.70): BG044981.D (-1030) (-)

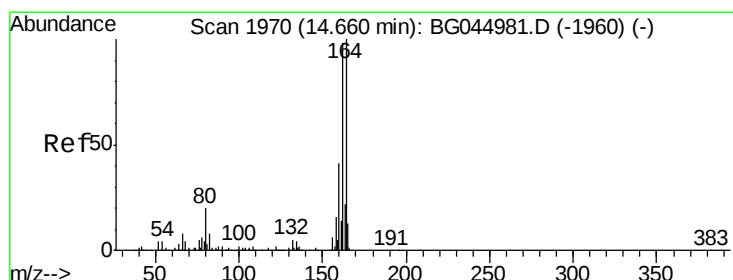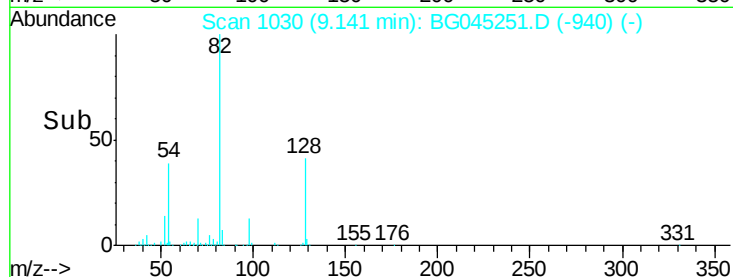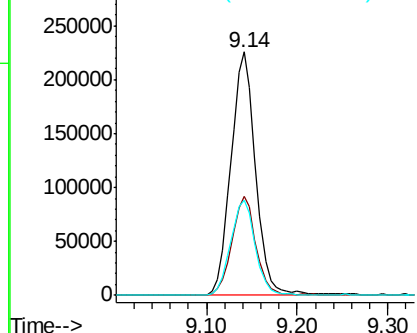

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.63 min Scan# 1964
 Delta R.T. -0.00 min
 Lab File: BG045251.D
 Acq: 6 May 2020 13:39



Tgt Ion	164	Resp	157725
Ion Ratio	Lower	Upper	
164	100		
162	96.6	78.7	118.1
160	43.6	32.8	49.2

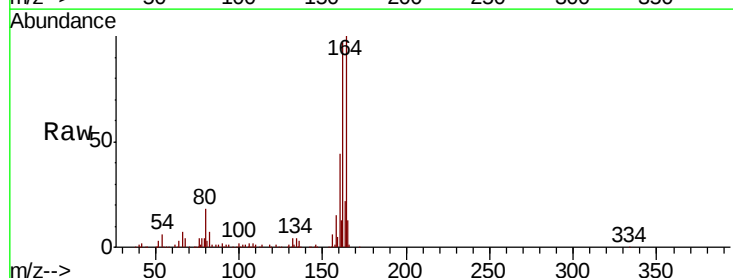

Abundance Ion 164.00 (163.70 to 164.70): BG044981.D (-1960) (-)

Ion 162.00 (161.70 to 162.70): BG044981.D (-1960) (-)

Ion 160.00 (159.70 to 160.70): BG044981.D (-1960) (-)



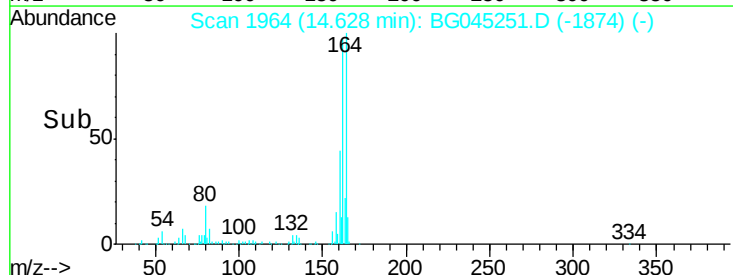
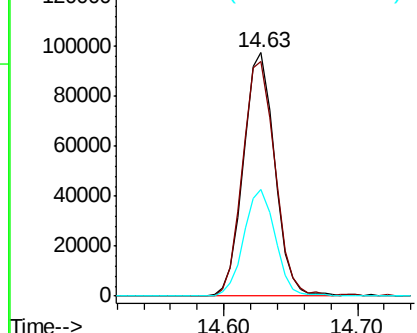




#42
 2,4,6-Tribromophenol
 Concen: 139.152 ng
 RT: 16.11 min Scan# 2217
 Delta R.T. -0.01 min
 Lab File: BG045251.D
 Acq: 6 May 2020 13:39




Instrument :
 BNA_G
 ClientSampleId :
 PB128675BL


Tot Ion	Ratio	Lower	Upper
330	100		
332	95.2	79.1	118.7
141	35.3	27.1	40.7

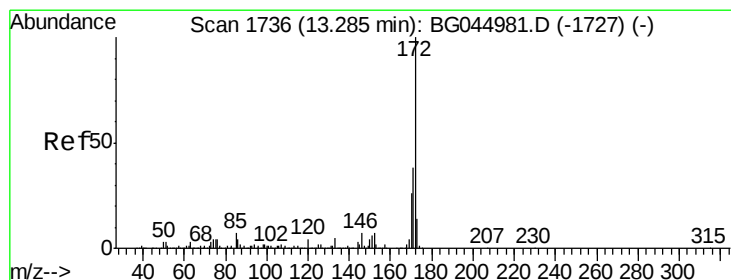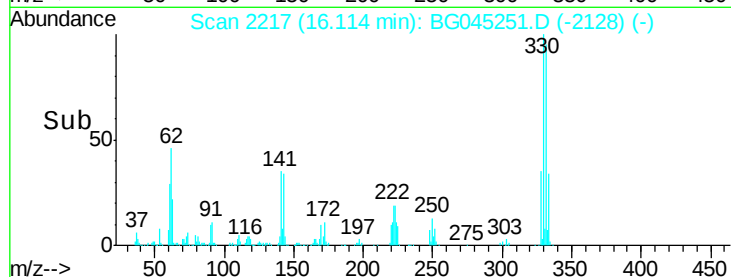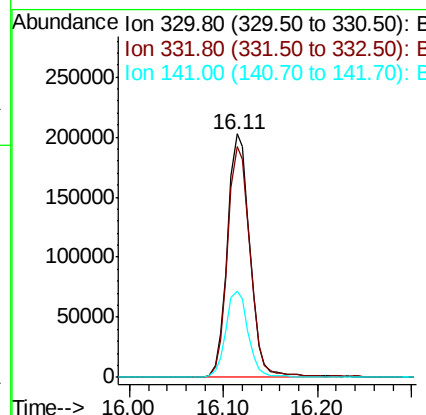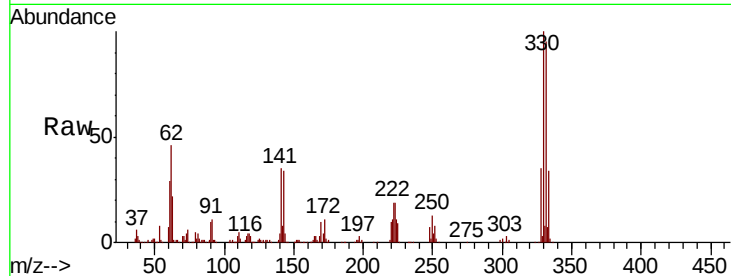

#45
 2-Fluorobiphenyl
 Concen: 95.051 ng
 RT: 13.25 min Scan# 1729
 Delta R.T. -0.00 min
 Lab File: BG045251.D
 Acq: 6 May 2020 13:39

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.4	30.6	46.0
170	24.1	20.5	30.7

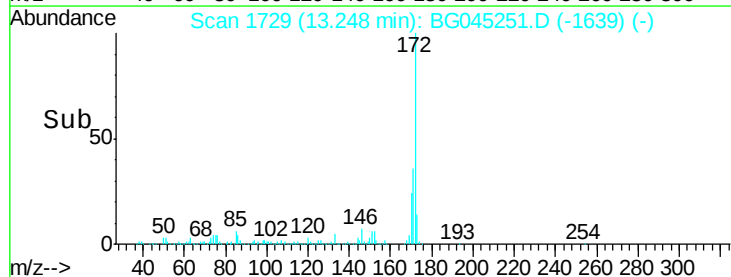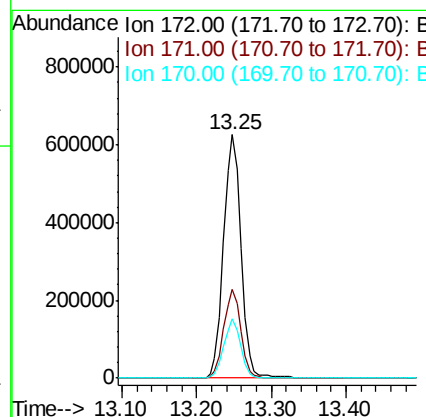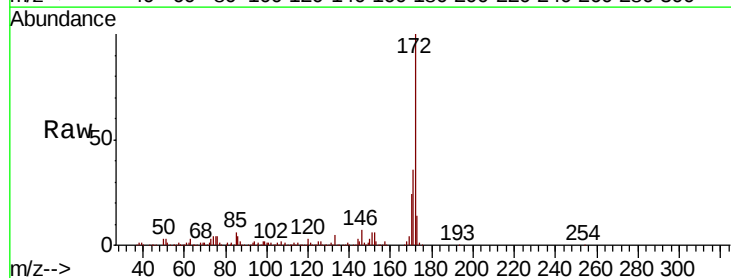


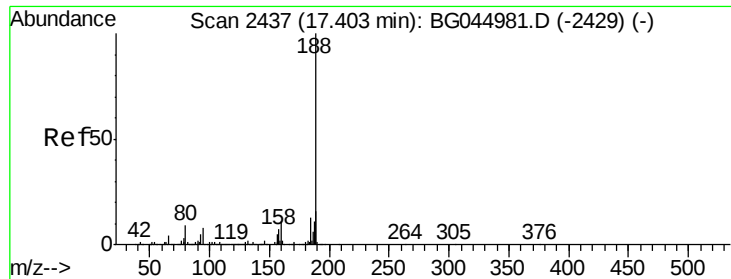




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.37 min Scan# 2431
Delta R.T. -0.01 min
Lab File: BG045251.D
Acq: 6 May 2020 13:39

Instrument :
BNA_G
ClientSampleId :
PB128675BL

Tot Ion:188 Resp: 396988
Ion Ratio Lower Upper
188 100
94 6.6 6.2 9.4
80 8.0 7.0 10.6

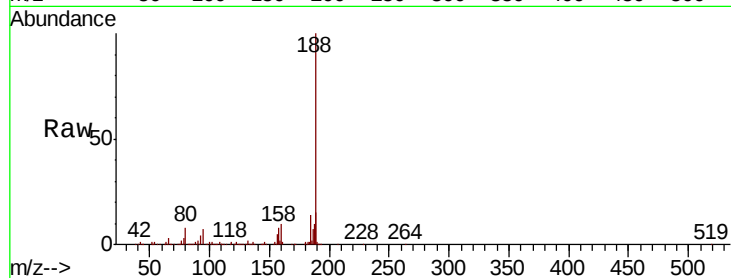


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BG
Ion 80.00 (79.70 to 80.70): BG

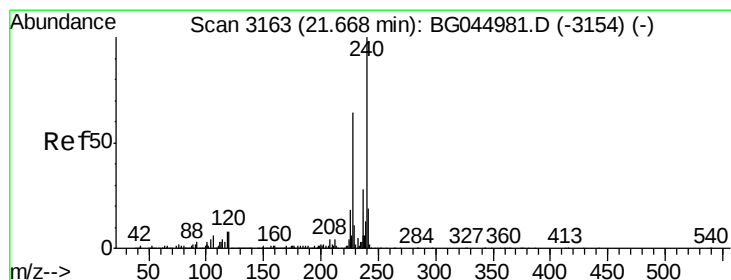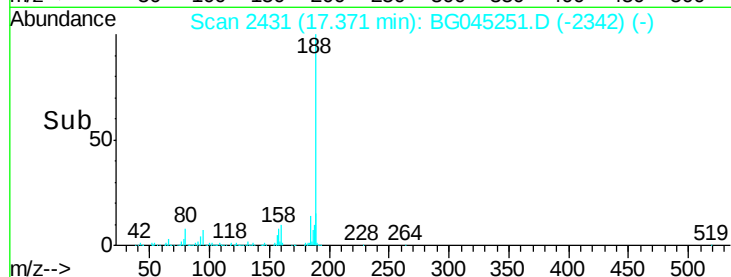
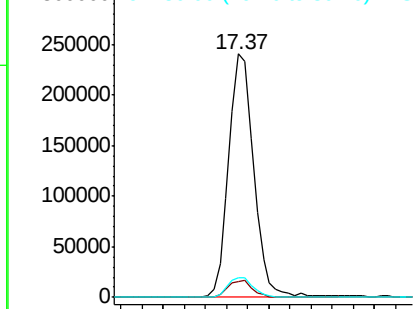



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.64 min Scan# 3158
Delta R.T. -0.00 min
Lab File: BG045251.D
Acq: 6 May 2020 13:39

Tgt Ion:240 Resp: 390401
Ion Ratio Lower Upper
240 100
120 6.1 6.6 10.0#
236 26.6 22.2 33.2

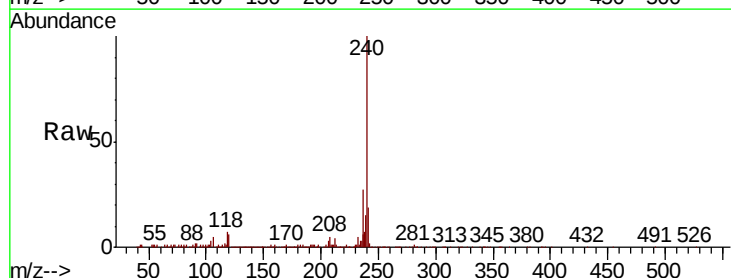

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

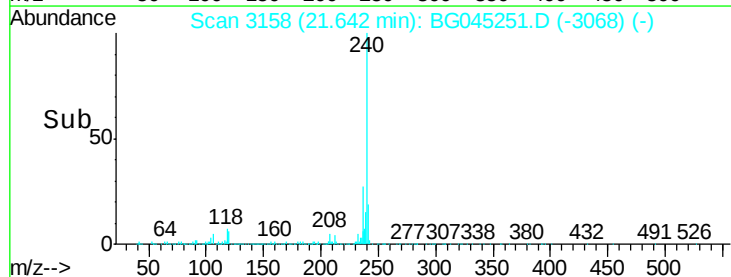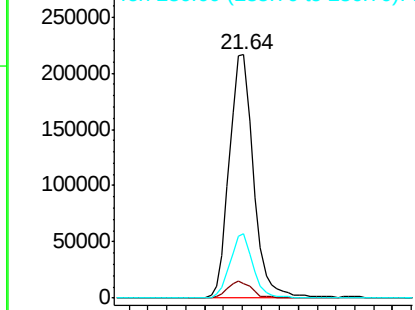

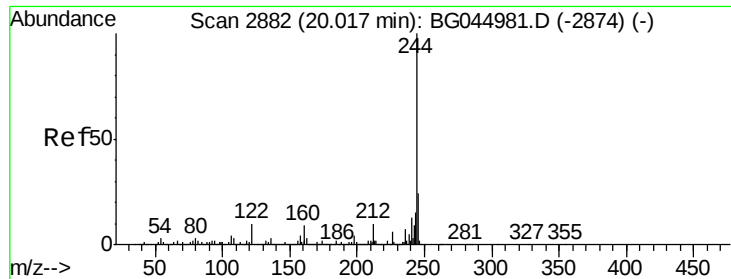

#79

Terphenyl-d14

Concen: 105.371 ng

RT: 19.99 min Scan# 2877

Delta R.T. -0.00 min

Lab File: BG045251.D

Acq: 6 May 2020 13:39

Instrument :

BNA_G

ClientSampleId :

PB128675BL


Tot Ion:244 Resp: 1887397

Ion Ratio Lower Upper

244 100

212 9.9 7.9 11.9




122 9.3 7.7 11.5

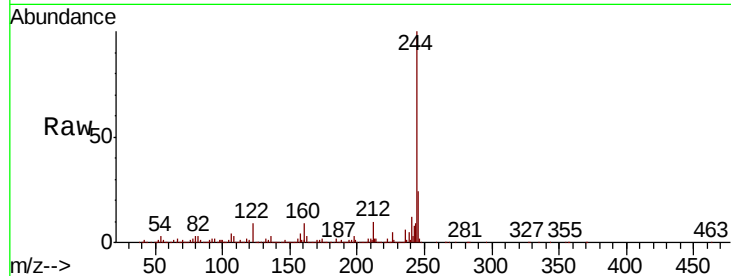

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

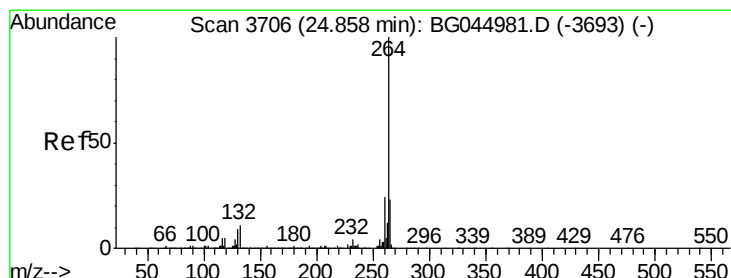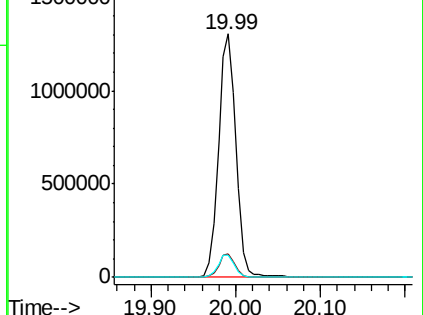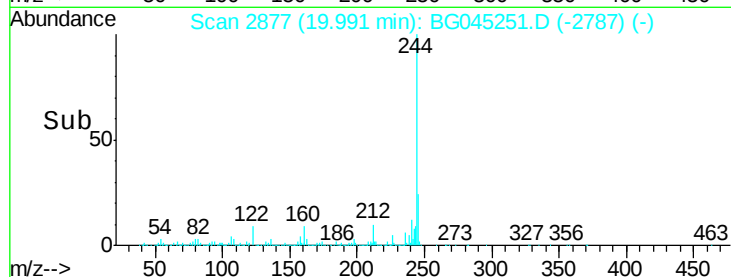

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.81 min Scan# 3698

Delta R.T. -0.00 min

Lab File: BG045251.D

Acq: 6 May 2020 13:39


Tgt Ion:264 Resp: 402828

Ion Ratio Lower Upper

264 100

260 24.8 19.2 28.8

265 23.9 19.0 28.4

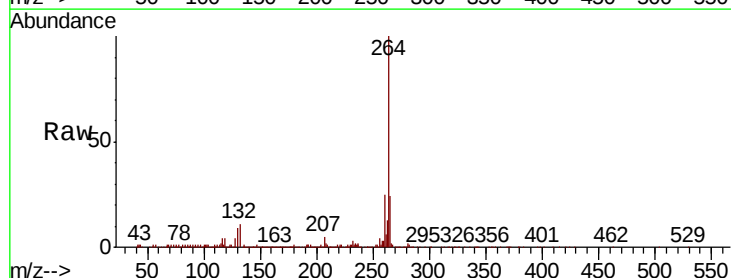

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

