

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG050719\
 Data File : BG040775.D
 Acq On : 7 May 2019 18:30
 Operator : HP/JU
 Sample : K2697-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-4-20190502

Quant Time: May 08 08:56:36 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG042319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 24 05:35:33 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.15	152	44627	20.00	ng	-0.01
21) Naphthalene-d8	10.97	136	180696	20.00	ng	-0.02
39) Acenaphthene-d10	14.77	164	135350	20.00	ng	-0.02
64) Phenanthrene-d10	17.51	188	362399	20.00	ng	-0.02
76) Chrysene-d12	21.80	240	369731	20.00	ng	-0.03
87) Perylene-d12	25.14	264	349399	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.67	112	206068	81.40	ng	-0.01
7) Phenol-d6	7.28	99	210343	53.96	ng	-0.02
23) Nitrobenzene-d5	9.32	82	478711	122.41	ng	-0.02
42) 2,4,6-Tribromophenol	16.26	330	311885	167.64	ng	-0.02
45) 2-Fluorobiphenyl	13.40	172	1040562	111.03	ng	-0.02
79) Terphenyl-d14	20.11	244	2012160	120.57	ng	-0.02


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG050719\
Data File : BG040775.D
Acq On : 7 May 2019 18:30
Operator : HP/JU
Sample : K2697-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-4-20190502

Quant Time: May 08 08:56:36 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG042319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 24 05:35:33 2019
Response via : Initial Calibration

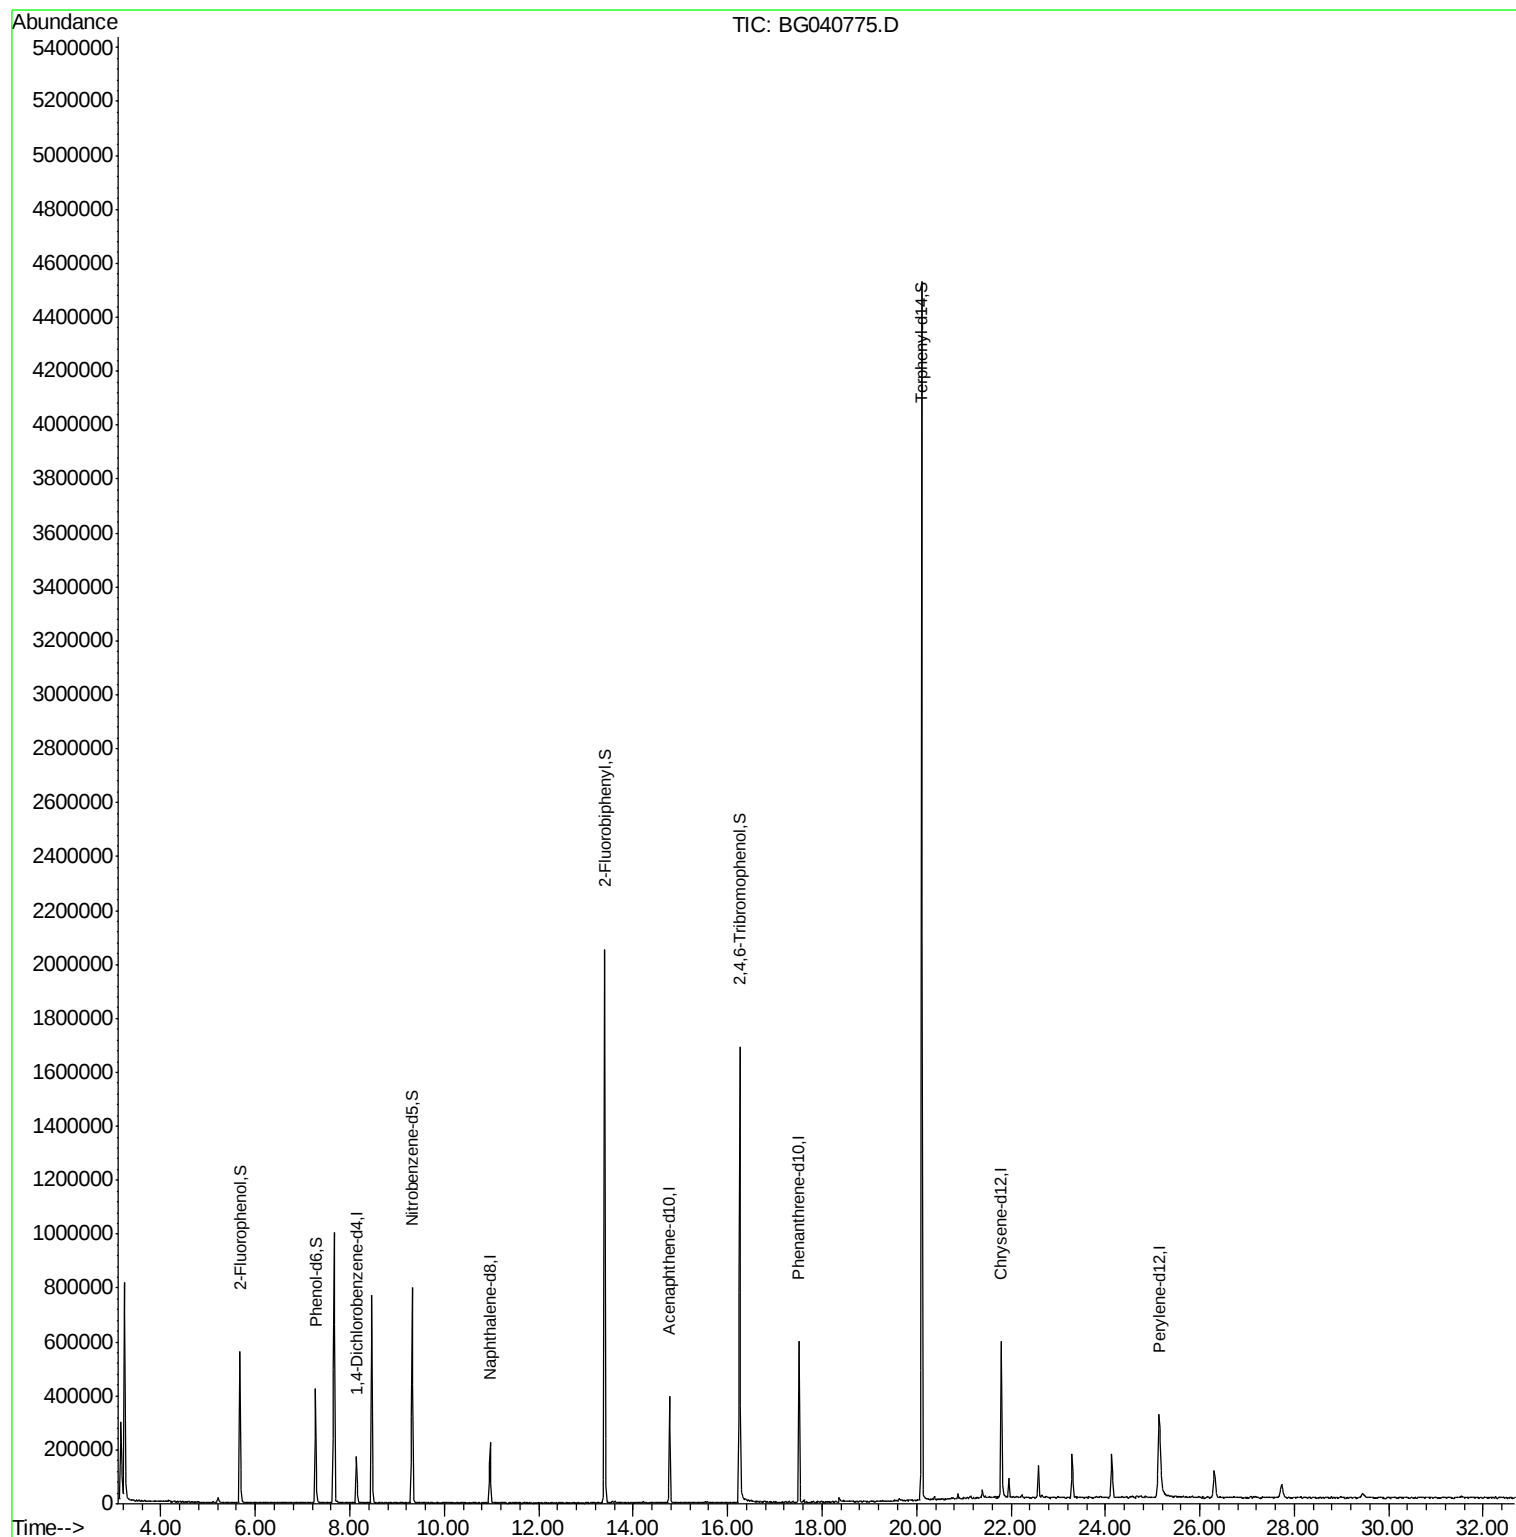




#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.15 min Scan# 861
Delta R.T. -0.01 min
Lab File: BG040775.D
Acq: 7 May 2019 18:30

Instrument :
BNA_G
ClientSampleId :
MW-4-20190502

Tot Ion	Ratio	Lower	Upper
152	100		
150	152.8	120.2	180.2
115	55.4	46.2	69.2



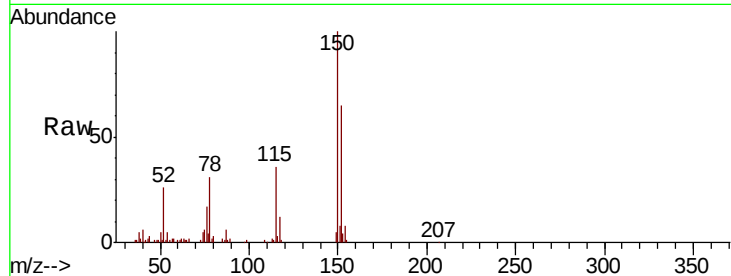


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

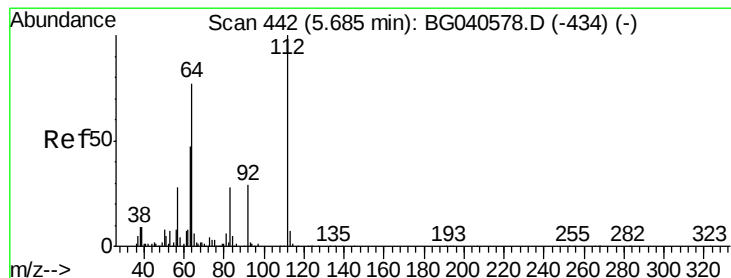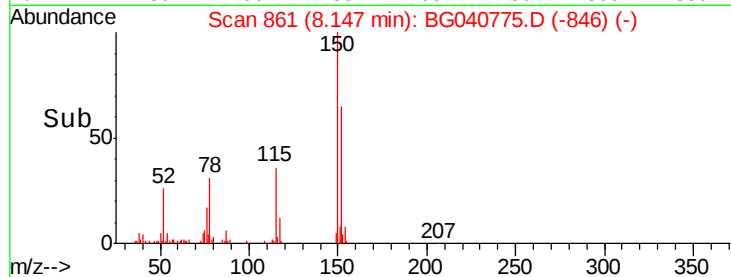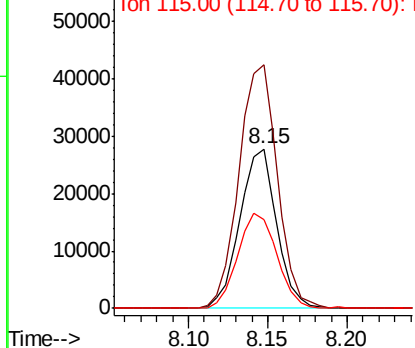

#5

2-Fluorophenol
Concen: 81.397 ng
RT: 5.67 min Scan# 440
Delta R.T. -0.01 min
Lab File: BG040775.D
Acq: 7 May 2019 18:30

Tgt Ion	Ratio	Lower	Upper
112	100		
64	75.6	61.4	92.0
63	41.7	37.8	56.6


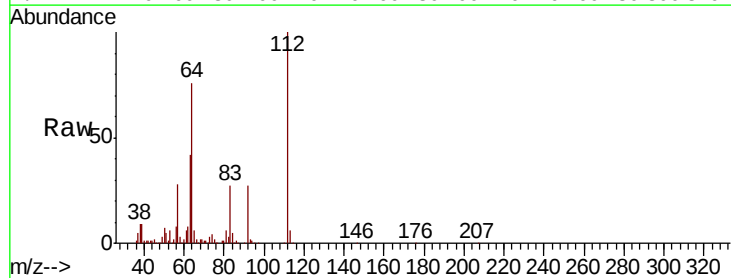


Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

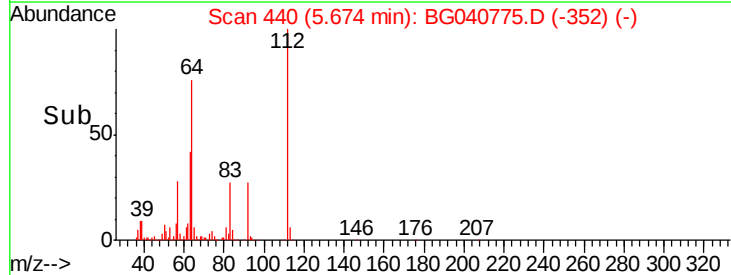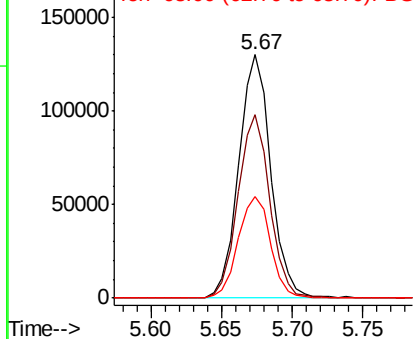



#7

Phenol-d6

Concen: 53.961 ng

RT: 7.28 min Scan# 713

Delta R.T. -0.02 min

Lab File: BG040775.D

Acq: 7 May 2019 18:30

Instrument :

BNA_G

ClientSampleId :

MW-4-20190502


Tot Ion: 99 Resp: 210343

Ion Ratio Lower Upper




99 100

42 23.9 21.8 32.8

71 46.2 38.6 57.8

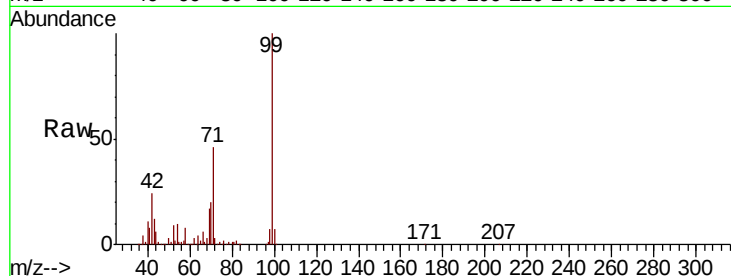

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

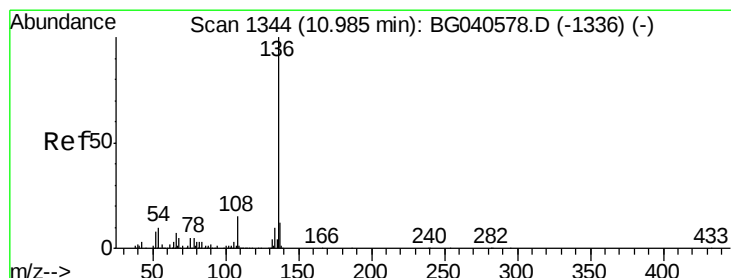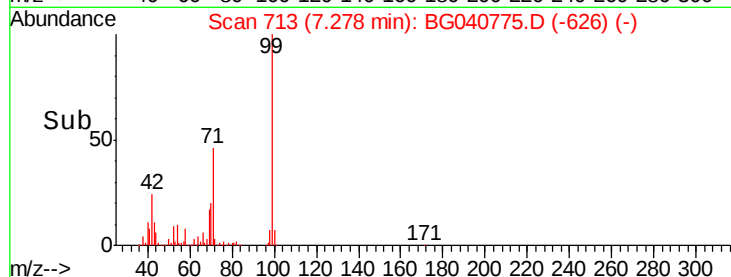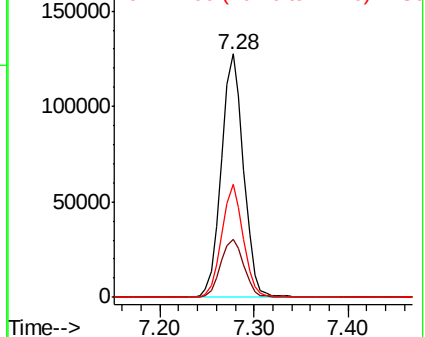

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.97 min Scan# 1341

Delta R.T. -0.02 min

Lab File: BG040775.D

Acq: 7 May 2019 18:30

Tgt Ion: 136 Resp: 180696


Ion Ratio Lower Upper

136 100



137 10.7 9.7 14.5

54 9.1 8.6 12.8

68 6.4 4.8 7.2

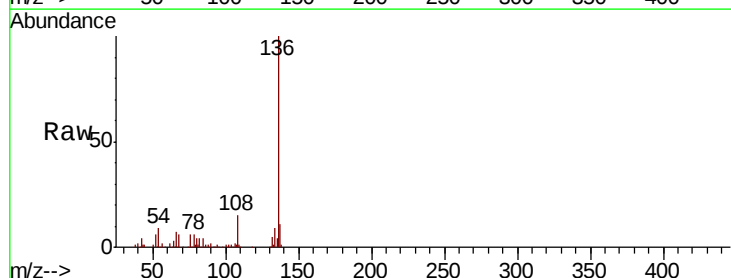

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



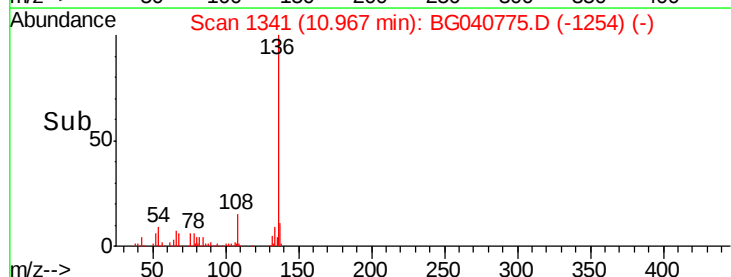
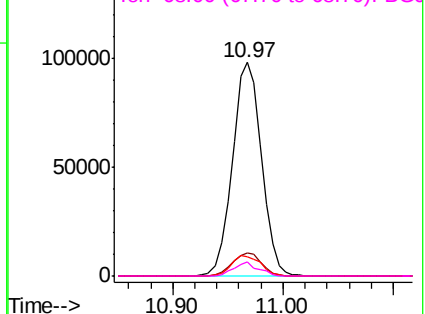




#23
 Nitrobenzene-d5
 Concen: 122.412 ng
 RT: 9.32 min Scan# 1061
 Delta R.T. -0.02 min
 Lab File: BG040775.D
 Acq: 7 May 2019 18:30




Instrument :
 BNA_G
 ClientSampleId :
 MW-4-20190502

Tot Ion	82	Resp	478711
Ion Ratio	Lower	Upper	
82	100		
128	38.6	28.9	43.3
54	54.7	47.2	70.8

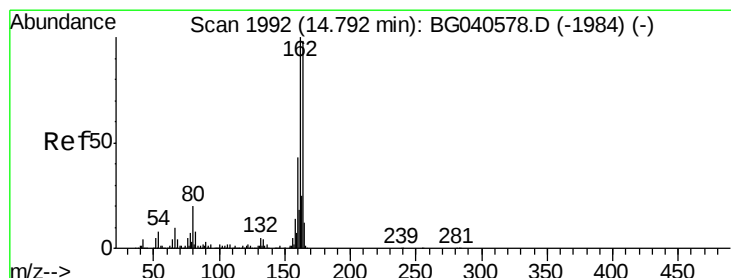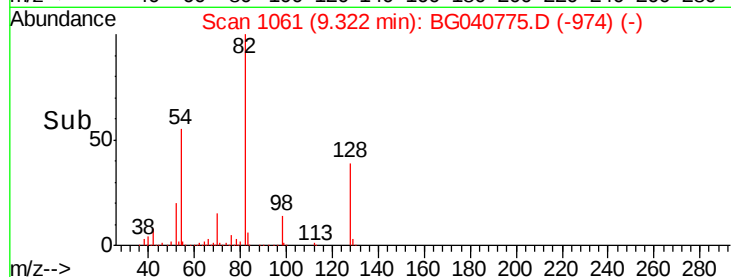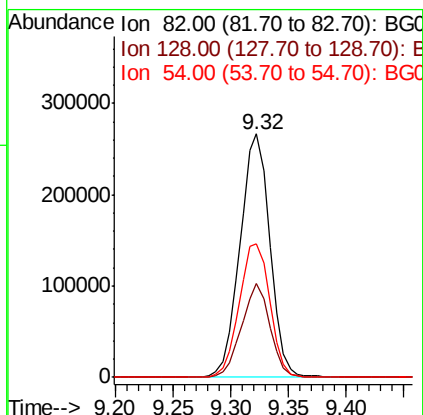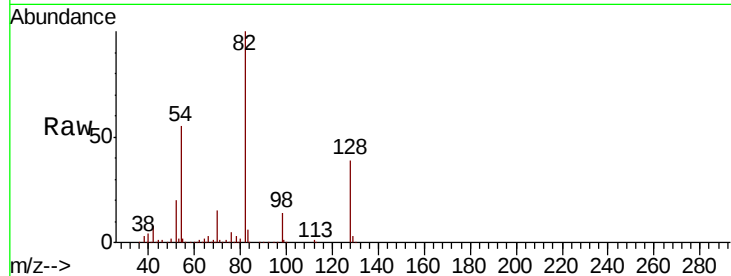

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.77 min Scan# 1988
 Delta R.T. -0.02 min
 Lab File: BG040775.D
 Acq: 7 May 2019 18:30

Tgt Ion	164	Resp	135350
Ion Ratio	Lower	Upper	
164	100		
162	104.6	81.9	122.9
160	44.1	35.4	53.2


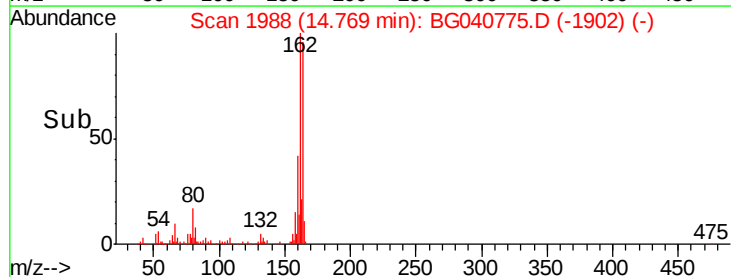
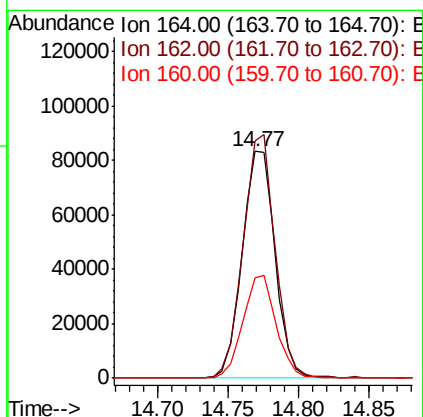
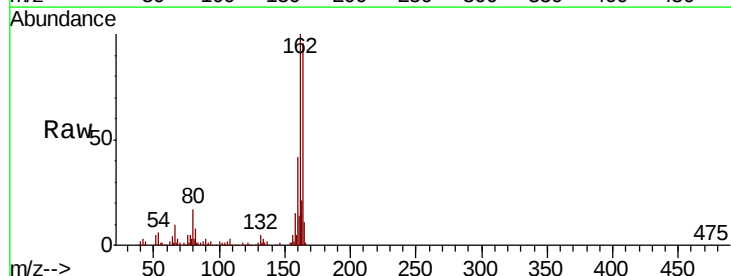




#42
 2,4,6-Tribromophenol
 Concen: 167.643 ng
 RT: 16.26 min Scan# 2241
 Delta R.T. -0.02 min
 Lab File: BG040775.D
 Acq: 7 May 2019 18:30




Instrument :
 BNA_G
 ClientSampleId :
 MW-4-20190502


Tot Ion	Ratio	Lower	Upper
330	100		
332	94.4	75.9	113.9
141	37.0	32.4	48.6

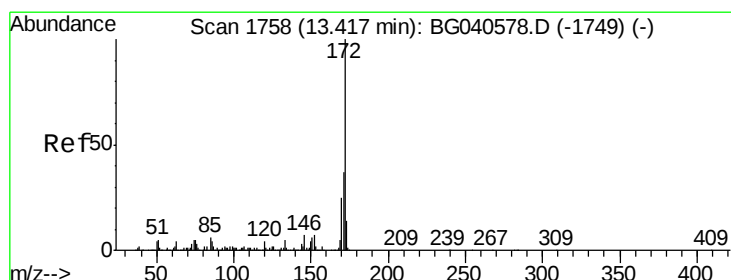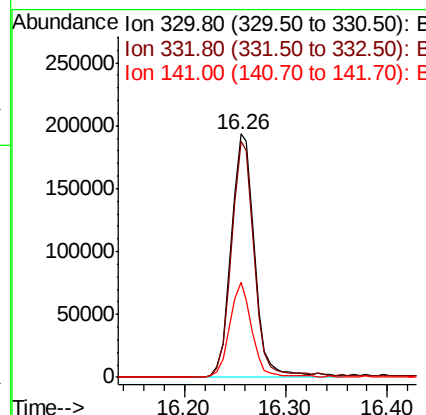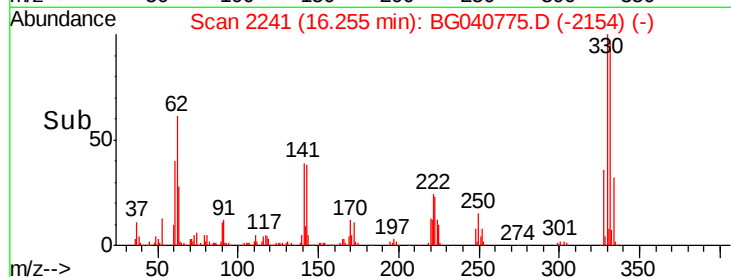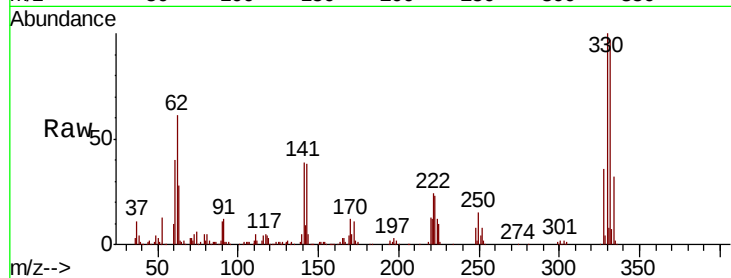

#45
 2-Fluorobiphenyl
 Concen: 111.029 ng
 RT: 13.40 min Scan# 1755
 Delta R.T. -0.02 min
 Lab File: BG040775.D
 Acq: 7 May 2019 18:30

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.0	29.4	44.2
170	25.7	19.9	29.9


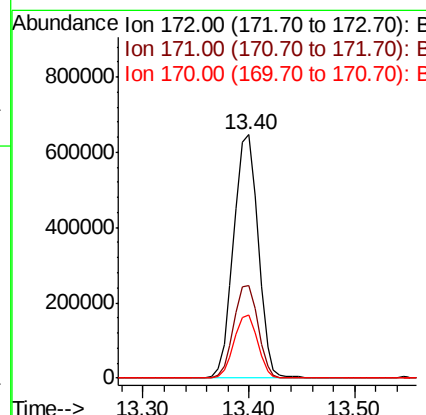
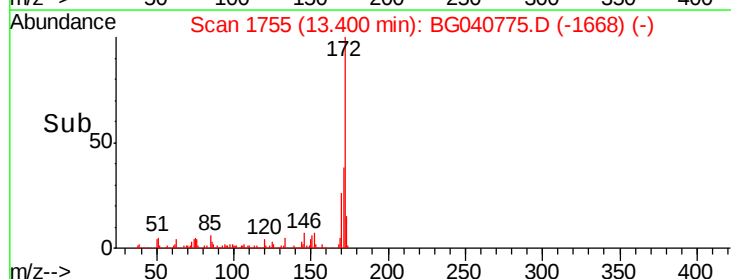
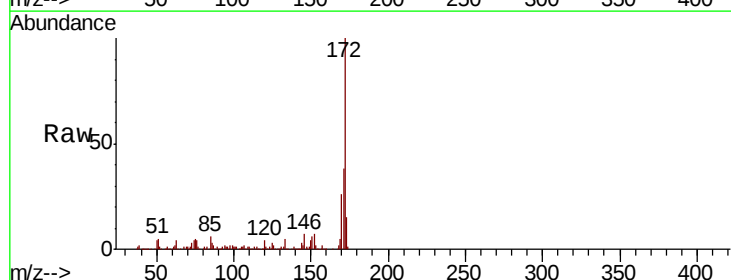


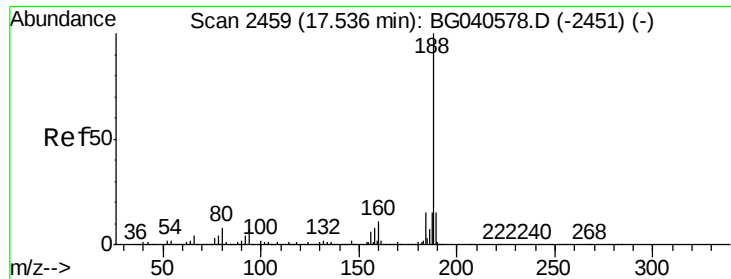

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.51 min Scan# 2455
Delta R.T. -0.02 min
Lab File: BG040775.D
Acq: 7 May 2019 18:30




Instrument :
BNA_G
ClientSampleId :
MW-4-20190502


Tot Ion	Ratio	Lower	Upper
188	100		
94	6.2	5.6	8.4
80	8.4	6.4	9.6

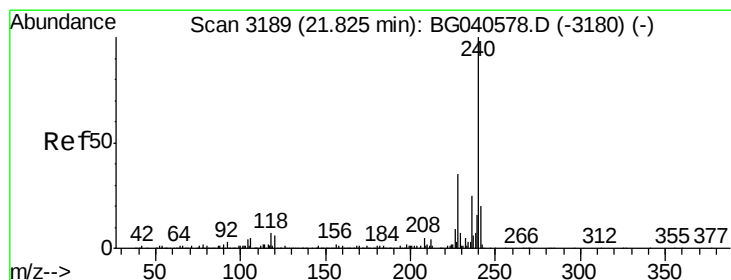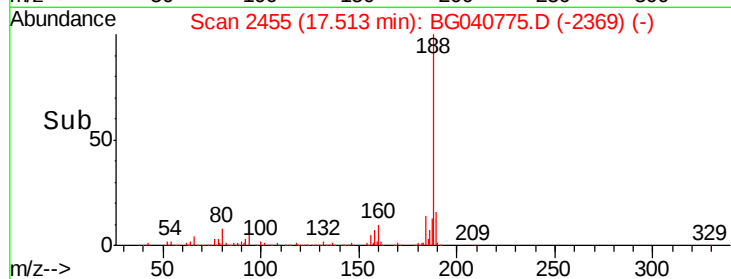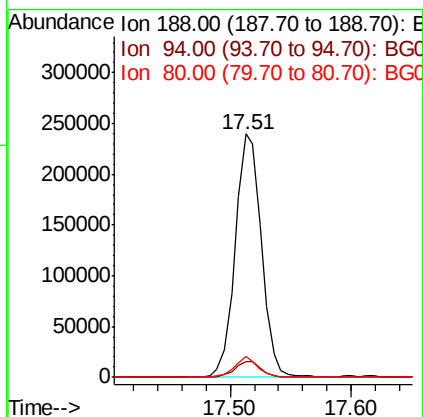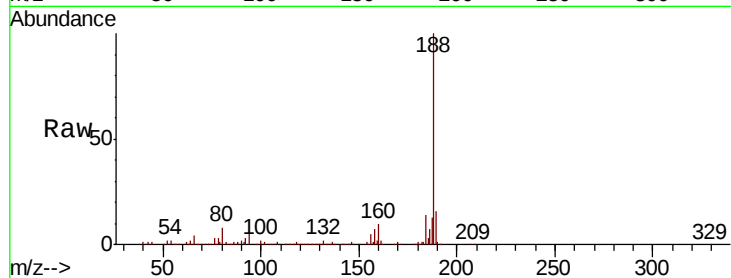

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.80 min Scan# 3184
Delta R.T. -0.03 min
Lab File: BG040775.D
Acq: 7 May 2019 18:30

Tgt Ion	Ratio	Lower	Upper
240	100		
120	5.9	5.0	7.6
236	26.2	20.3	30.5

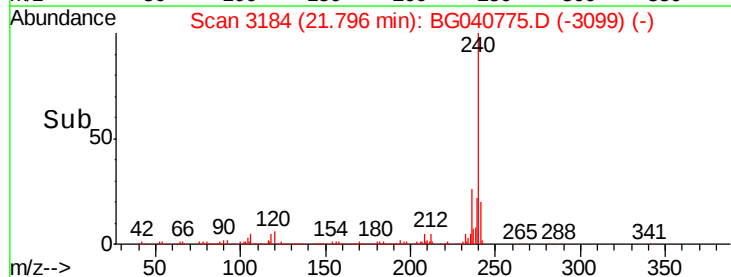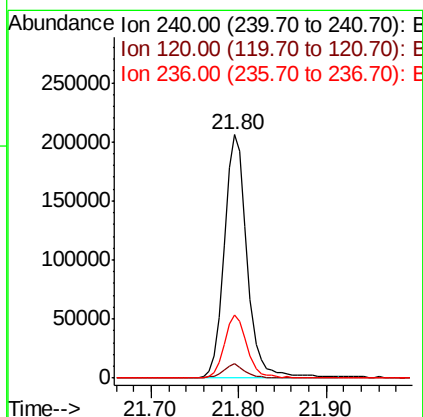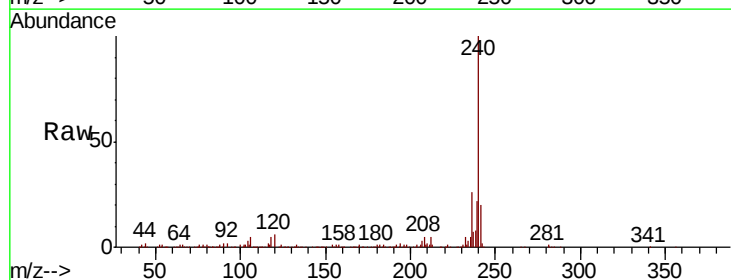

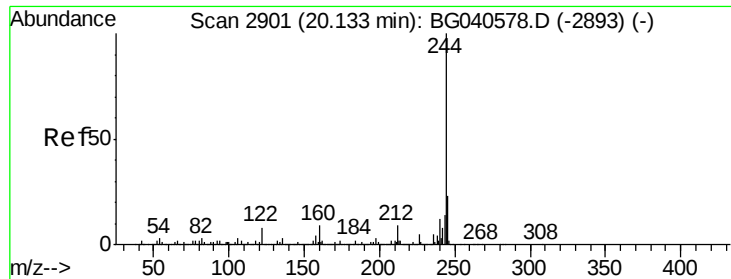

#79

Terphenyl-d14

Concen: 120.568 ng

RT: 20.11 min Scan# 2897

Delta R.T. -0.02 min

Lab File: BG040775.D

Acq: 7 May 2019 18:30

Instrument :

BNA_G

ClientSampleId :

MW-4-20190502


Tot Ion:244 Resp: 2012160

Ion Ratio Lower Upper

244 100

212 9.8 7.2 10.8




122 8.2 6.6 10.0

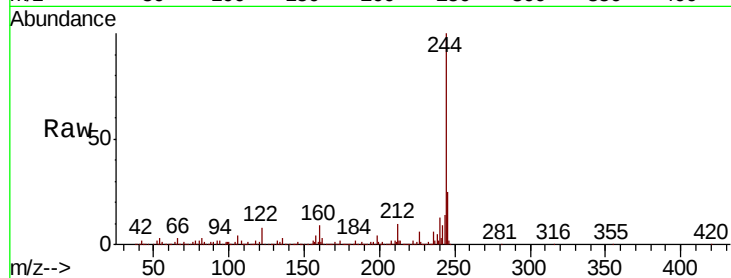

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

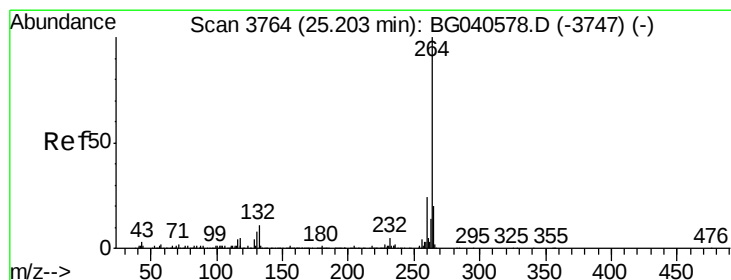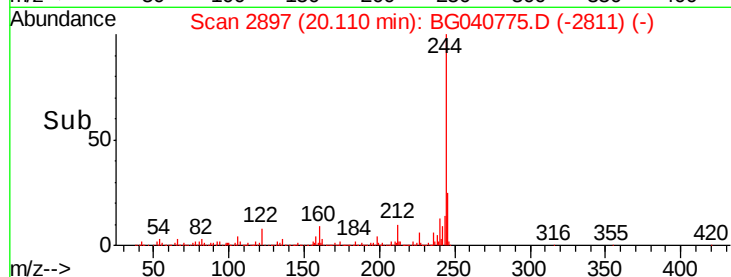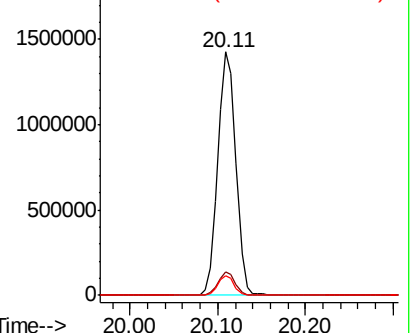

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.14 min Scan# 3754

Delta R.T. -0.06 min

Lab File: BG040775.D

Acq: 7 May 2019 18:30


Tgt Ion:264 Resp: 349399

Ion Ratio Lower Upper

264 100

260 22.7 19.2 28.8

265 22.0 16.6 25.0

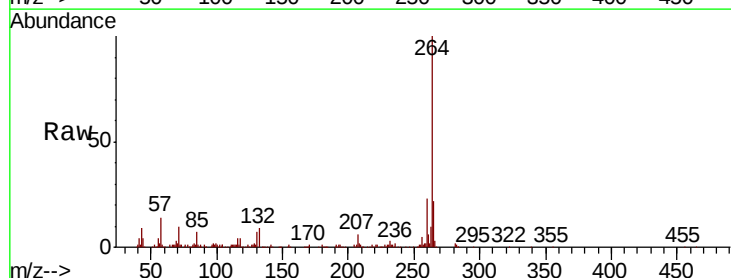

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

