

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050719\
 Data File : BG040774.D
 Acq On : 7 May 2019 17:52
 Operator : HP/JU
 Sample : K2675-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 OUTFALL001-WK-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.157	6	12	21	rBV	107607	197622	3.44%	0.962%
2	3.234	21	25	31	rVB	86578	117489	2.05%	0.572%
3	5.214	357	362	370	rVB2	46532	73178	1.28%	0.356%
4	5.672	434	440	448	rBV	436758	699405	12.19%	3.405%
5	7.276	706	713	723	rBV	352594	594538	10.36%	2.895%
6	7.664	771	779	788	rBV	891997	1508852	26.30%	7.346%
7	8.145	854	861	871	rBV	173283	300745	5.24%	1.464%
8	8.469	908	916	924	rBV	788557	1352472	23.57%	6.585%
9	9.320	1052	1061	1069	rBV	791510	1405350	24.49%	6.843%
10	10.966	1332	1341	1348	rBV	228424	401518	7.00%	1.955%
11	13.398	1745	1755	1764	rBV	2129915	3205297	55.87%	15.606%
12	14.773	1979	1989	1998	rBV2	388226	637922	11.12%	3.106%
13	16.254	2235	2241	2267	rBV	1042632	1734071	30.22%	8.443%
14	17.517	2448	2456	2466	rBV2	563322	868919	15.14%	4.231%
15	20.114	2891	2898	2909	rBV	4123055	5737469	100.00%	27.935%
16	21.794	3178	3184	3203	rBV2	507405	965776	16.83%	4.702%
17	25.155	3745	3756	3770	rBV2	213054	737871	12.86%	3.593%


Sum of corrected areas: 20538494

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050719\
Data File : BG040774.D
Acq On : 7 May 2019 17:52
Operator : HP/JU
Sample : K2675-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OUTFALL001-WK-1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

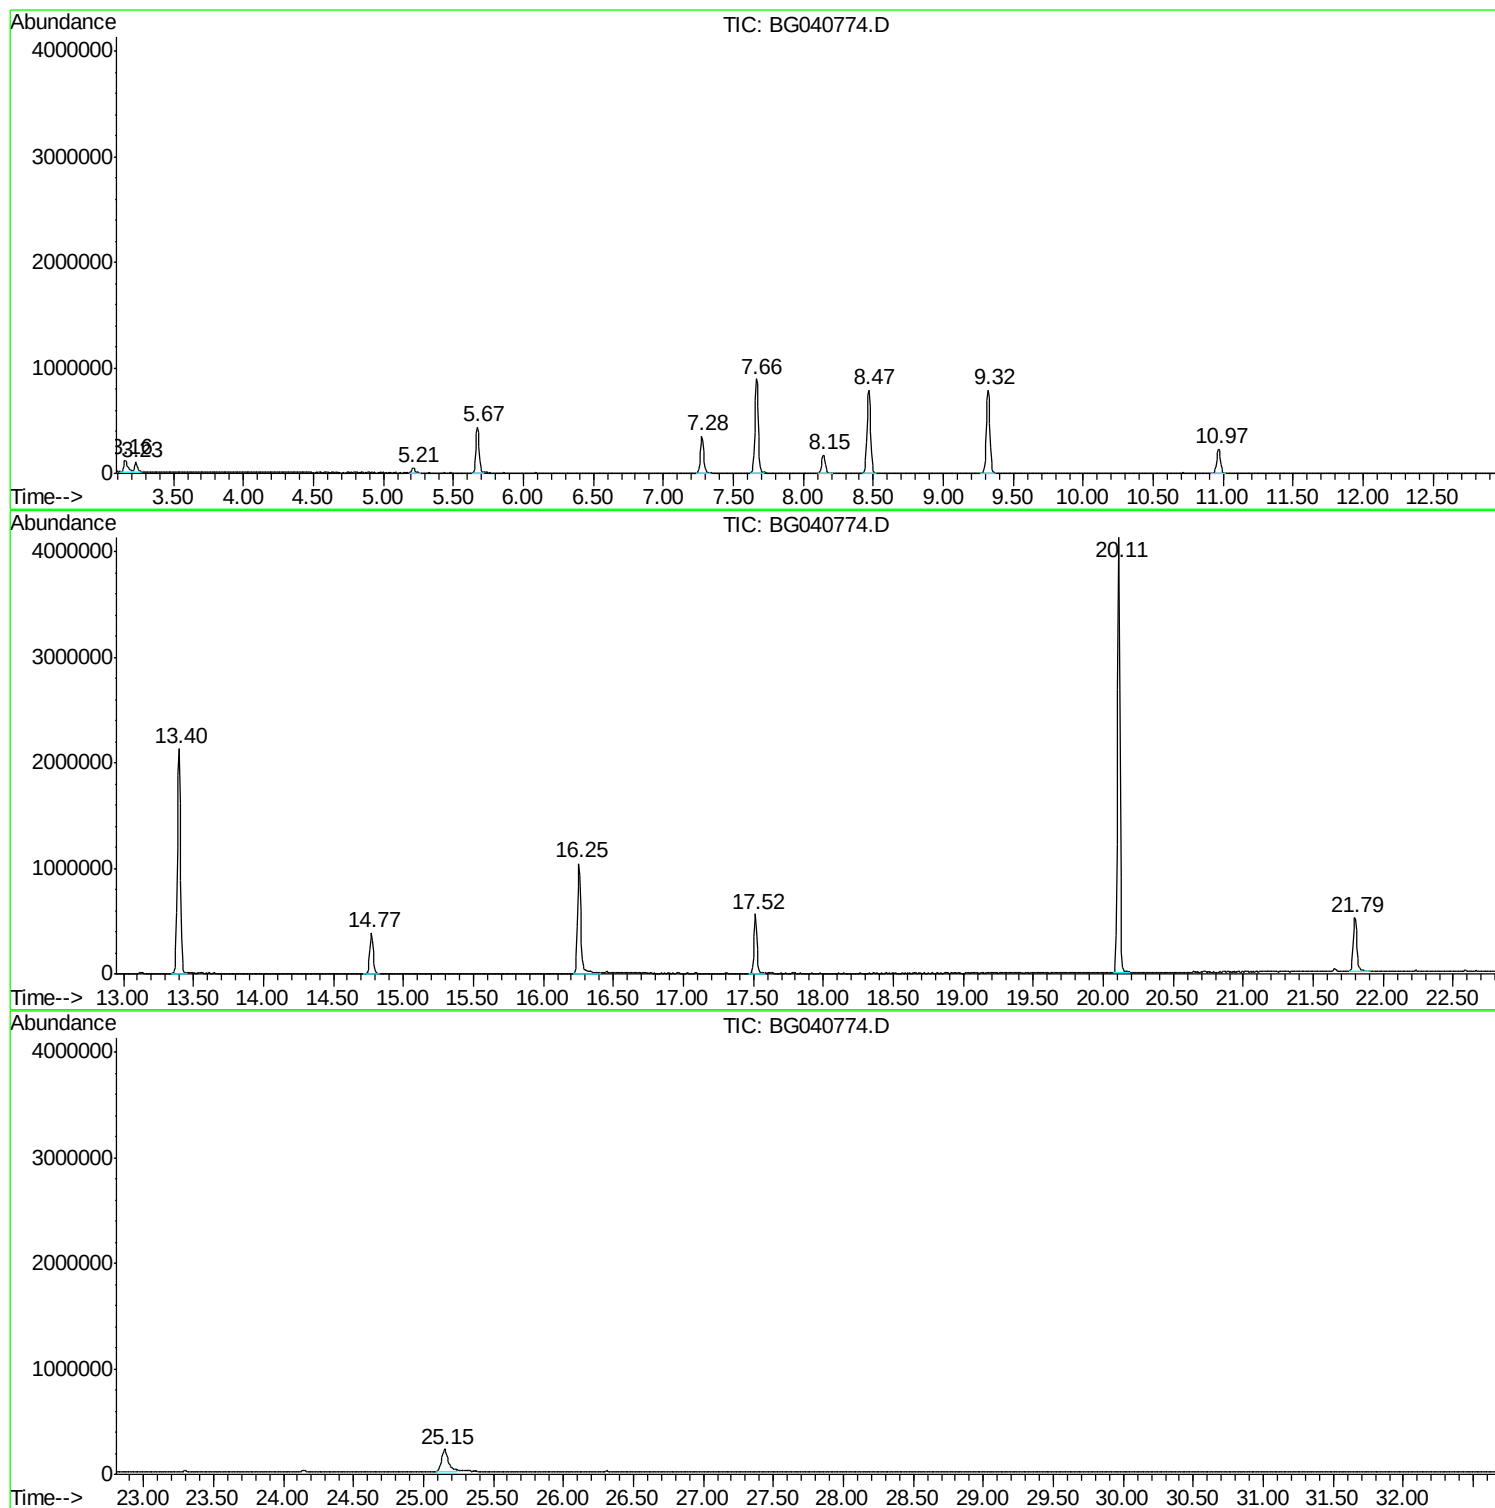

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050719\
Data File : BG040774.D
Acq On : 7 May 2019 17:52
Operator : HP/JU
Sample : K2675-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OUTFALL001-WK-1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050719\
Data File : BG040774.D
Acq On : 7 May 2019 17:52
Operator : HP/JU
Sample : K2675-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OUTFALL001-WK-1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc