


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG050719\
 Data File : BG040763.D
 Acq On : 7 May 2019 9:35
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 24 05:35:33 2019

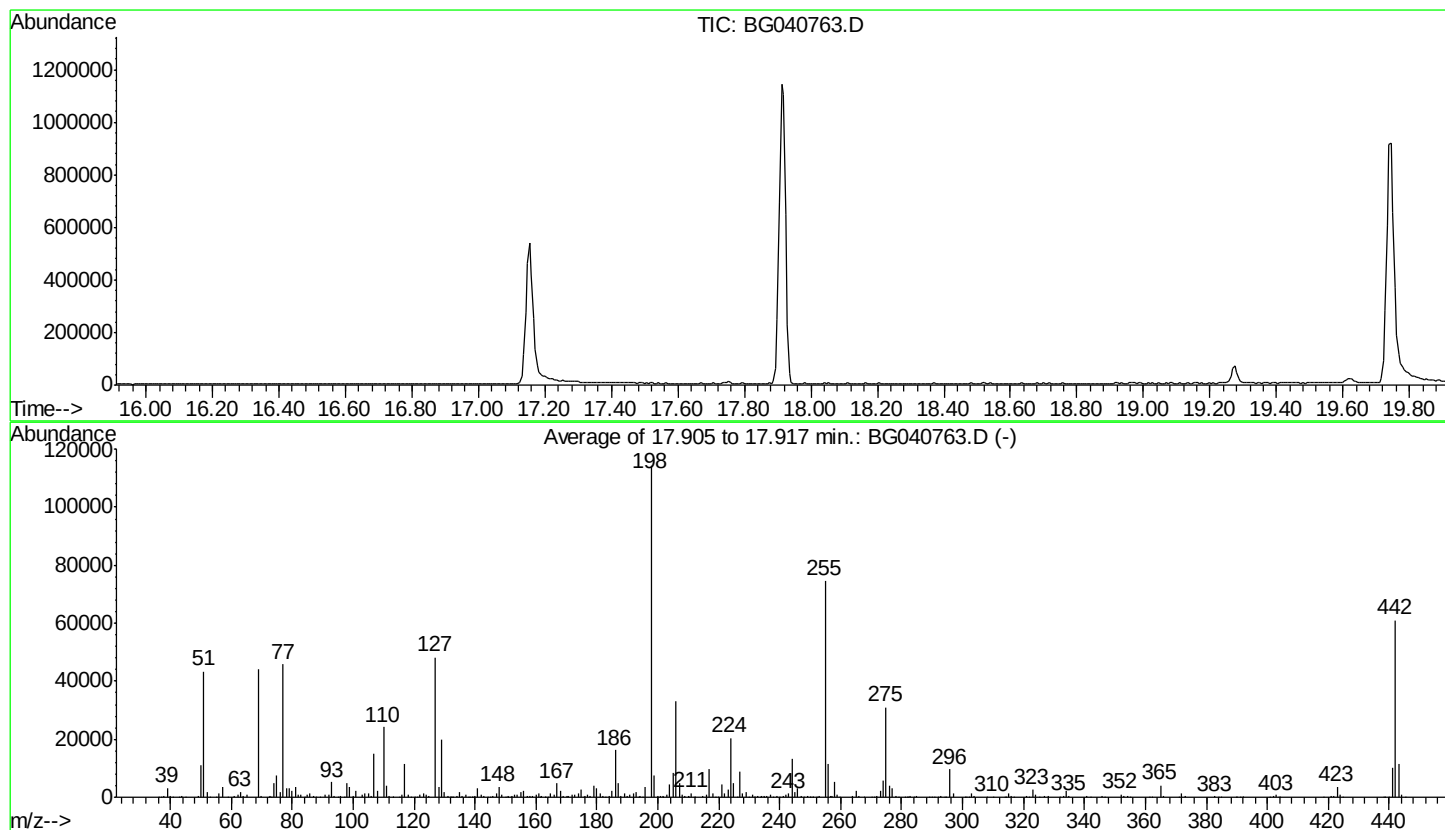

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2516

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	43360	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.5	43992	PASS
70	69	0.00	2	0.6	278	PASS
127	198	10	80	42.2	48296	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	114328	PASS
199	198	5	9	6.7	7668	PASS
275	198	10	60	27.1	30970	PASS
365	198	1	100	3.6	4134	PASS
441	198	0.01	100	8.7	9990	PASS
442	198	50	100	53.4	61016	PASS
443	442	15	24	18.9	11509	PASS