

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG050720\
 Data File : BG045288.D
 Acq On : 8 May 2020 3:19
 Operator : CG/JU
 Sample : L2497-01 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 HD-01-050620

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.147	6	10	15	rVB4	16943	31511	2.69%	0.330%
2	5.549	412	419	430	rBV	202558	355147	30.35%	3.719%
3	7.141	684	690	703	rBV	217556	403280	34.46%	4.224%
4	7.981	823	833	840	rBV	269933	469847	40.15%	4.921%
5	8.304	881	888	898	rVB	194978	346873	29.64%	3.633%
6	9.139	1022	1030	1040	rBV	140626	260745	22.28%	2.731%
7	10.789	1302	1311	1321	rBV	353186	669014	57.16%	7.007%
8	13.245	1722	1729	1736	rBV	428677	678609	57.98%	7.107%
9	13.521	1769	1776	1783	rVB2	23657	39142	3.34%	0.410%
10	14.067	1864	1869	1876	rBV	42055	66171	5.65%	0.693%
11	14.625	1957	1964	1975	rBV2	602903	989584	84.55%	10.364%
12	16.111	2208	2217	2229	rBV	314177	509614	43.54%	5.337%
13	17.369	2423	2431	2442	rBV	719477	1170363	100.00%	12.257%
14	18.267	2577	2584	2587	rBV9	7924	15557	1.33%	0.163%
15	19.419	2776	2780	2785	rBV	18935	29113	2.49%	0.305%
16	19.783	2838	2842	2847	rVB2	20544	39423	3.37%	0.413%
17	19.983	2870	2876	2887	rBV	698181	937678	80.12%	9.820%
18	20.729	3001	3003	3006	rBV4	16366	20171	1.72%	0.211%
19	21.299	3097	3100	3108	rVB7	42068	68111	5.82%	0.713%
20	21.633	3150	3157	3166	rBV2	657753	1137884	97.22%	11.917%
21	21.839	3190	3192	3197	rVB4	38884	54745	4.68%	0.573%
22	22.444	3291	3295	3302	rBV3	52417	95893	8.19%	1.004%
23	23.131	3408	3412	3418	rVB2	58602	100159	8.56%	1.049%
24	24.806	3688	3697	3706	rBV2	354563	1059721	90.55%	11.098%


Sum of corrected areas: 9548355

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG050720\
Data File : BG045288.D
Acq On : 8 May 2020 3:19
Operator : CG/JU
Sample : L2497-01 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
HD-01-050620

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

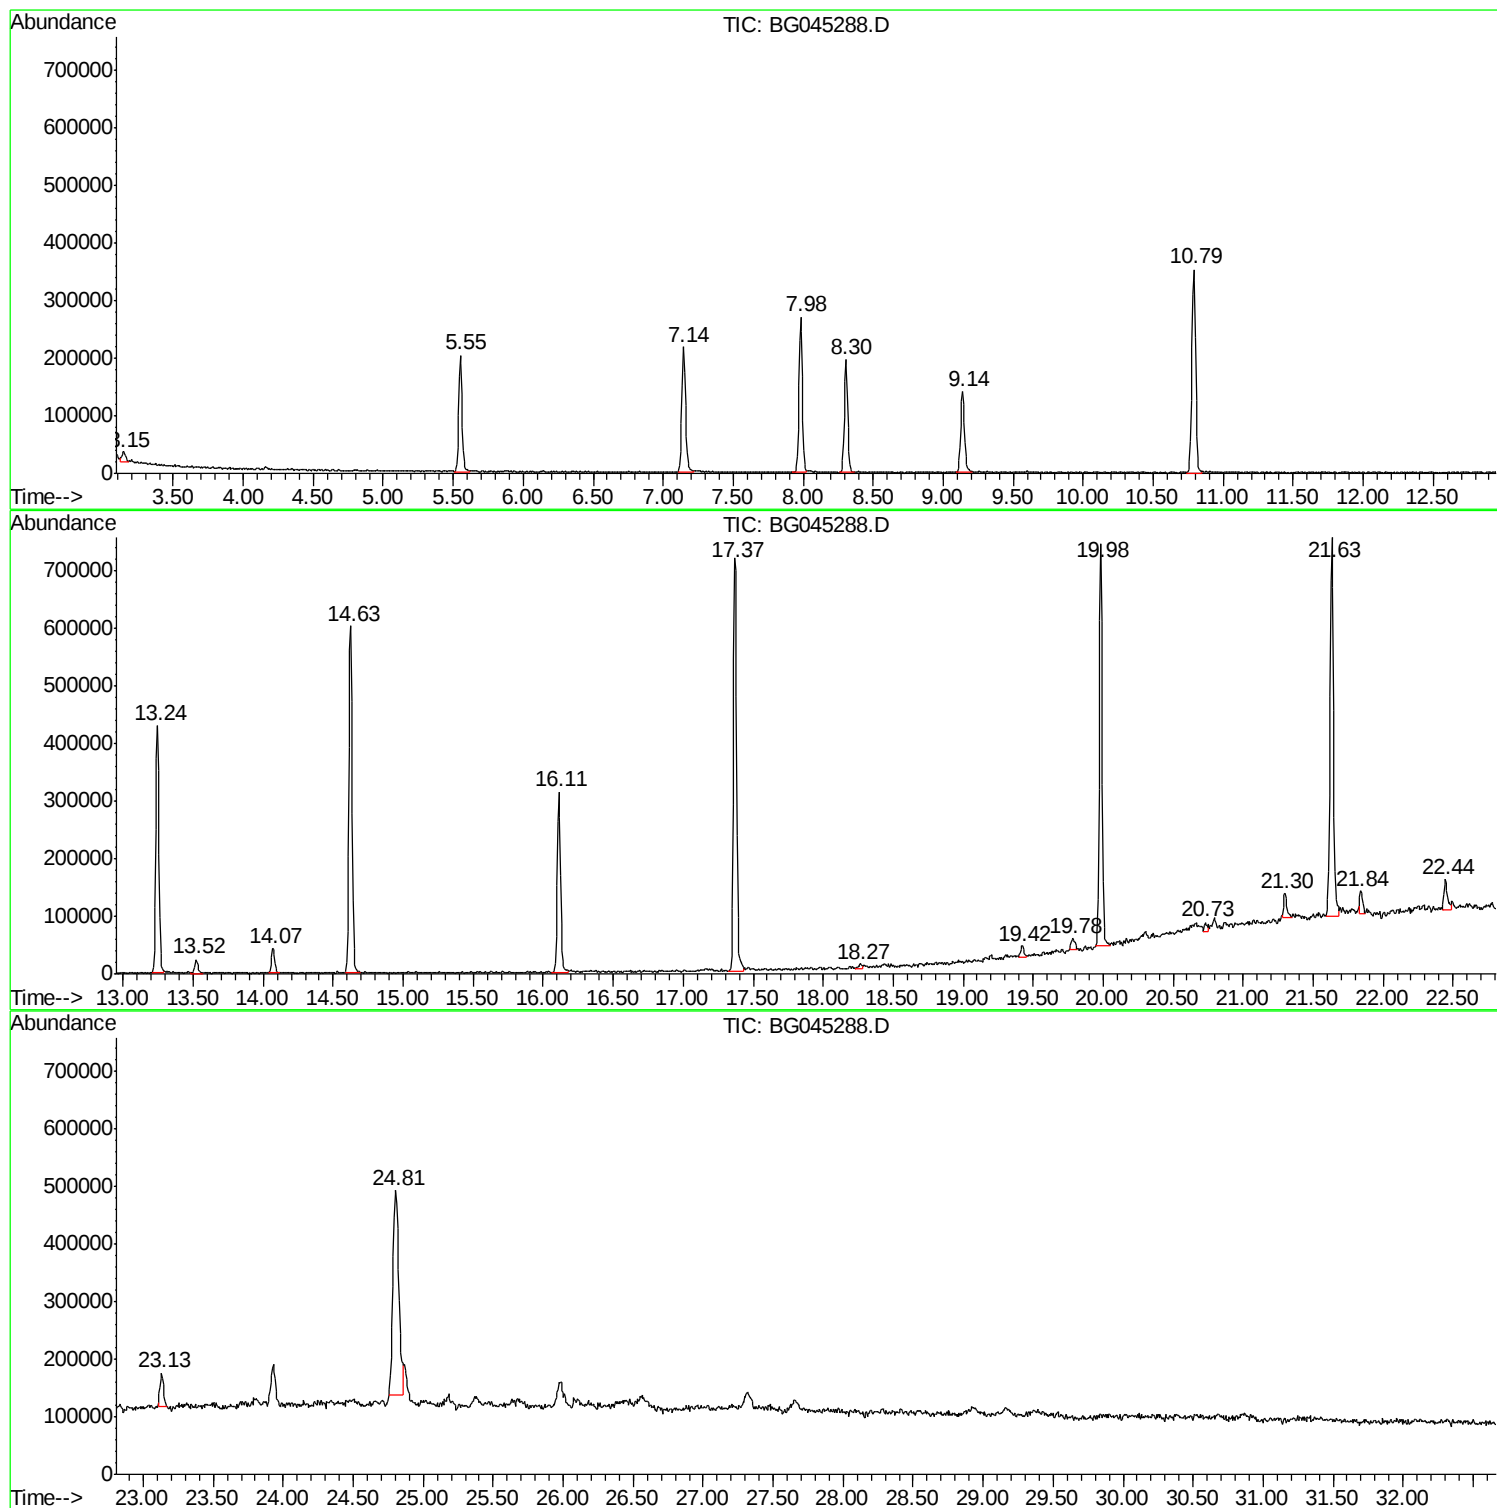

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG050720\
Data_File : BG045288.D
Acq_On : 8_May, 2020 3:199
Operator : CG/JUU
Sample : L2497-01_5XX
Misc :
ALS_Vial : 23 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
HD-01-050620

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
