


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG050720\
 Data File : BG045264.D
 Acq On : 7 May 2020 11:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 07 12:51:10 2020

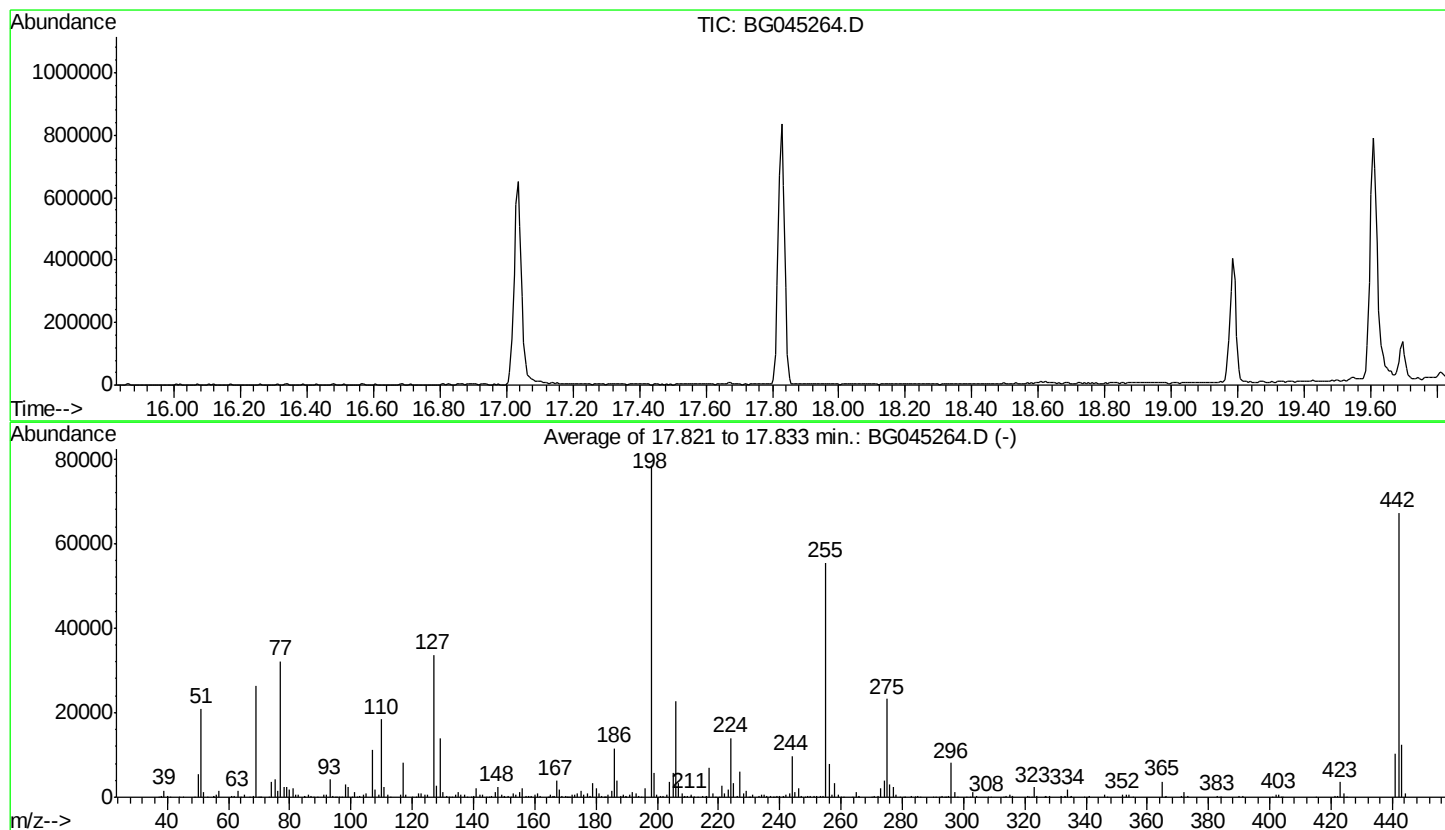

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.7	20893	PASS
68	69	0.00	2	1.7	446	PASS
69	198	0.00	100	33.6	26321	PASS
70	69	0.00	2	0.3	69	PASS
127	198	10	80	42.9	33645	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	78384	PASS
199	198	5	9	7.4	5836	PASS
275	198	10	60	29.6	23240	PASS
365	198	1	100	4.8	3770	PASS
441	198	0.01	100	13.3	10438	PASS
442	198	50	100	85.7	67181	PASS
443	442	15	24	18.4	12335	PASS