
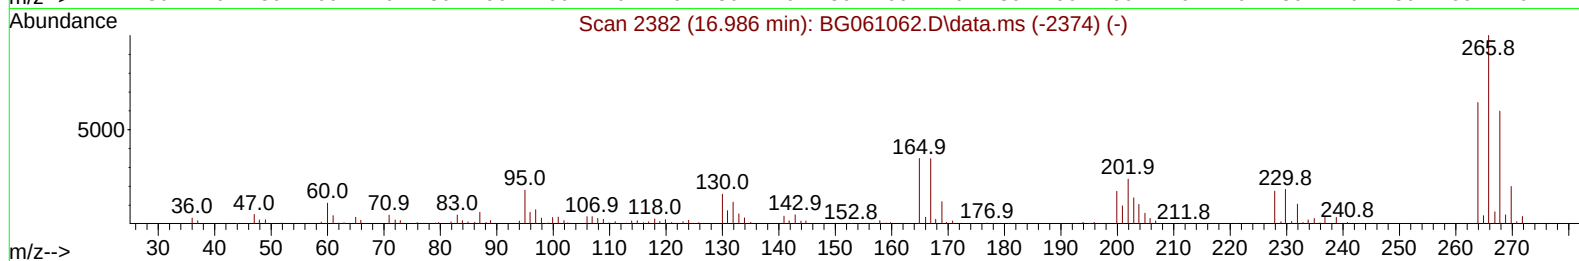
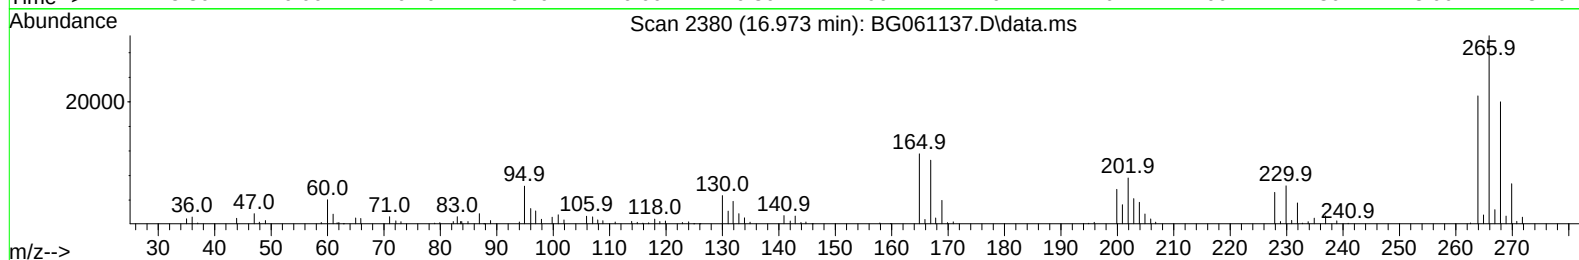


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050824\
Data File : BG061137.D
Acq On : 8 May 2024 10:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 11:59:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

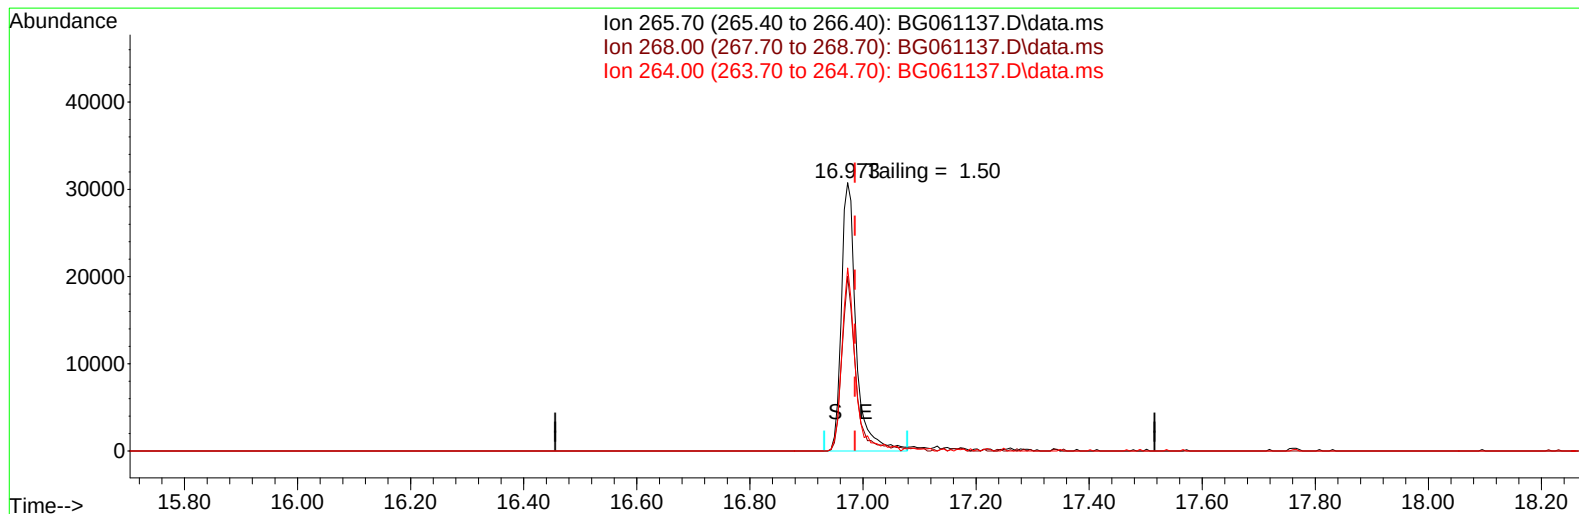

TIC: BG061137.D\data.ms

(70) Pentachlorophenol (C)




16.973min (-0.013) 20316.27 ng

response 55633

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.80	65.05
264.00	64.40	68.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050824\
Data File : BG061137.D
Acq On : 8 May 2024 10:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 11:59:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

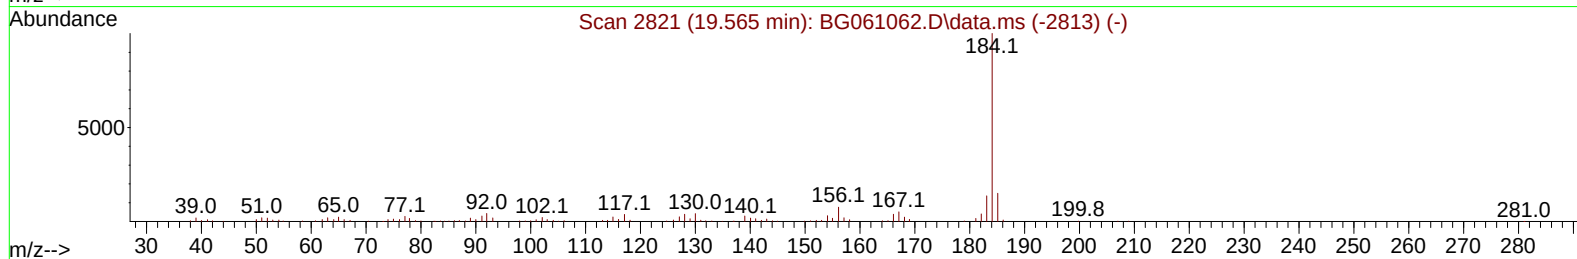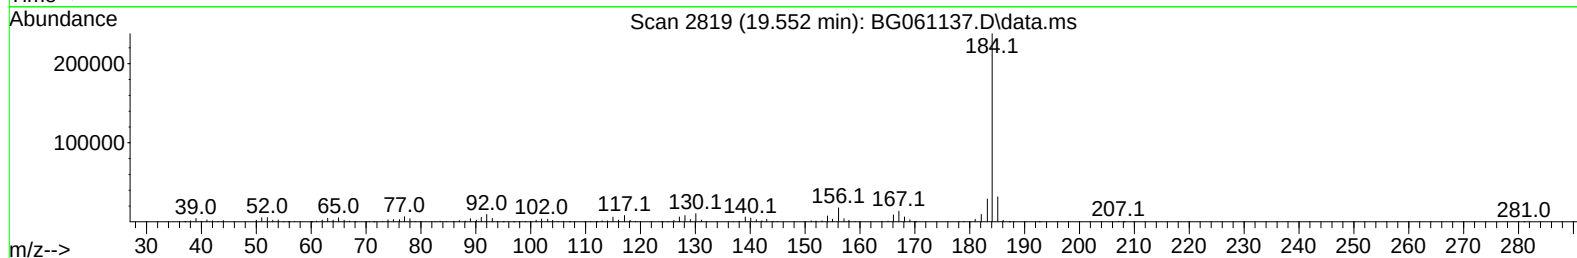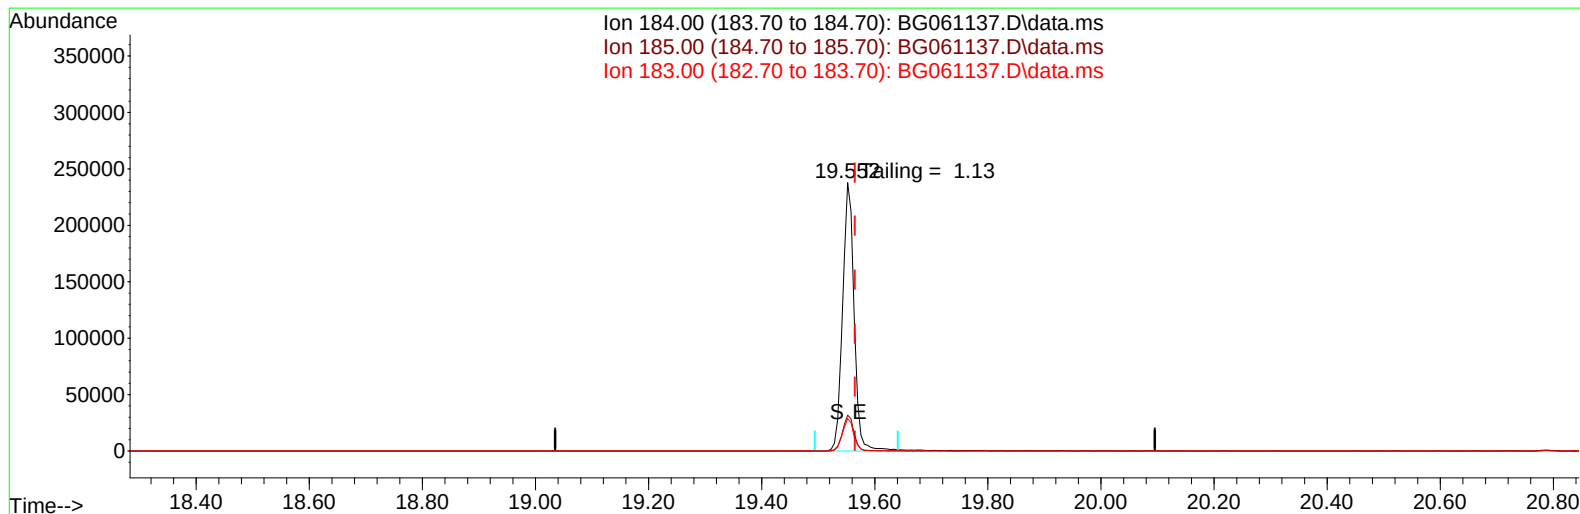

TIC: BG061137.D\data.ms

(77) Benzidine

19.552min (-0.013) 268249.19 ng m

response 336050

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.37
183.00	13.60	12.14
0.00	0.00	0.00