


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050824\
Data File : BG061137.D
Acq On : 8 May 2024 10:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 01 05:11:25 2024

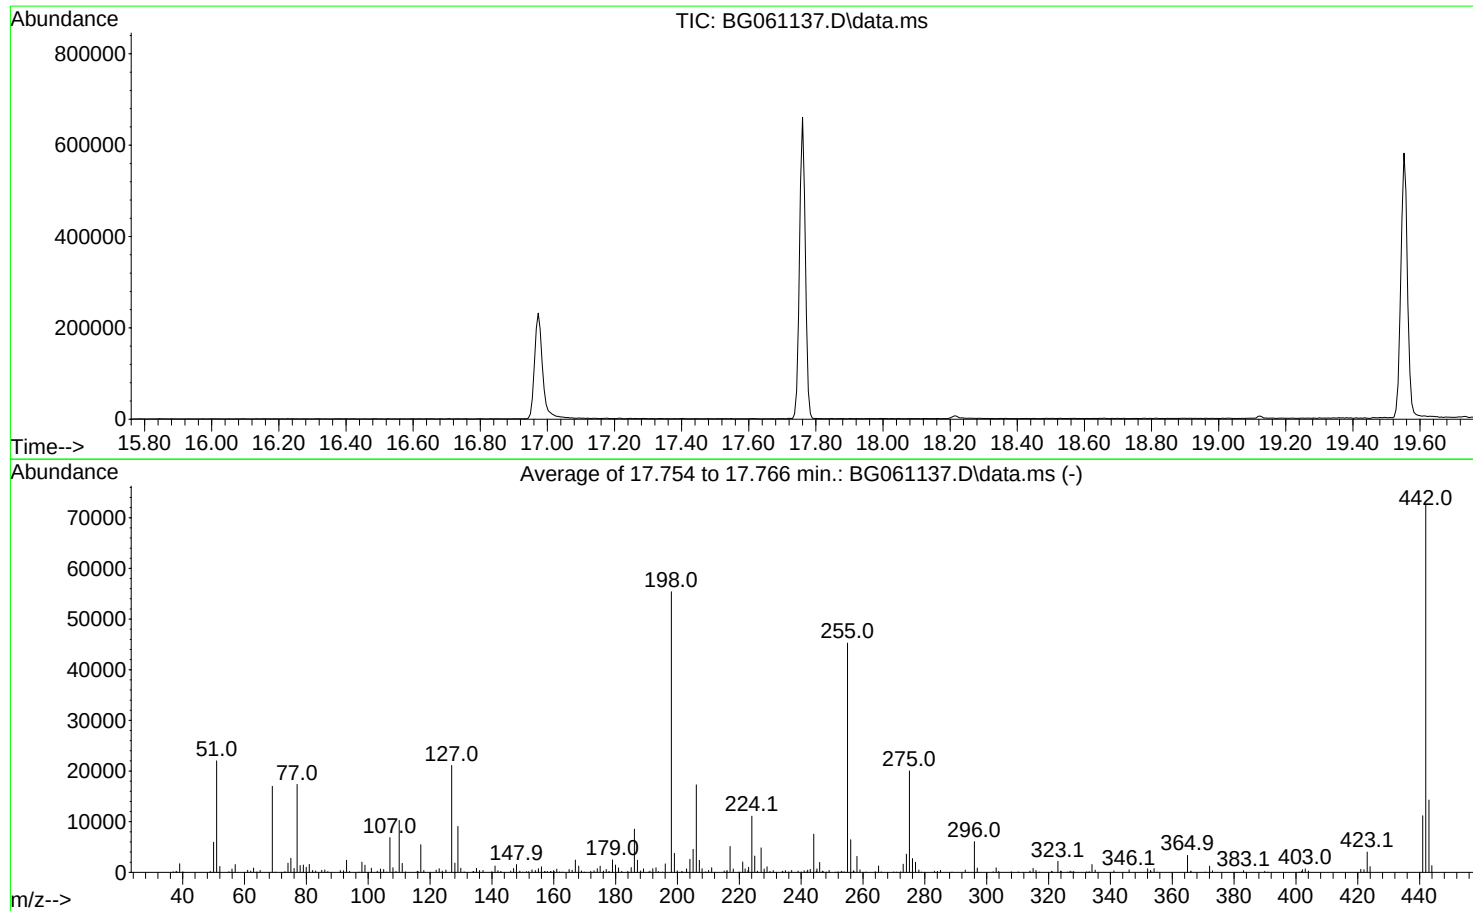

AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	22006	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.7	16993	PASS
70	69	0.00	2	0.4	66	PASS
127	198	10	80	38.1	21107	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55400	PASS
199	198	5	9	6.8	3751	PASS
275	198	10	60	36.2	20043	PASS
365	198	1	100	6.1	3362	PASS
441	198	0.01	100	20.2	11187	PASS
442	442	50	100	100.0	72616	PASS
443	442	15	24	19.7	14293	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/8/2024	BNA_G	<u>BG061137.D</u>
Compound Name	Response	Retention Time
DDT	216420	20.786
DDD	5399	20.345
DDE	569	19.846
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5968	222388	2.68

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050824\
Data File : BG061137.D
Acq On : 8 May 2024 10:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 08 11:59:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

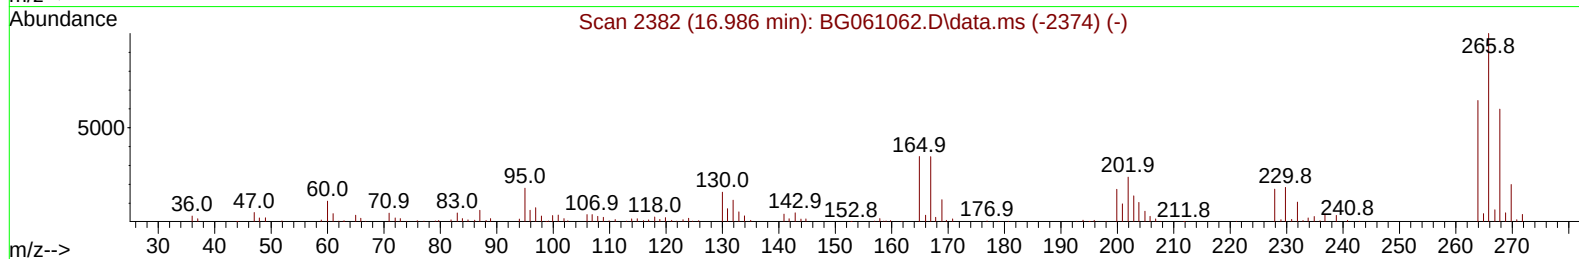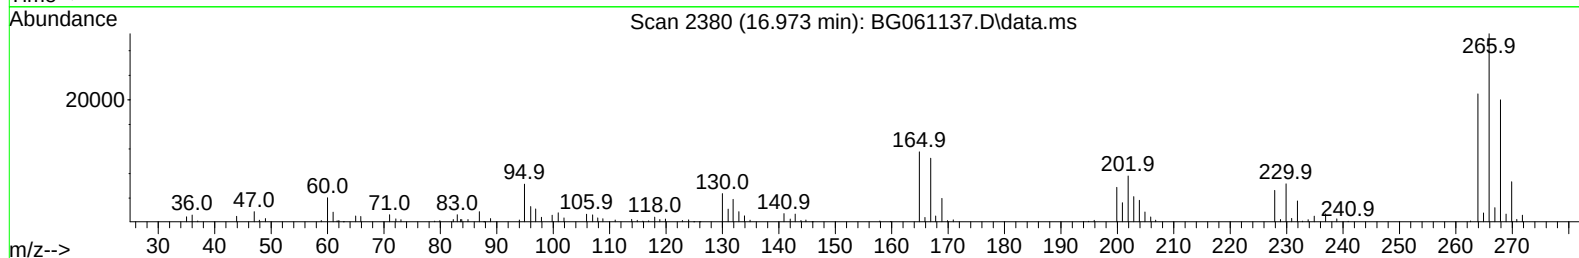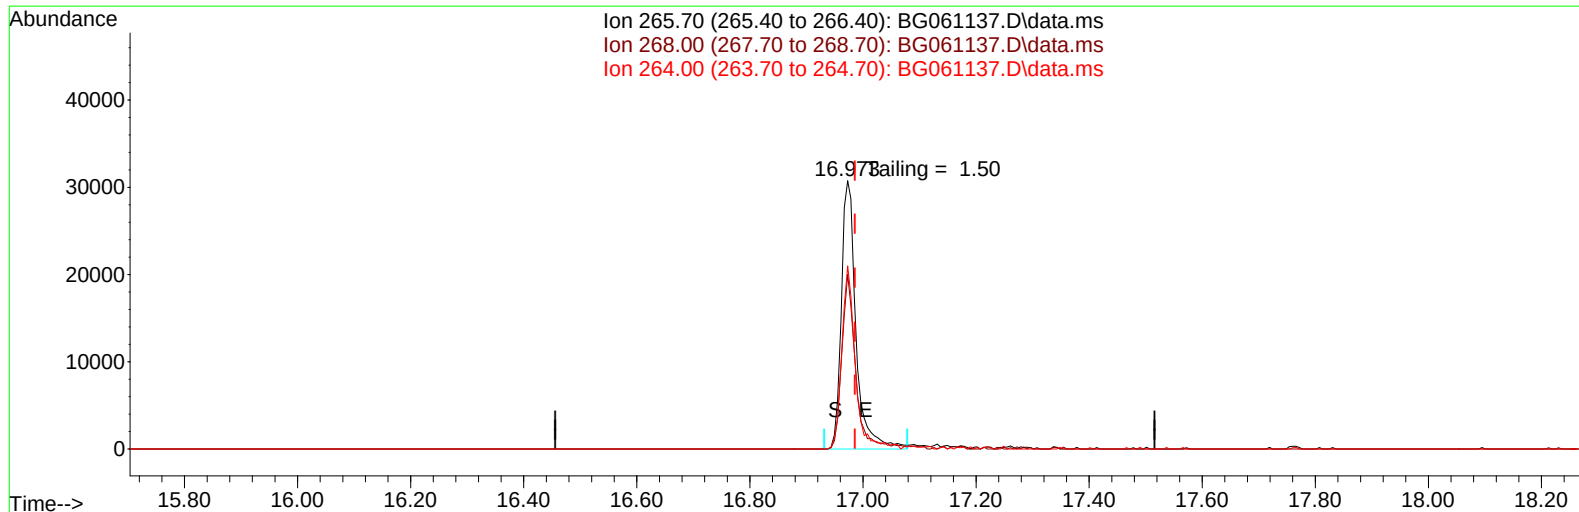

TIC: BG061137.D\data.ms

(70) Pentachlorophenol (C)

16.973min (-0.013) 20316.27 ng




response 55633

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.80	65.05
264.00	64.40	68.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050824\
Data File : BG061137.D
Acq On : 8 May 2024 10:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 08 11:59:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

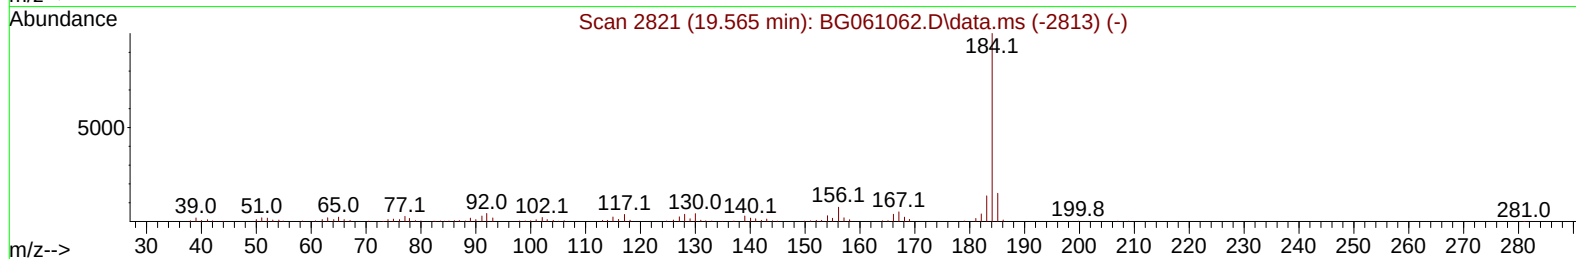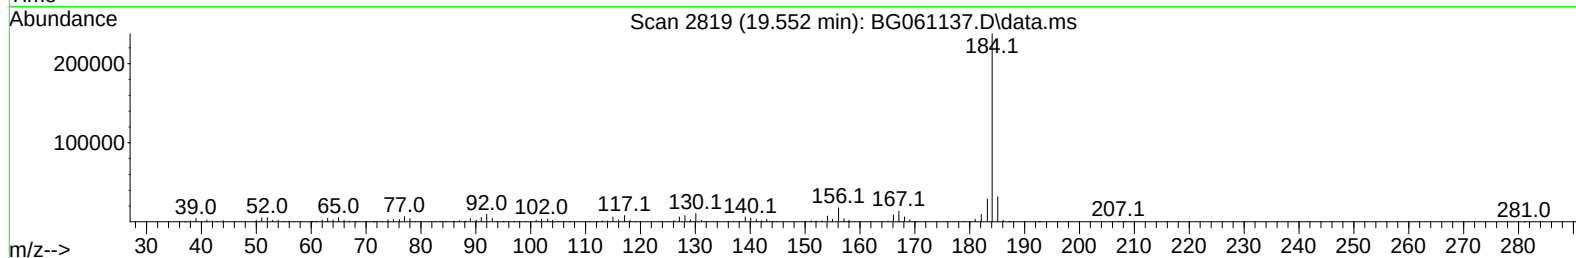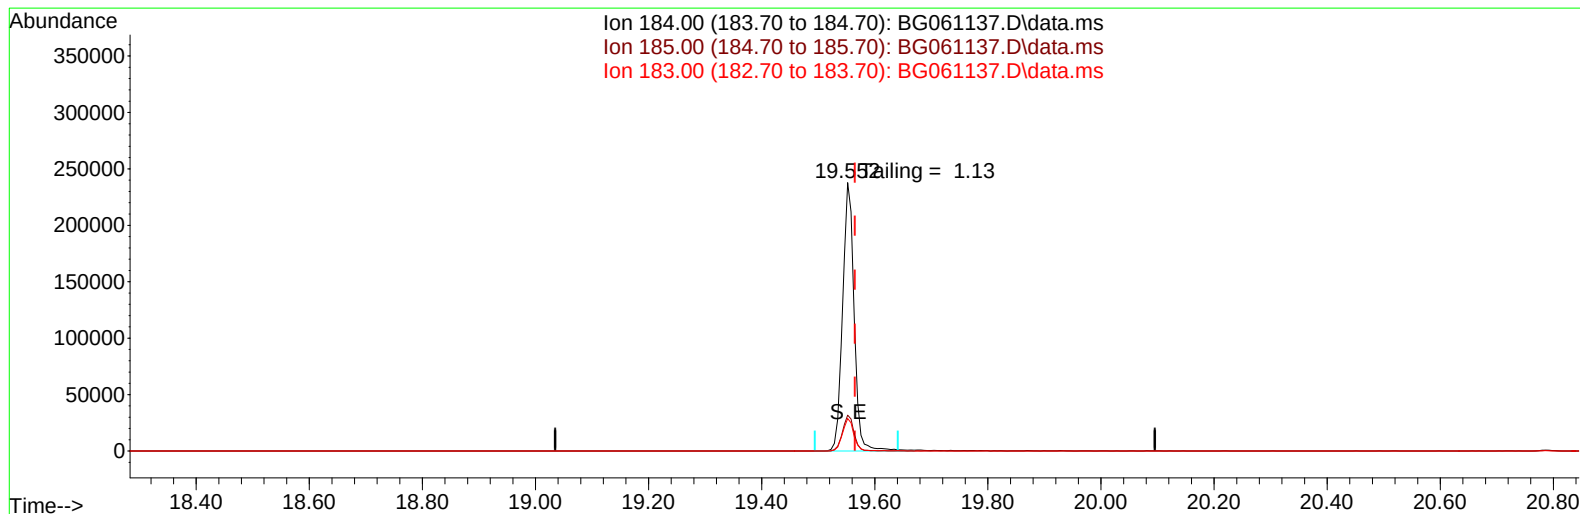

TIC: BG061137.D\data.ms

(77) Benzidine

19.552min (-0.013) 268249.19 ng m

response 336050

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.37
183.00	13.60	12.14
0.00	0.00	0.00