

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG050919\
 Data File : BG040824.D
 Acq On : 9 May 2019 20:25
 Operator : HP/JU
 Sample : PB119594BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB119594BL

Quant Time: May 10 06:45:21 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG042319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 24 05:35:33 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.14	152	49127	20.00	ng	-0.02
21) Naphthalene-d8	10.96	136	198301	20.00	ng	-0.02
39) Acenaphthene-d10	14.77	164	154225	20.00	ng	-0.02
64) Phenanthrene-d10	17.51	188	420775	20.00	ng	-0.02
76) Chrysene-d12	21.80	240	399648	20.00	ng	-0.03
87) Perylene-d12	25.15	264	285128	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.67	112	359922	129.15	ng	-0.01
7) Phenol-d6	7.28	99	529457	123.39	ng	-0.02
23) Nitrobenzene-d5	9.32	82	368738	85.92	ng	-0.02
42) 2,4,6-Tribromophenol	16.25	330	266793	125.85	ng	-0.02
45) 2-Fluorobiphenyl	13.40	172	878524	82.27	ng	-0.02
79) Terphenyl-d14	20.11	244	1720846	95.39	ng	-0.03


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG050919\
Data File : BG040824.D
Acq On : 9 May 2019 20:25
Operator : HP/JU
Sample : PB119594BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB119594BL

Quant Time: May 10 06:45:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG042319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 24 05:35:33 2019
Response via : Initial Calibration

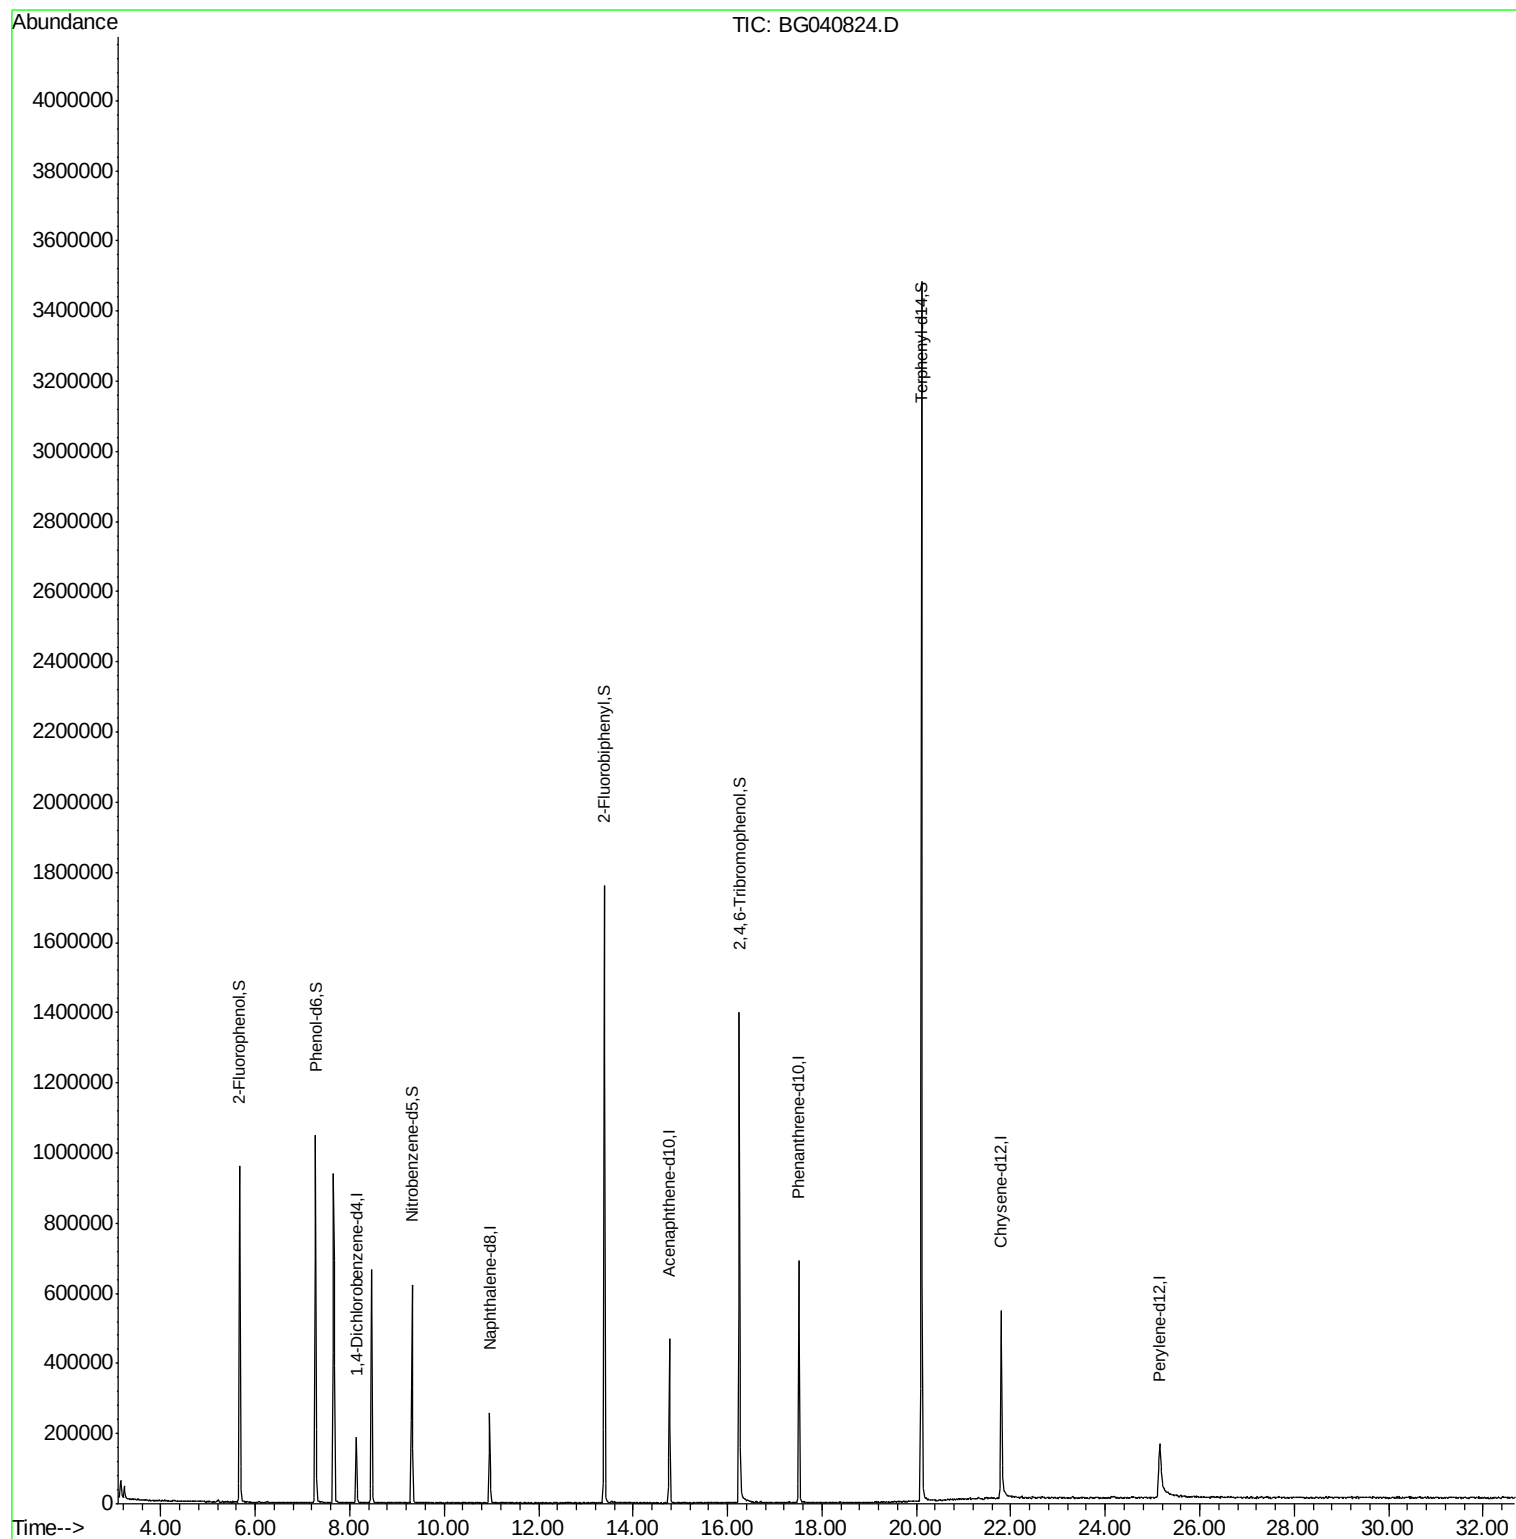

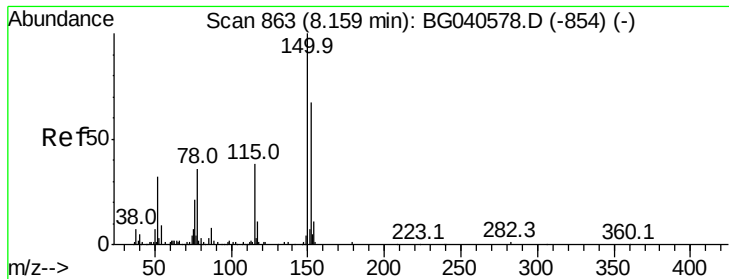


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.14 min Scan# 860
Delta R.T. -0.02 min
Lab File: BG040824.D
Acq: 9 May 2019 20:25

Instrument :
BNA_G
ClientSampleId :
PB119594BL

Tot Ion	Ratio	Lower	Upper
152	100		
150	151.0	120.2	180.2
115	56.9	46.2	69.2



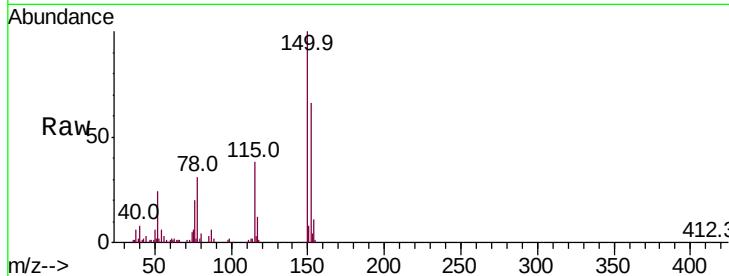


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

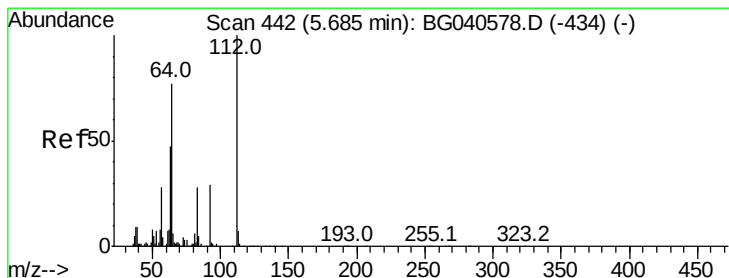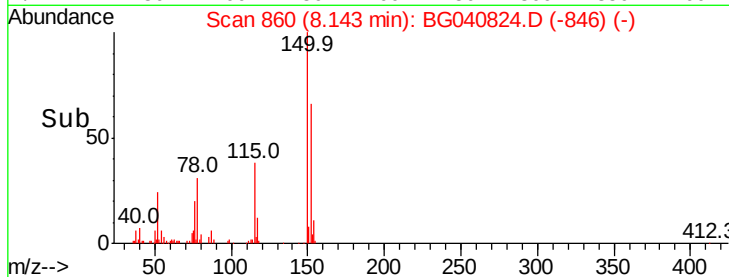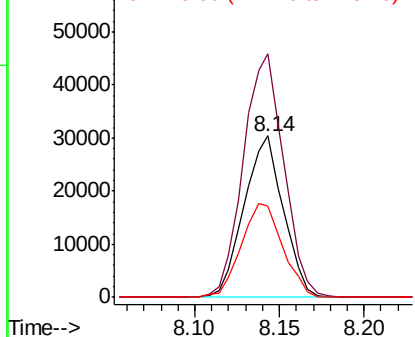

#5

2-Fluorophenol
Concen: 129.146 ng
RT: 5.67 min Scan# 439
Delta R.T. -0.01 min
Lab File: BG040824.D
Acq: 9 May 2019 20:25

Tgt Ion	Ratio	Lower	Upper
112	100		
64	72.8	61.4	92.0
63	40.9	37.8	56.6


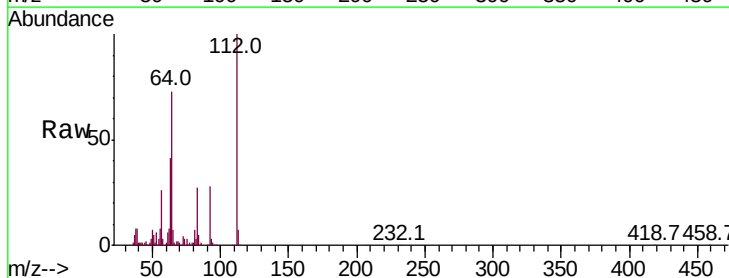



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG

Ion 63.00 (62.70 to 63.70): BG

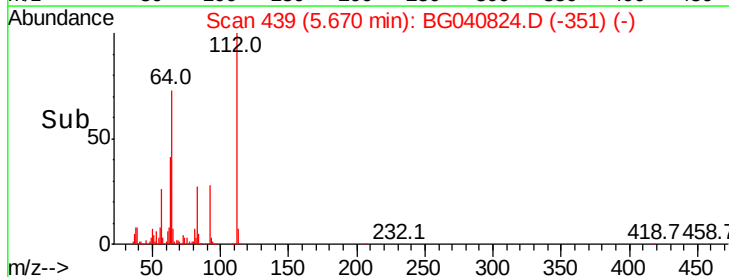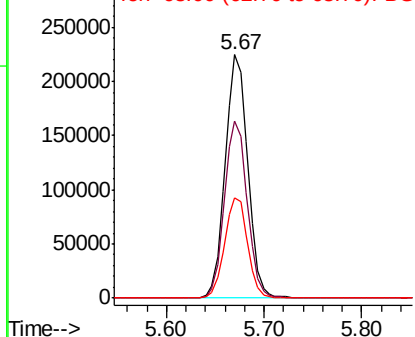

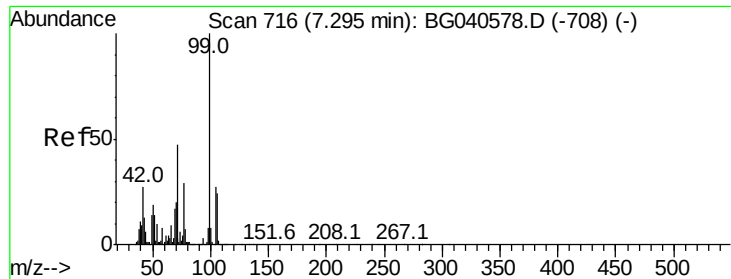

#7

Phenol-d6

Concen: 123.385 ng

RT: 7.28 min Scan# 713

Delta R.T. -0.02 min

Lab File: BG040824.D

Acq: 9 May 2019 20:25

Instrument :

BNA_G

ClientSampleId :

PB119594BL


Tot Ion: 99 Resp: 529457

Ion Ratio Lower Upper




99 100

42 23.6 21.8 32.8

71 44.8 38.6 57.8

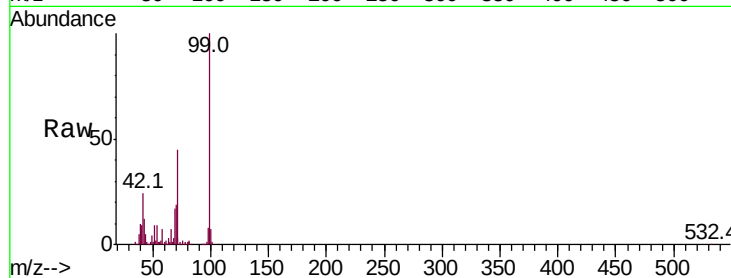

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

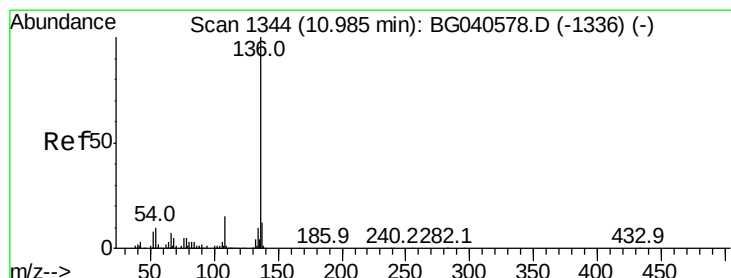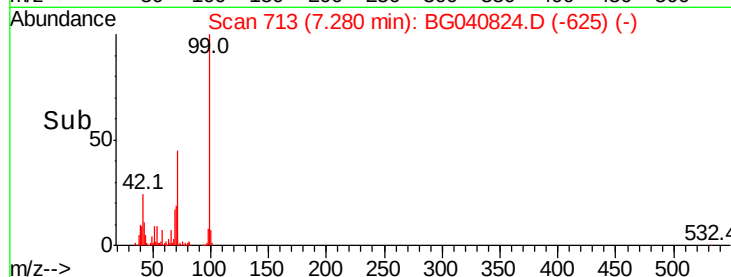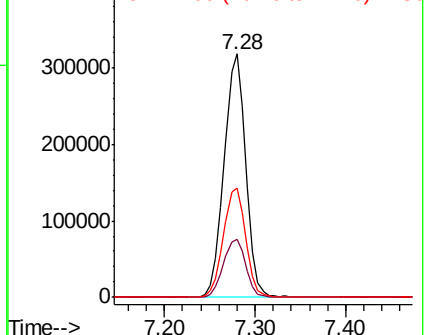

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.96 min Scan# 1340

Delta R.T. -0.02 min

Lab File: BG040824.D

Acq: 9 May 2019 20:25

Tgt Ion: 136 Resp: 198301


Ion Ratio Lower Upper

136 100



137 11.3 9.7 14.5


54 10.2 8.6 12.8

68 5.8 4.8 7.2

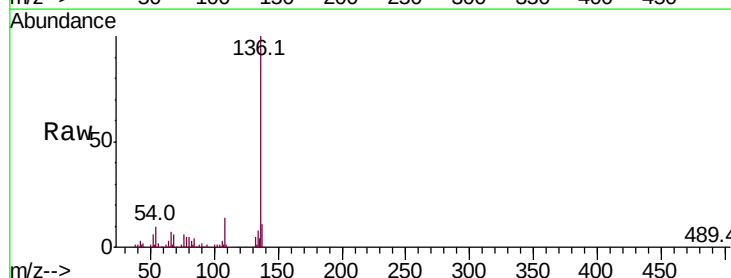

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



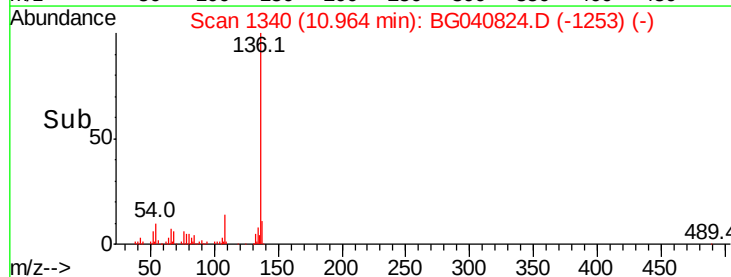
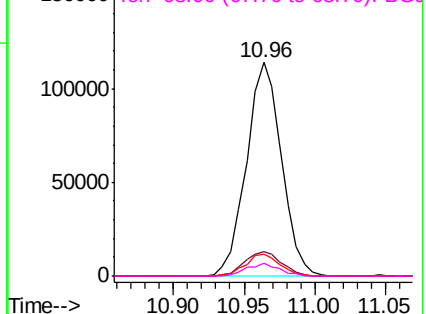


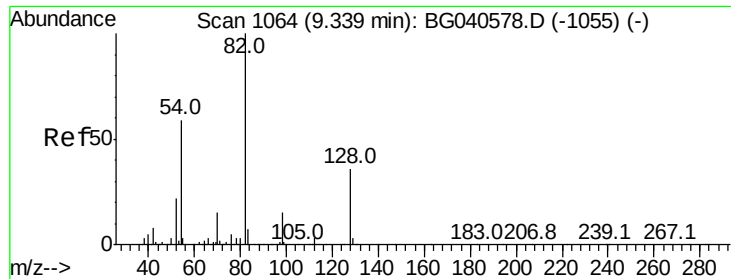

#23
 Nitrobenzene-d5
 Concen: 85.920 ng
 RT: 9.32 min Scan# 1060
 Delta R.T. -0.02 min
 Lab File: BG040824.D
 Acq: 9 May 2019 20:25




Instrument :
 BNA_G
 ClientSampleId :
 PB119594BL


Tot Ion	82	Resp	368738
Ion Ratio	Lower	Upper	
82	100		
128	35.6	28.9	43.3
54	54.9	47.2	70.8

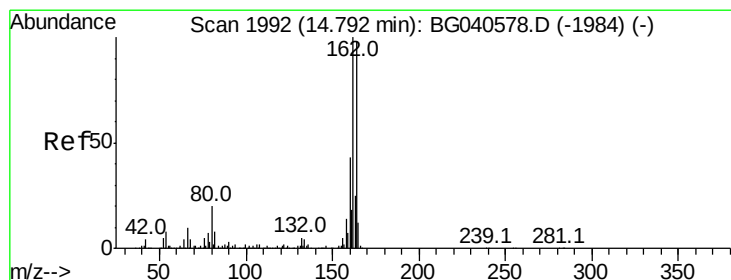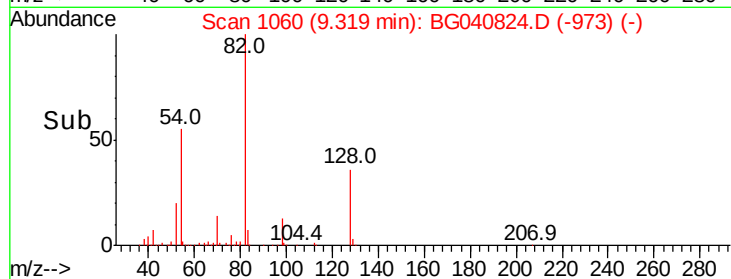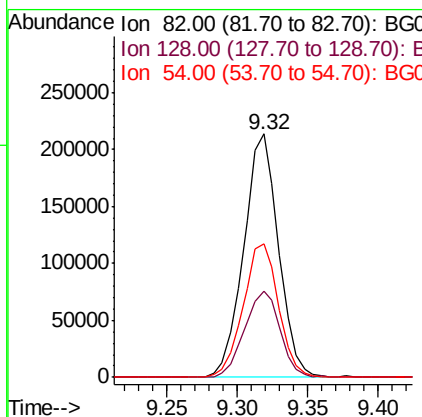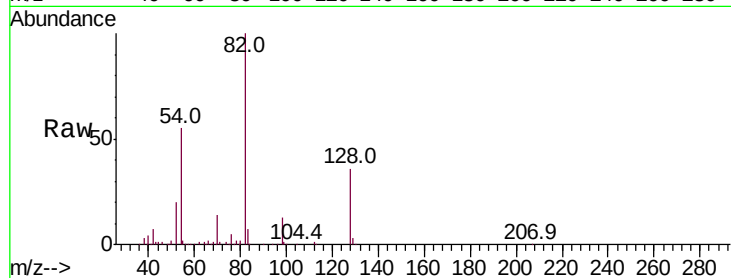

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.77 min Scan# 1988
 Delta R.T. -0.02 min
 Lab File: BG040824.D
 Acq: 9 May 2019 20:25

Tgt Ion	164	Resp	154225
Ion Ratio	Lower	Upper	
164	100		
162	106.6	81.9	122.9
160	44.3	35.4	53.2

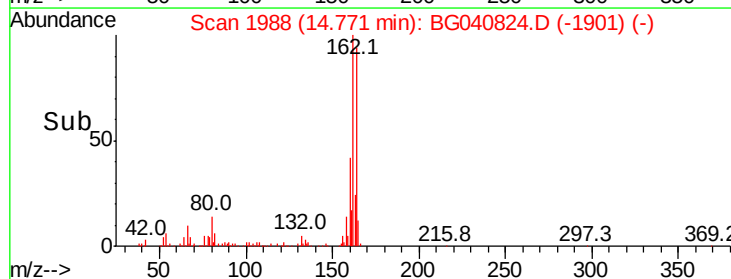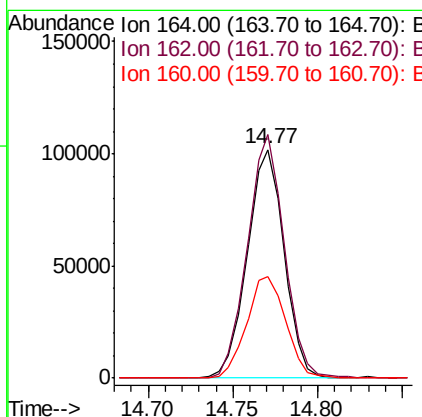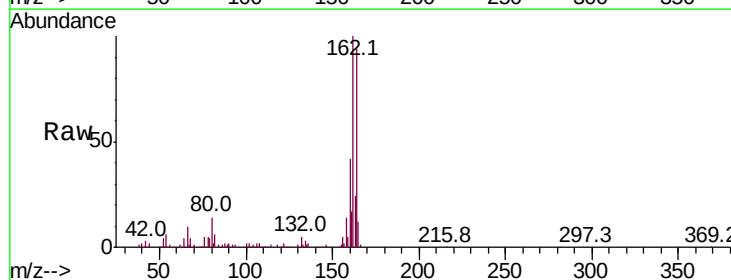

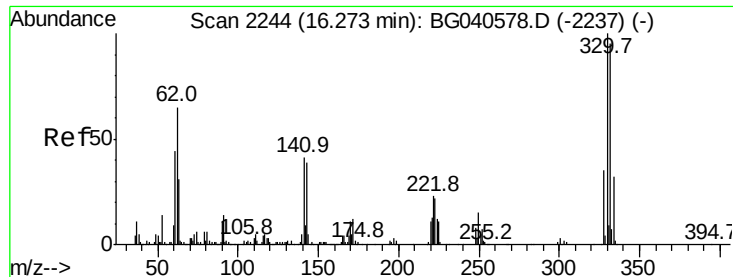

#42

2,4,6-Tribromophenol

Concen: 125.854 ng

RT: 16.25 min Scan# 2240

Delta R.T. -0.02 min

Lab File: BG040824.D

Acq: 9 May 2019 20:25

Instrument :

BNA_G

ClientSampleId :

PB119594BL


Tot Ion:330 Resp: 266793

Ion Ratio Lower Upper

330 100

332 95.5 75.9 113.9




141 36.6 32.4 48.6

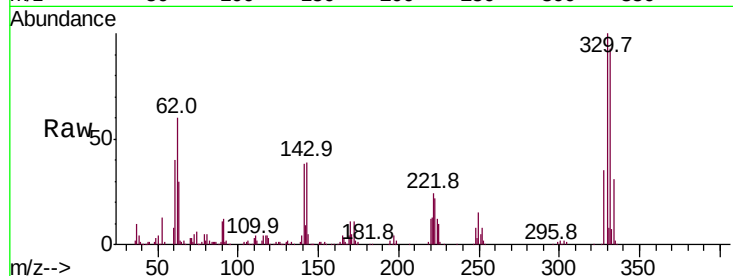

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

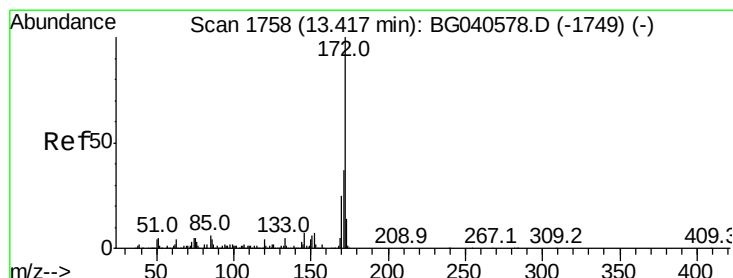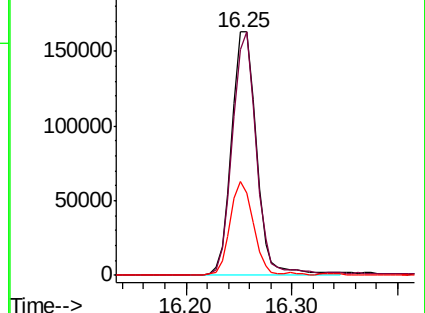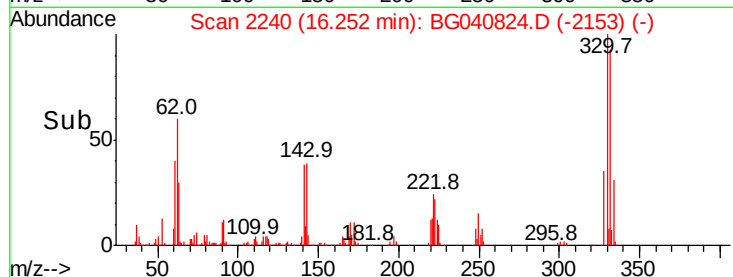

#45

2-Fluorobiphenyl

Concen: 82.267 ng

RT: 13.40 min Scan# 1754

Delta R.T. -0.02 min

Lab File: BG040824.D

Acq: 9 May 2019 20:25


Tgt Ion:172 Resp: 878524

Ion Ratio Lower Upper

172 100

171 38.0 29.4 44.2



170 24.9 19.9 29.9

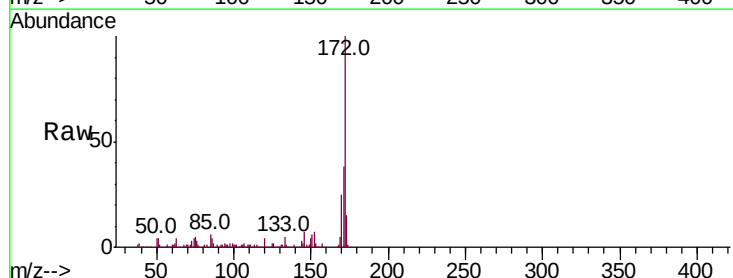


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

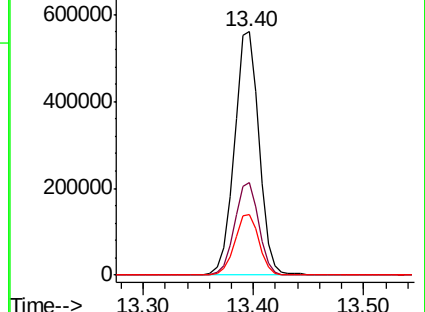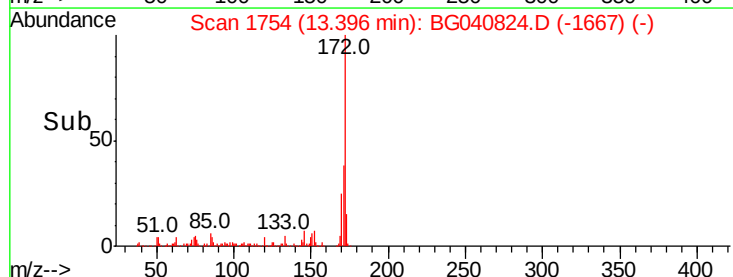

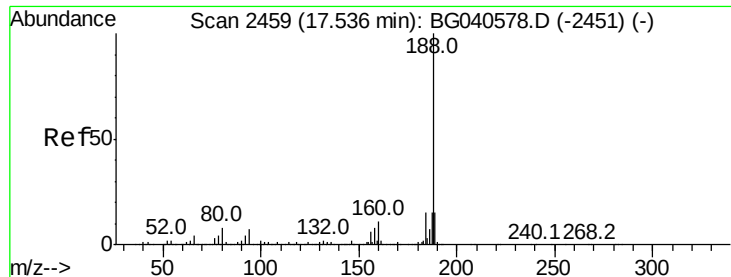

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.51 min Scan# 2455

Delta R.T. -0.02 min

Lab File: BG040824.D

Acq: 9 May 2019 20:25

Instrument :

BNA_G

ClientSampleId :

PB119594BL


Tot Ion:188 Resp: 420775

Ion Ratio Lower Upper

188 100

94 5.1 5.6 8.4#




80 7.0 6.4 9.6

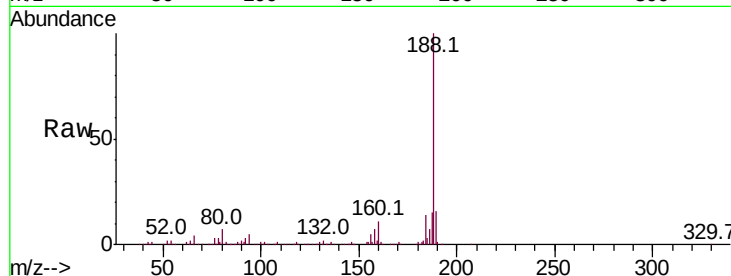

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

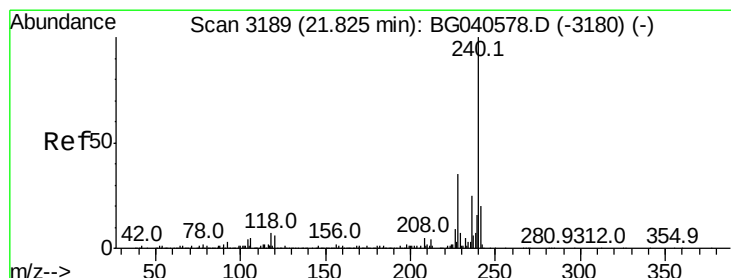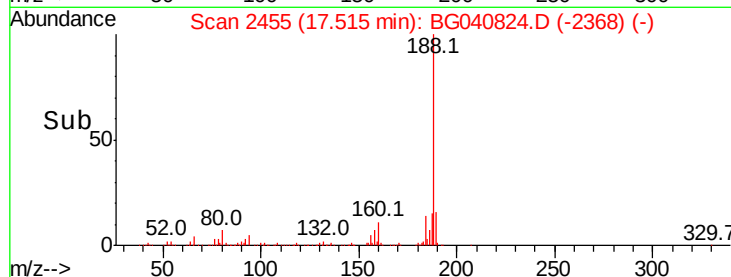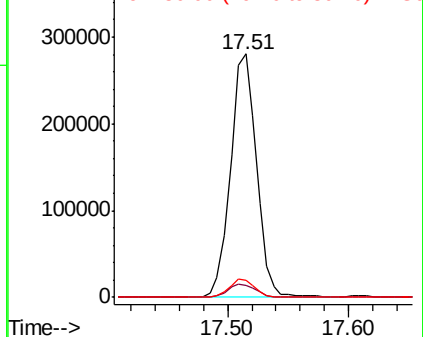

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.80 min Scan# 3184

Delta R.T. -0.03 min

Lab File: BG040824.D

Acq: 9 May 2019 20:25


Tgt Ion:240 Resp: 399648

Ion Ratio Lower Upper

240 100

120 5.0 5.0 7.6#



236 25.7 20.3 30.5

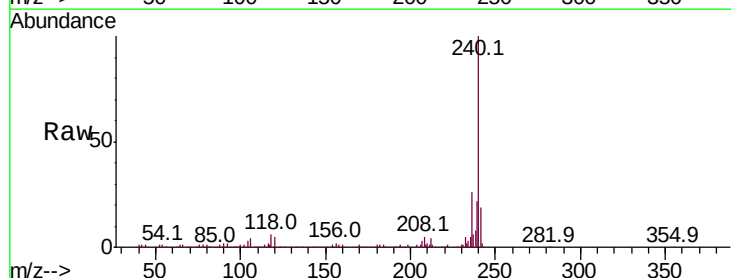


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

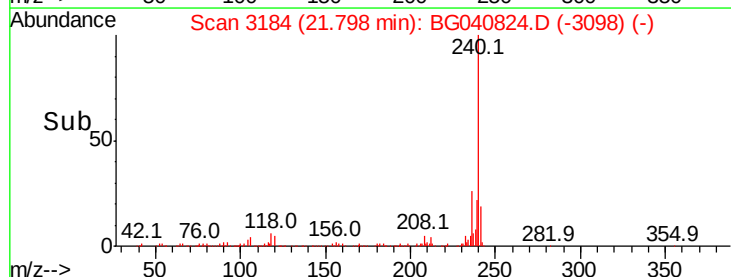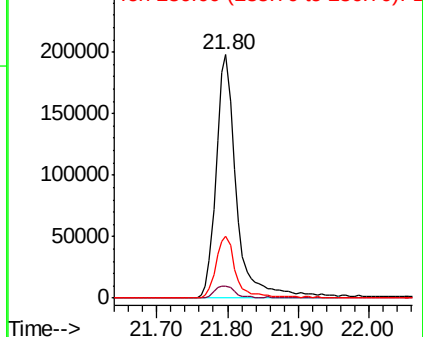

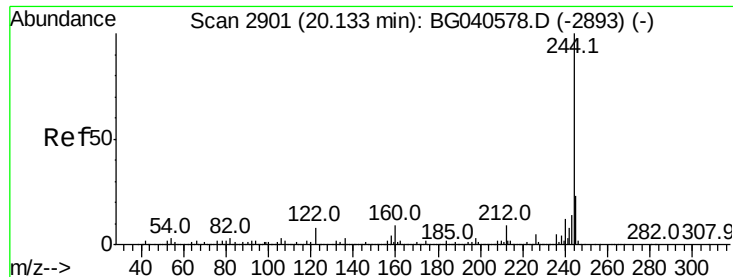

#79

Terphenyl-d14

Concen: 95.394 ng

RT: 20.11 min Scan# 2896

Delta R.T. -0.03 min

Lab File: BG040824.D

Acq: 9 May 2019 20:25

Instrument :


BNA_G

ClientSampleId :

PB119594BL

Tot Ion:244 Resp: 1720846

Ion	Ratio	Lower	Upper
244	100		
212	8.9	7.2	10.8
122	8.0	6.6	10.0



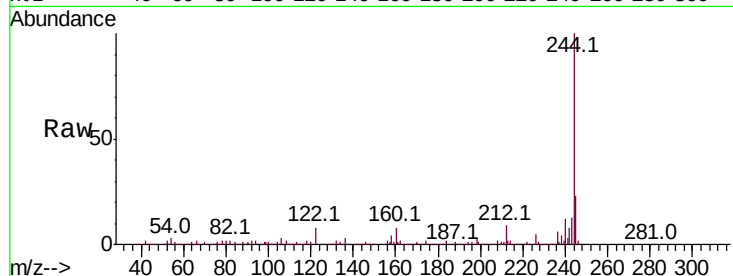


Abundance

Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

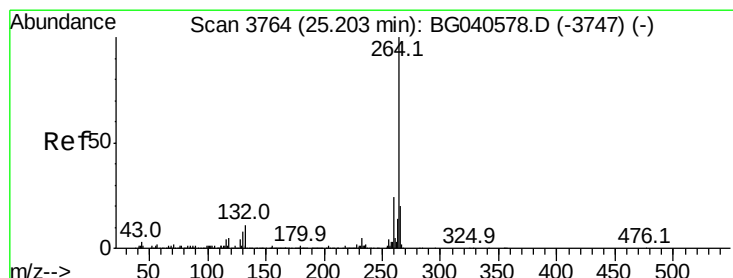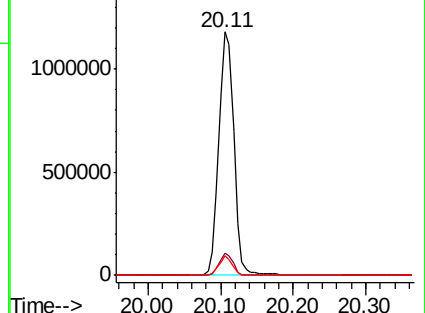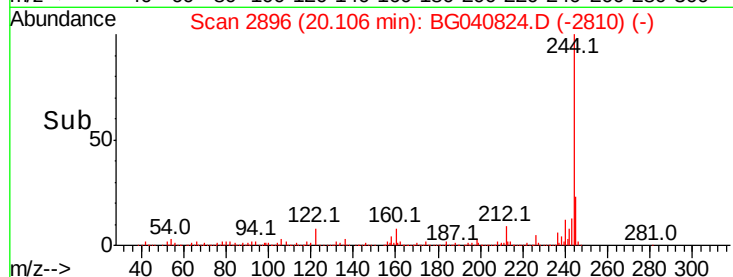

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.15 min Scan# 3754


Delta R.T. -0.06 min

Lab File: BG040824.D

Acq: 9 May 2019 20:25

Tgt Ion:264 Resp: 285128

Ion	Ratio	Lower	Upper
264	100		
260	22.3	19.2	28.8
265	19.3	16.6	25.0

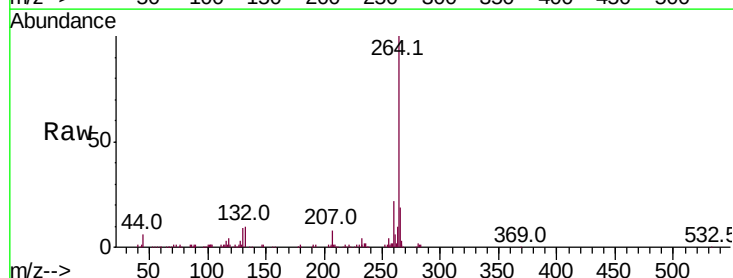

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

