

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG050919\
 Data File : BG040842.D
 Acq On : 10 May 2019 9:01
 Operator : HP/JU
 Sample : PB119587BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB119587BL

Quant Time: May 10 15:18:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG042319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 24 05:35:33 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.14	152	57232	20.00	ng	-0.02
21) Naphthalene-d8	10.97	136	230525	20.00	ng	-0.02
39) Acenaphthene-d10	14.77	164	170843	20.00	ng	-0.02
64) Phenanthrene-d10	17.51	188	426538	20.00	ng	-0.02
76) Chrysene-d12	21.80	240	413723	20.00	ng	-0.03
87) Perylene-d12	25.16	264	407813	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.67	112	411388	126.71	ng	-0.01
7) Phenol-d6	7.28	99	599540	119.93	ng	-0.01
23) Nitrobenzene-d5	9.32	82	420688	84.32	ng	-0.02
42) 2,4,6-Tribromophenol	16.26	330	321538	136.93	ng	-0.02
45) 2-Fluorobiphenyl	13.39	172	970727	82.06	ng	-0.02
79) Terphenyl-d14	20.11	244	1670189	89.44	ng	-0.02


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG050919\
Data File : BG040842.D
Acq On : 10 May 2019 9:01
Operator : HP/JU
Sample : PB119587BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB119587BL

Quant Time: May 10 15:18:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG042319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 24 05:35:33 2019
Response via : Initial Calibration

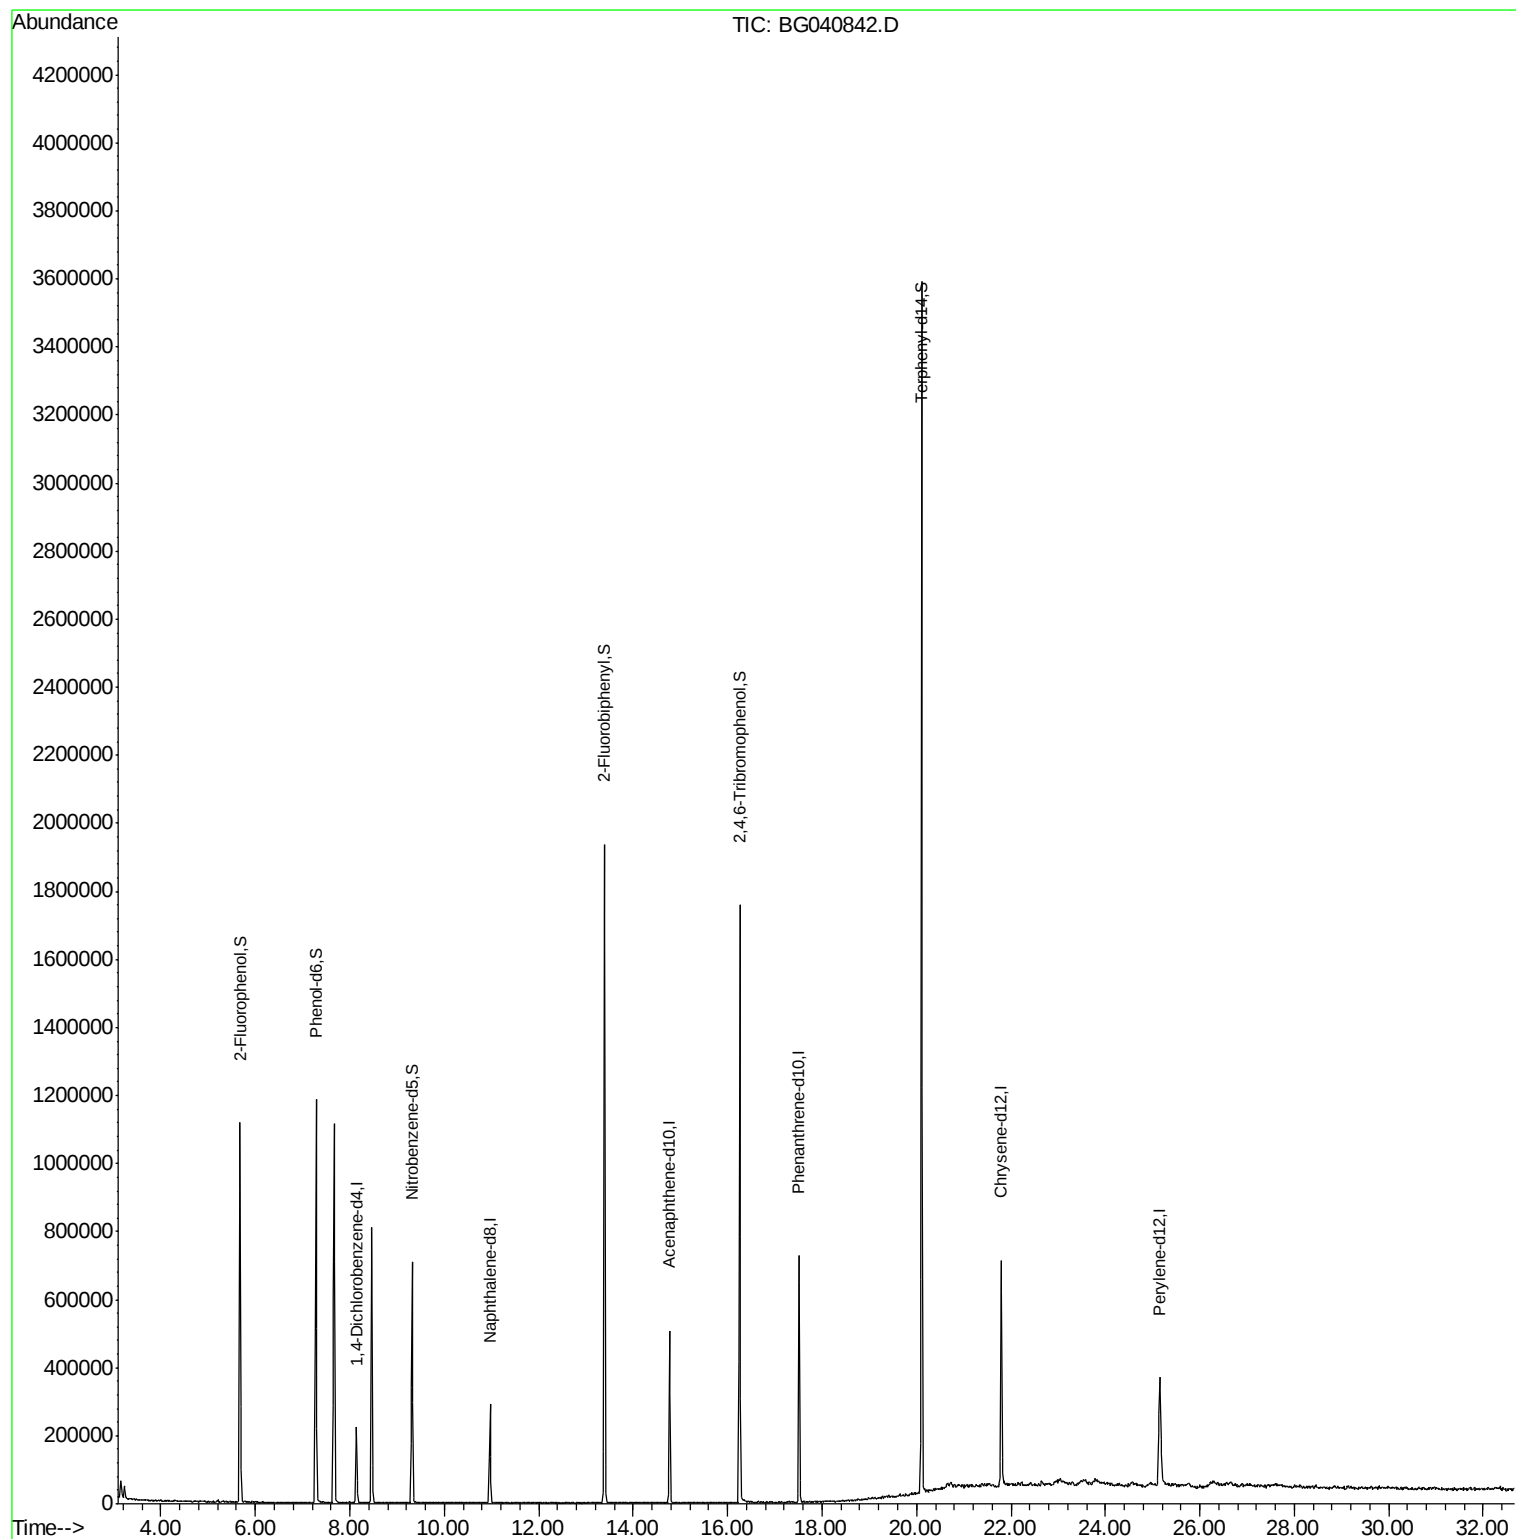

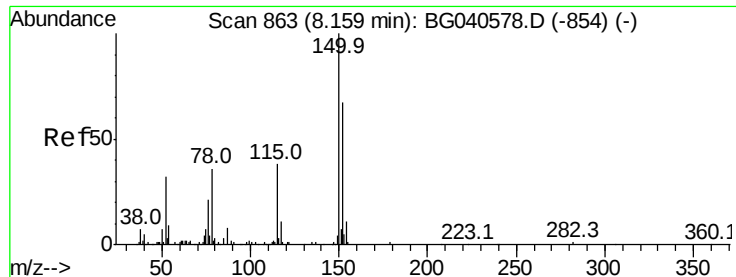


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.14 min Scan# 860
Delta R.T. -0.02 min
Lab File: BG040842.D
Acq: 10 May 2019 9:01

Instrument :
BNA_G
ClientSampleId :
PB119587BL

Tot Ion	Ratio	Lower	Upper
152	100		
150	148.0	120.2	180.2
115	52.5	46.2	69.2



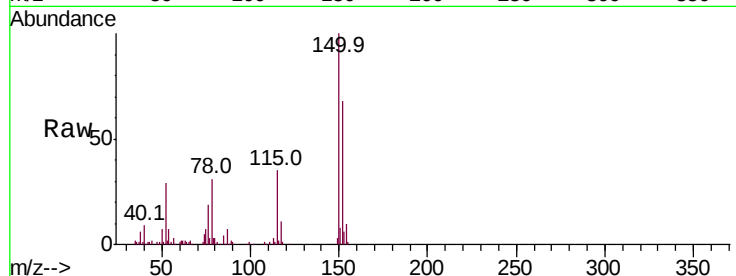


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

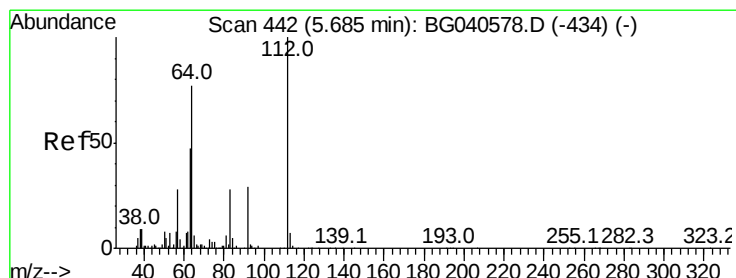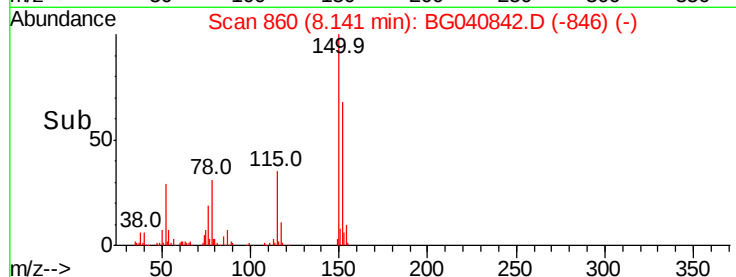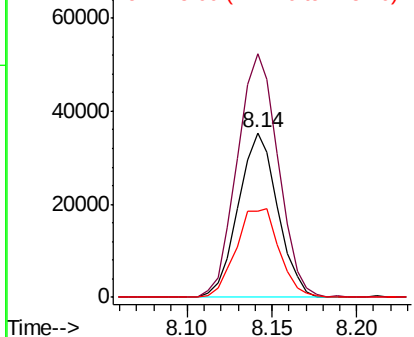

#5

2-Fluorophenol
Concen: 126.709 ng
RT: 5.67 min Scan# 440
Delta R.T. -0.01 min
Lab File: BG040842.D
Acq: 10 May 2019 9:01

Tgt Ion	Ratio	Lower	Upper
112	100		
64	71.6	61.4	92.0
63	42.6	37.8	56.6


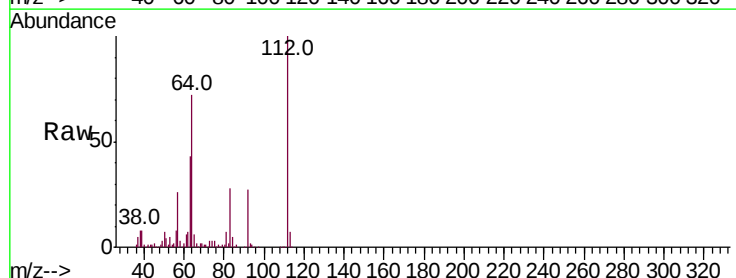



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

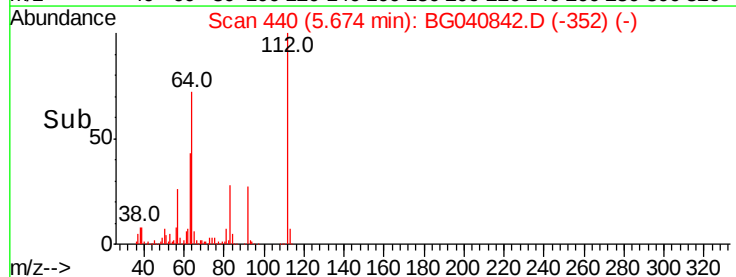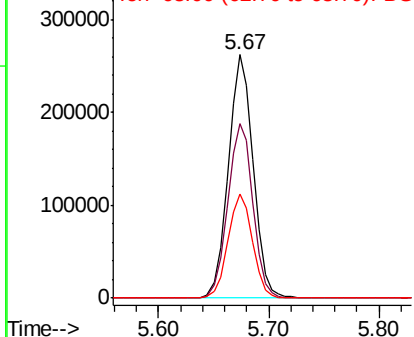

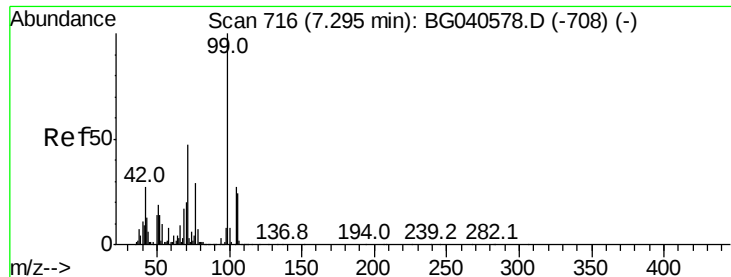

#7

Phenol-d6

Concen: 119.931 ng

RT: 7.28 min Scan# 714

Delta R.T. -0.01 min

Lab File: BG040842.D

Acq: 10 May 2019 9:01

Instrument :

BNA_G

ClientSampled :

PB119587BL


Tot Ion: 99 Resp: 599540

Ion Ratio Lower Upper

99 100

42 25.4 21.8 32.8




71 47.1 38.6 57.8

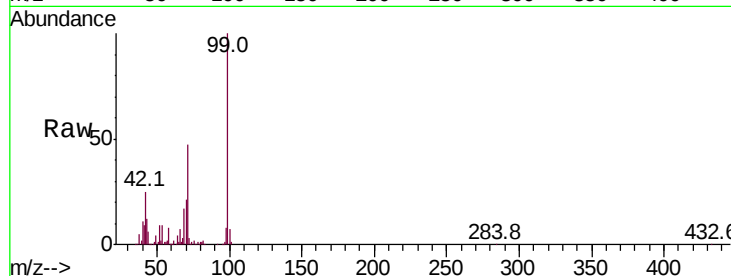

Abundance Ion 99.00 (98.70 to 99.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 71.00 (70.70 to 71.70): BGC

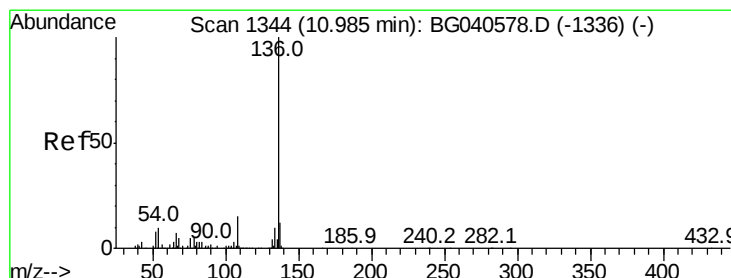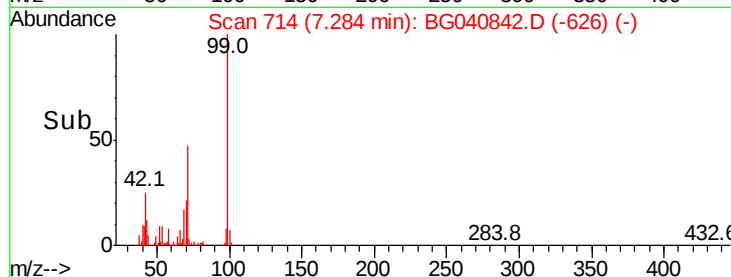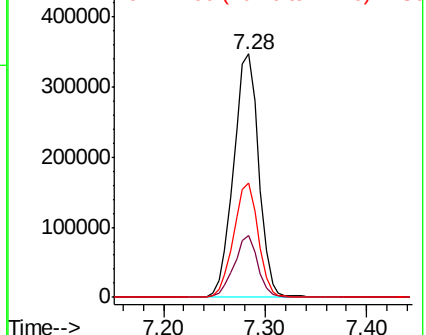

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.97 min Scan# 1341

Delta R.T. -0.02 min

Lab File: BG040842.D

Acq: 10 May 2019 9:01

Tgt Ion: 136 Resp: 230525


Ion Ratio Lower Upper

136 100

137 11.3 9.7 14.5

54 9.2 8.6 12.8

68 5.4 4.8 7.2


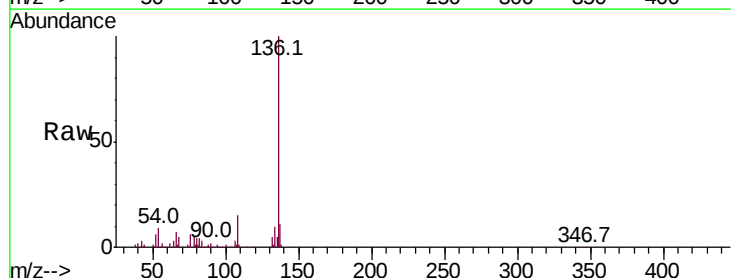



Abundance Ion 136.00 (135.70 to 136.70): BGC

Ion 137.00 (136.70 to 137.70): BGC

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC



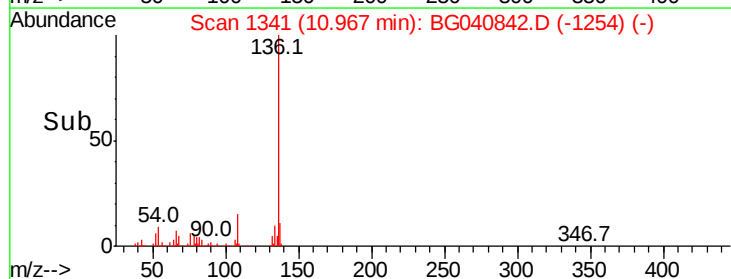
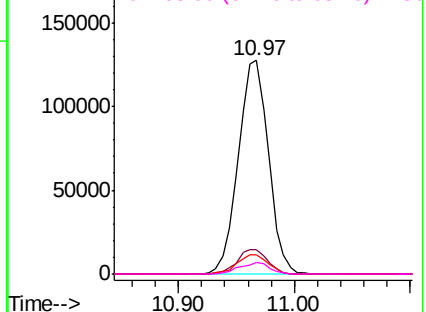


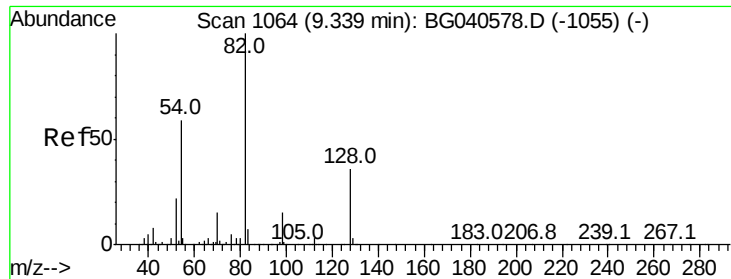

#23
Nitrobenzene-d5
Concen: 84.322 ng
RT: 9.32 min Scan# 1060
Delta R.T. -0.02 min
Lab File: BG040842.D
Acq: 10 May 2019 9:01




Instrument :
BNA_G
ClientSampleId :
PB119587BL


Tot Ion	Ratio	Lower	Upper
82	100		
128	37.5	28.9	43.3
54	55.6	47.2	70.8

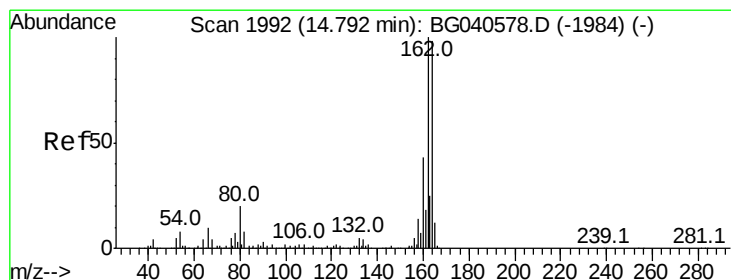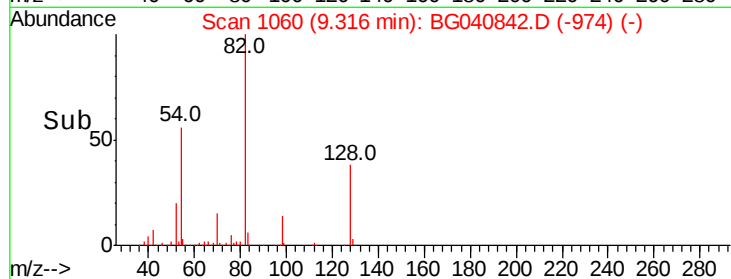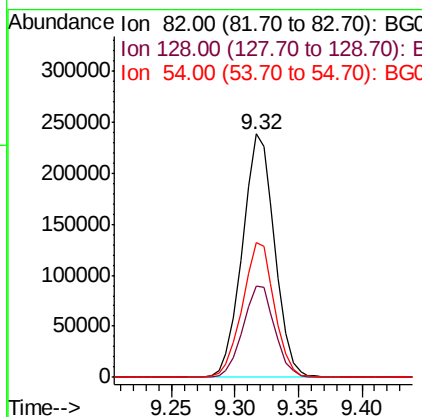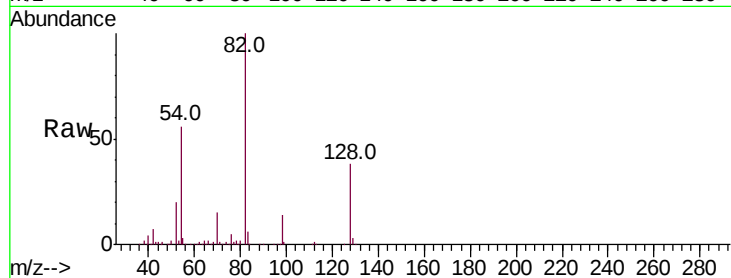

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.77 min Scan# 1988
Delta R.T. -0.02 min
Lab File: BG040842.D
Acq: 10 May 2019 9:01

Tgt Ion	Ratio	Lower	Upper
164	100		
162	105.3	81.9	122.9
160	44.9	35.4	53.2

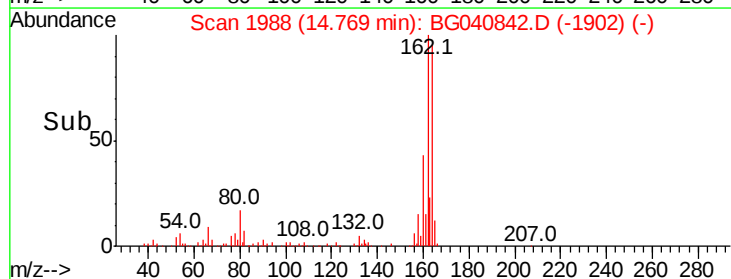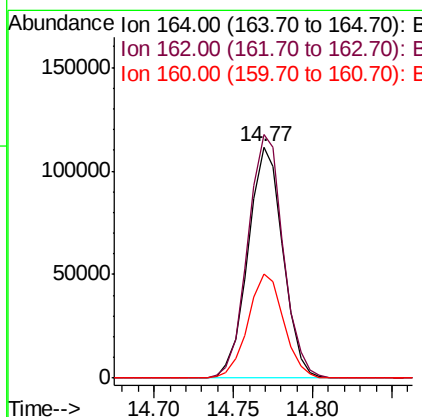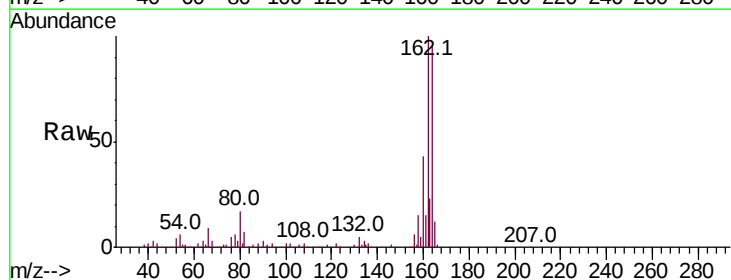


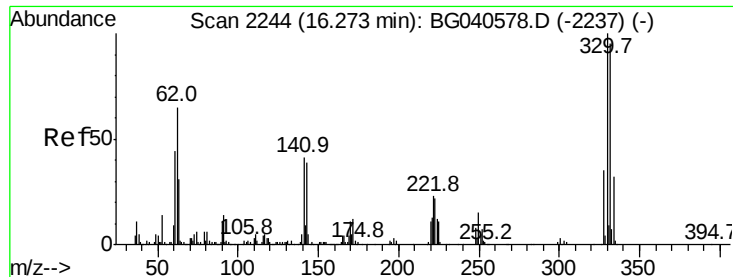




#42
2,4,6-Tribromophenol
Concen: 136.925 ng
RT: 16.26 min Scan# 2241
Delta R.T. -0.02 min
Lab File: BG040842.D
Acq: 10 May 2019 9:01

Instrument :
BNA_G
ClientSampled :
PB119587BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	94.8	75.9	113.9
141	35.9	32.4	48.6

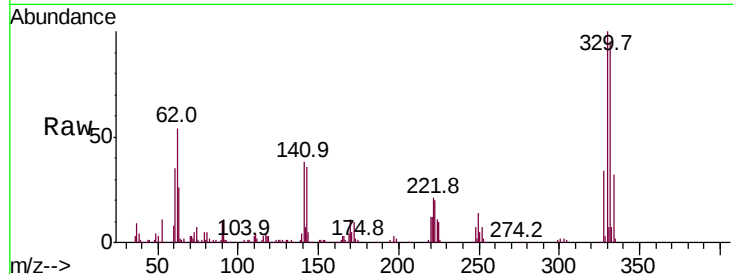


Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

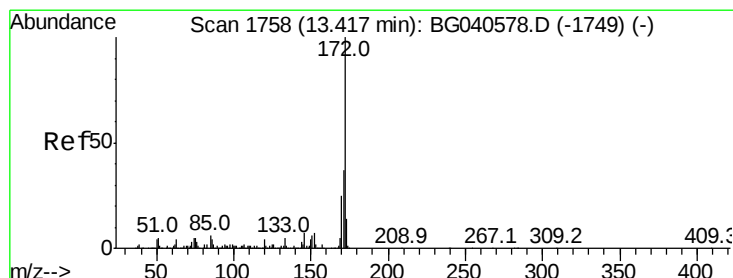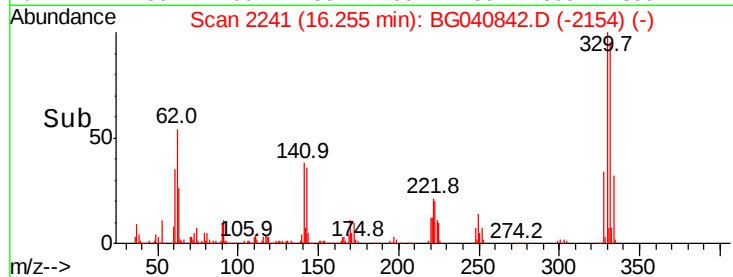
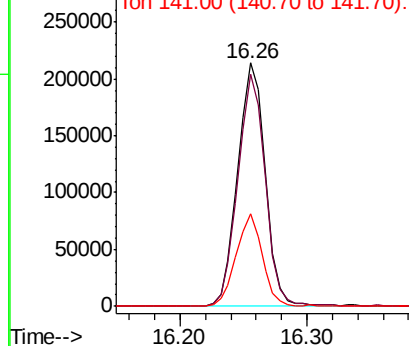



#45
2-Fluorobiphenyl
Concen: 82.059 ng
RT: 13.39 min Scan# 1754
Delta R.T. -0.02 min
Lab File: BG040842.D
Acq: 10 May 2019 9:01

Tgt Ion	Ratio	Lower	Upper
172	100		
171	39.0	29.4	44.2
170	26.1	19.9	29.9

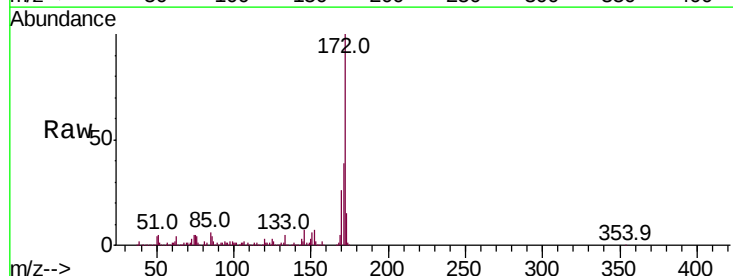

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

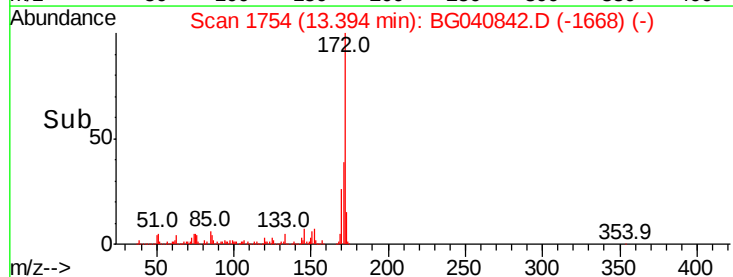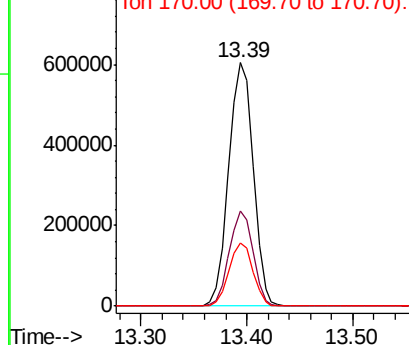

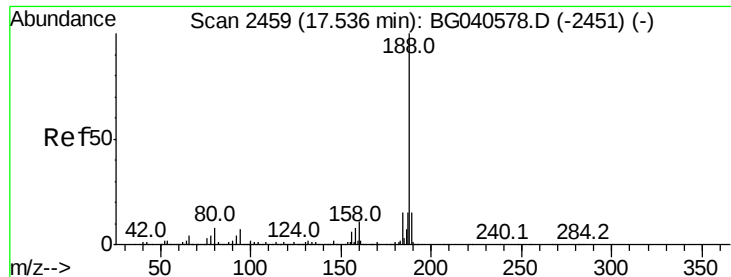

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.51 min Scan# 2455

Delta R.T. -0.02 min

Lab File: BG040842.D

Acq: 10 May 2019 9:01

Instrument :

BNA_G

ClientSampleId :

PB119587BL


Tot Ion:188 Resp: 426538

Ion Ratio Lower Upper

188 100

94 6.2 5.6 8.4




80 7.5 6.4 9.6

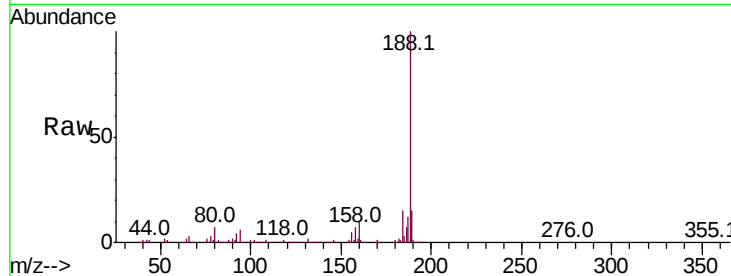

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

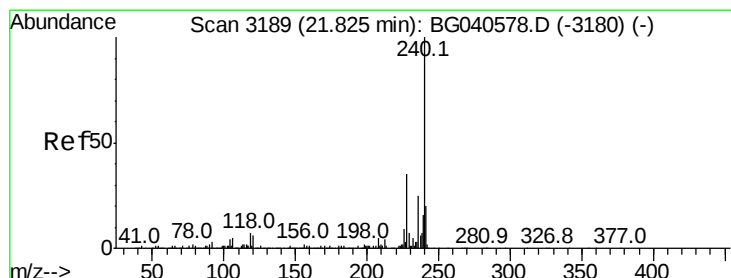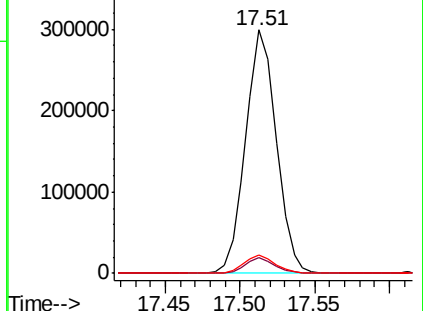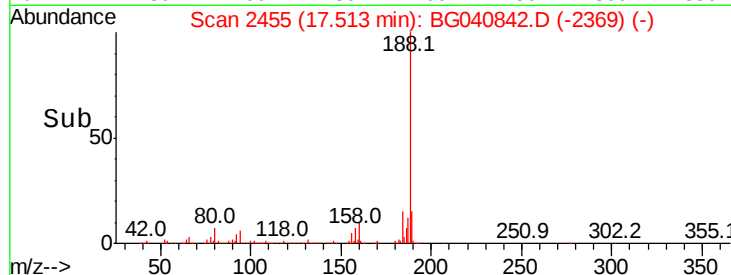

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.80 min Scan# 3184

Delta R.T. -0.03 min

Lab File: BG040842.D

Acq: 10 May 2019 9:01


Tgt Ion:240 Resp: 413723

Ion Ratio Lower Upper

240 100

120 4.5 5.0 7.6#



236 25.0 20.3 30.5

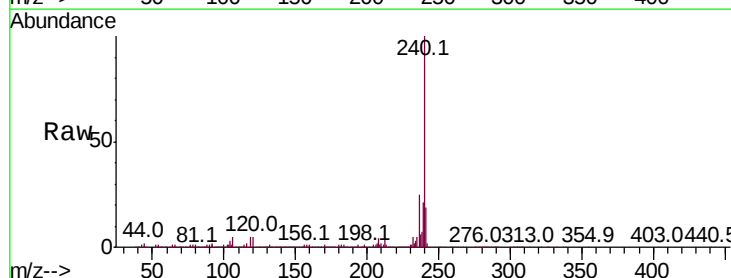


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

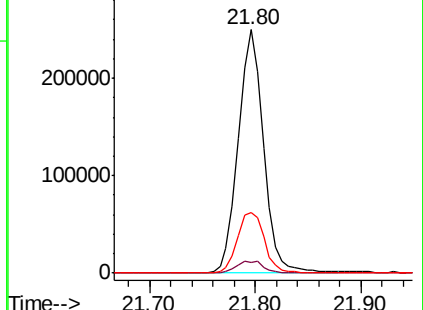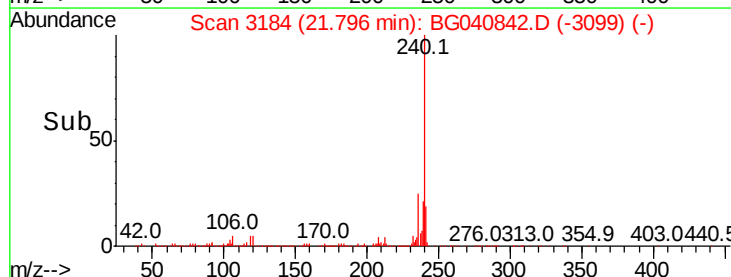

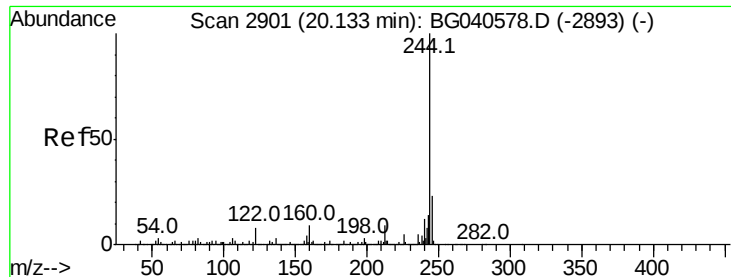

#79

Terphenyl-d14

Concen: 89.436 ng

RT: 20.11 min Scan# 2897

Delta R.T. -0.02 min

Lab File: BG040842.D

Acq: 10 May 2019 9:01

Instrument :

BNA_G

ClientSampleId :

PB119587BL


Tot Ion:244 Resp: 1670189

Ion Ratio Lower Upper




244 100

212 9.3 7.2 10.8

122 7.5 6.6 10.0

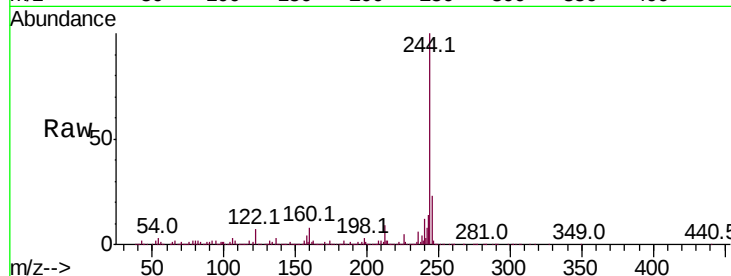

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

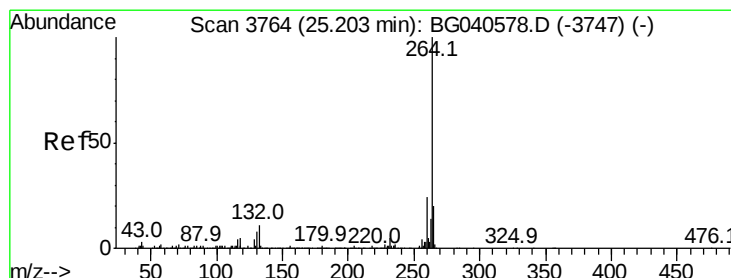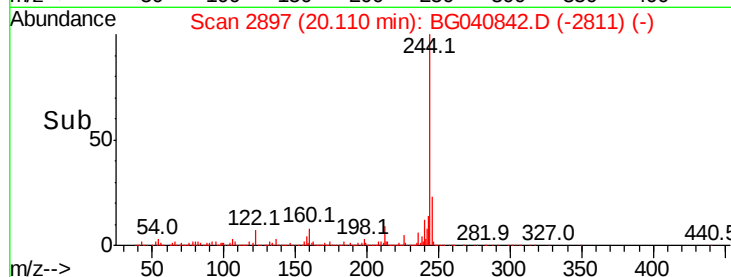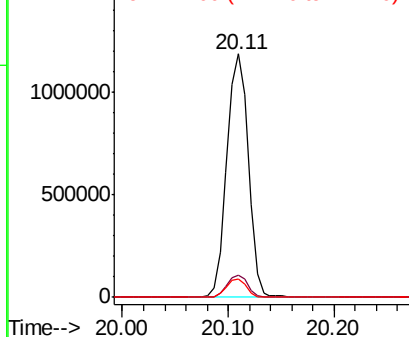

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.16 min Scan# 3756

Delta R.T. -0.05 min

Lab File: BG040842.D

Acq: 10 May 2019 9:01


Tgt Ion:264 Resp: 407813

Ion Ratio Lower Upper

264 100

260 22.5 19.2 28.8

265 22.4 16.6 25.0

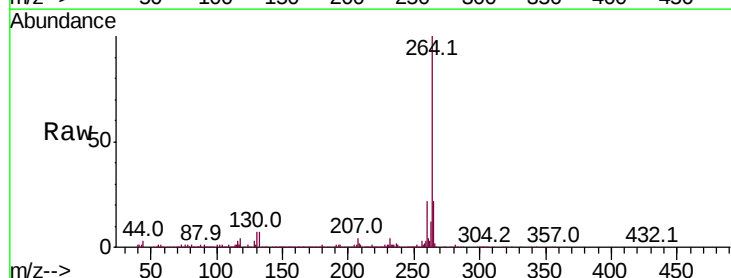

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

