

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG050919\
 Data File : BG040823.D
 Acq On : 9 May 2019 19:47
 Operator : HP/JU
 Sample : PB119587BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB119587BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.153	6	11	17	rBV	44028	72263	1.62%	0.388%
2	5.674	431	440	449	rBV	872874	1397003	31.24%	7.495%
3	7.278	705	713	725	rBV	973896	1635204	36.57%	8.773%
4	7.665	771	779	790	rBV	881460	1493017	33.39%	8.011%
5	8.141	854	860	868	rVB	131339	218920	4.90%	1.175%
6	8.464	907	915	923	rVB	640096	1071560	23.97%	5.749%
7	9.316	1050	1060	1069	rBV	554201	1003365	22.44%	5.383%
8	10.961	1334	1340	1347	rBV	172272	306417	6.85%	1.644%
9	13.394	1747	1754	1764	rBV	1594138	2486579	55.61%	13.341%
10	14.769	1979	1988	1998	rBV	329281	516474	11.55%	2.771%
11	16.255	2233	2241	2256	rBV	1303524	2074599	46.40%	11.131%
12	17.513	2447	2455	2465	rBV	502488	748180	16.73%	4.014%
13	20.110	2890	2897	2909	rBV	3293030	4471256	100.00%	23.990%
14	21.796	3177	3184	3196	rBV	359670	727910	16.28%	3.905%
15	25.151	3743	3755	3767	rBV3	110929	415375	9.29%	2.229%




Sum of corrected areas: 18638122

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG050919\
Data File : BG040823.D
Acq On : 9 May 2019 19:47
Operator : HP/JU
Sample : PB119587BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB119587BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG042319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

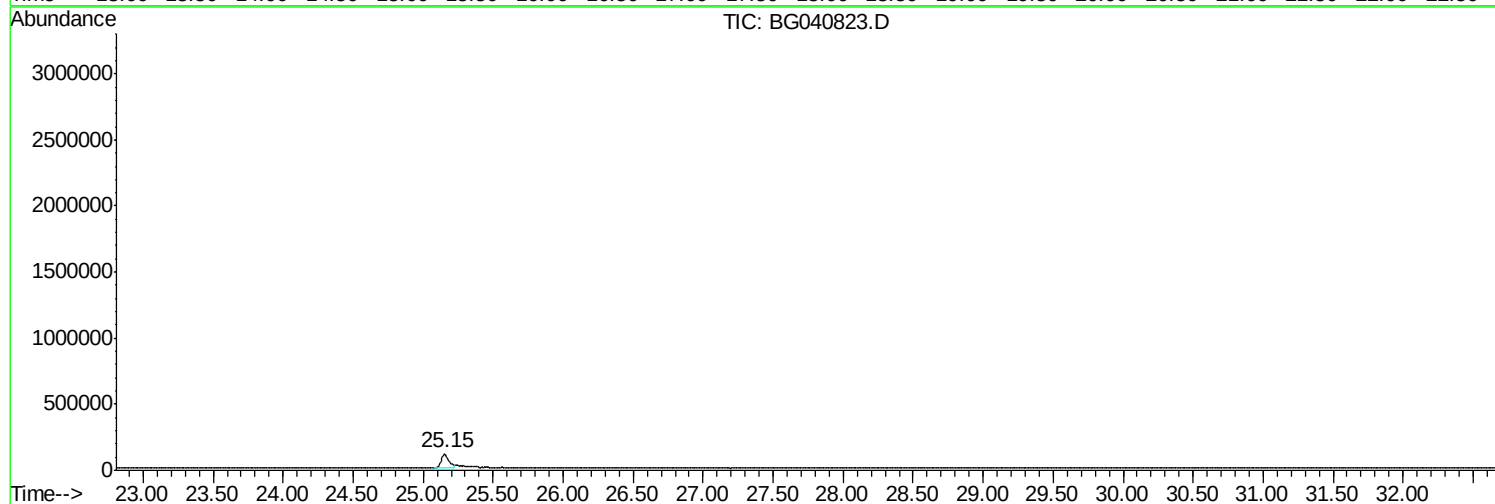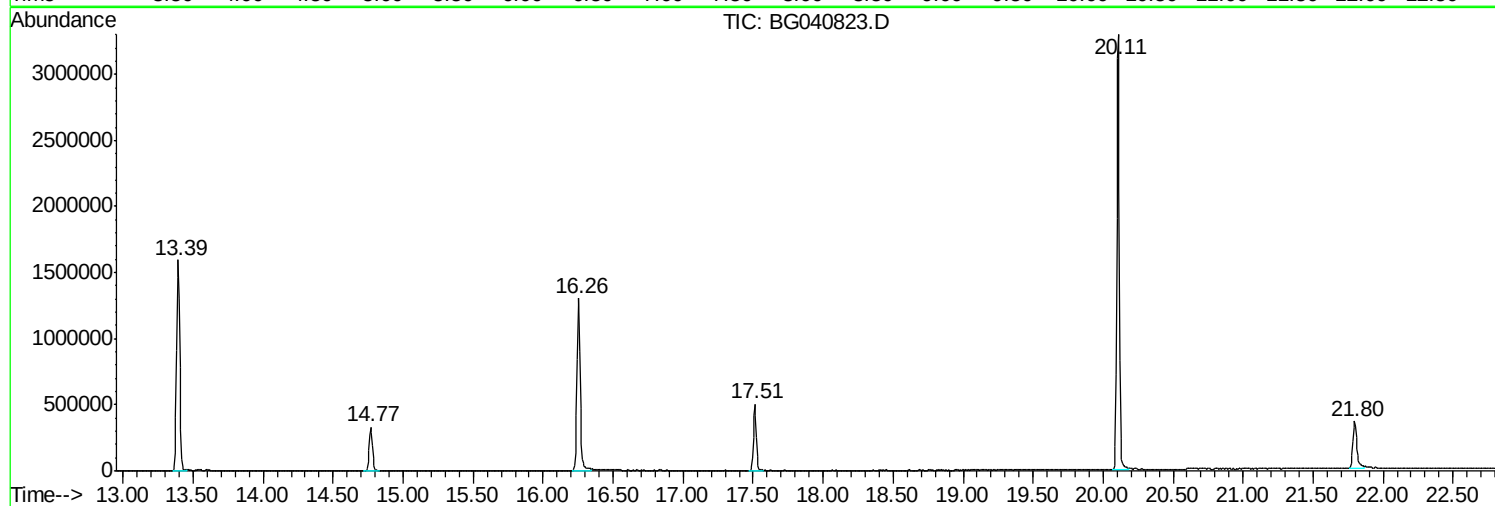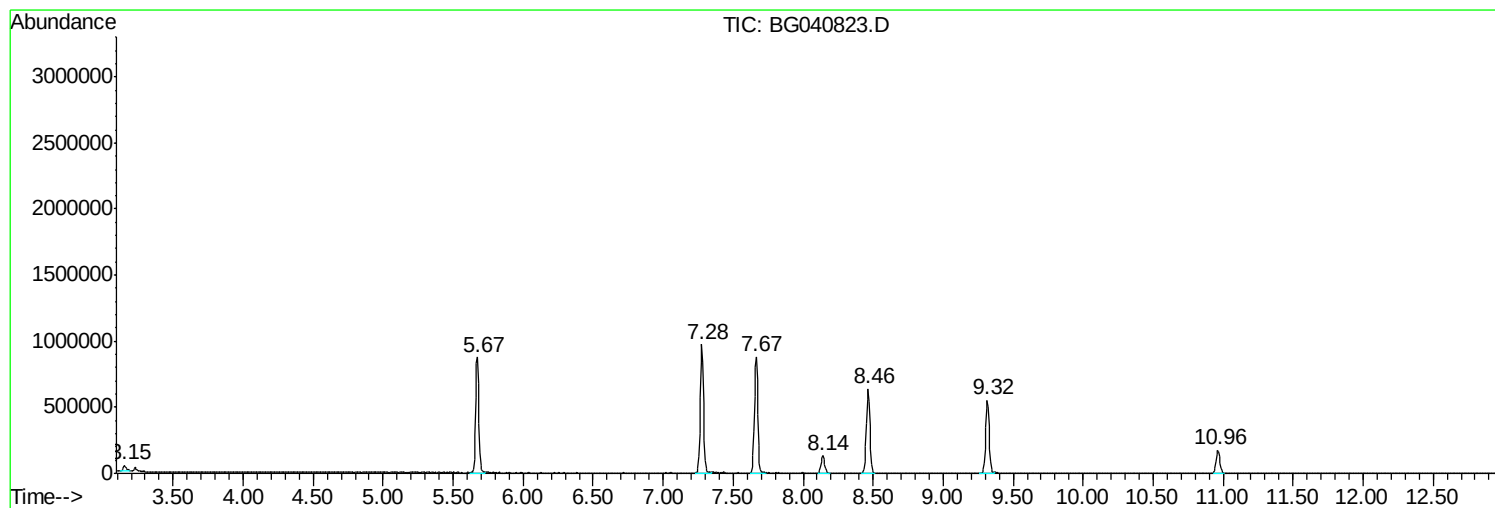

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG050919\
Data File : BG040823.D
Acq On : 9 May 2019 19:47
Operator : HP/JU
Sample : PB119587BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB119587BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG042319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.67 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.67	136.40 ng	1493020	1,4-Dichlorobenzene-d4	8.14

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
2		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
3		5-Aminoindole	132	C8H8N2	005192-03-0	22
4		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
5		Cyclopropanamine, 1-phenyl-	133	C9H11N	1000351-26-2	14

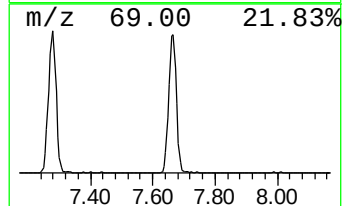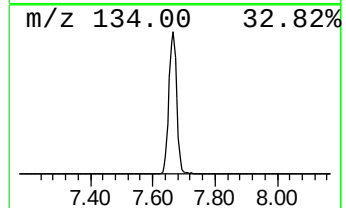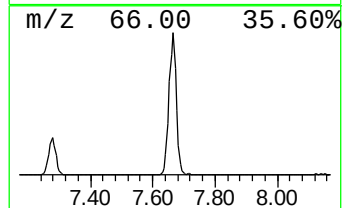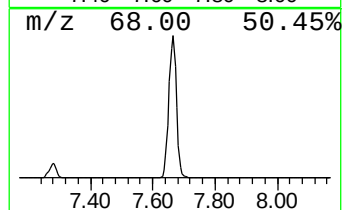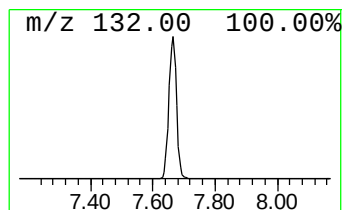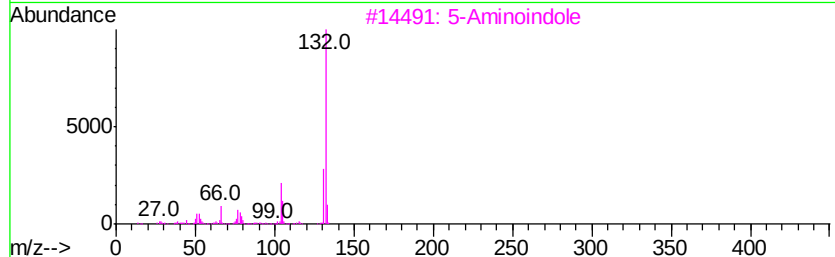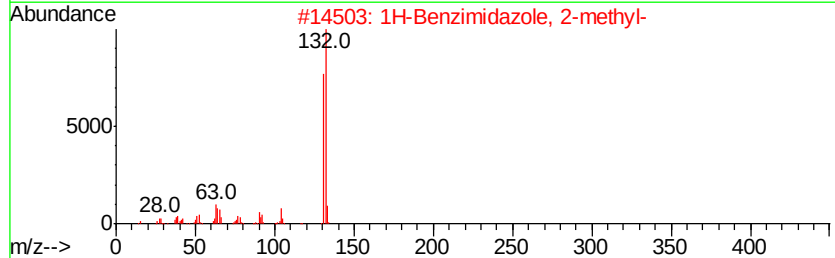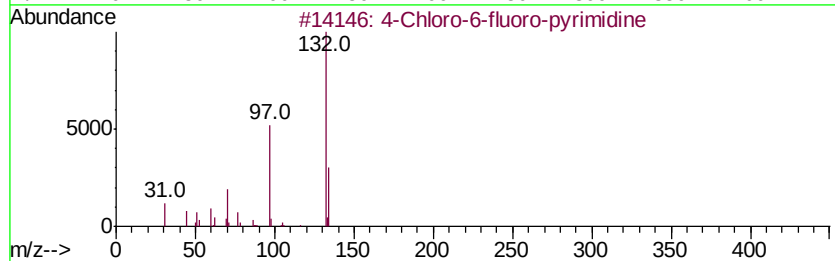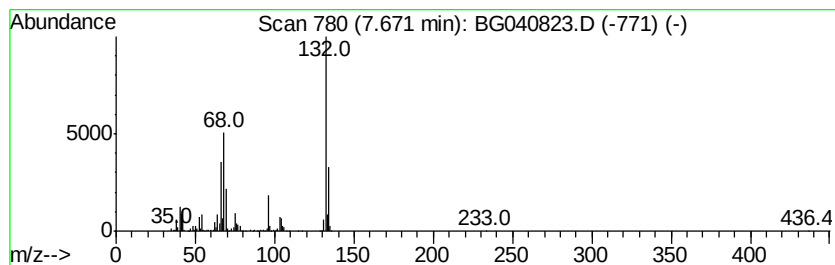

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG050919\
Data File : BG040823.D
Acq On : 9 May 2019 19:47
Operator : HP/JU
Sample : PB119587BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB119587BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.67	7.67	136.4	ng	1493020	1	8.14	218920	20.0