


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG050919\
 Data File : BG040820.D
 Acq On : 9 May 2019 17:15
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 24 05:35:33 2019

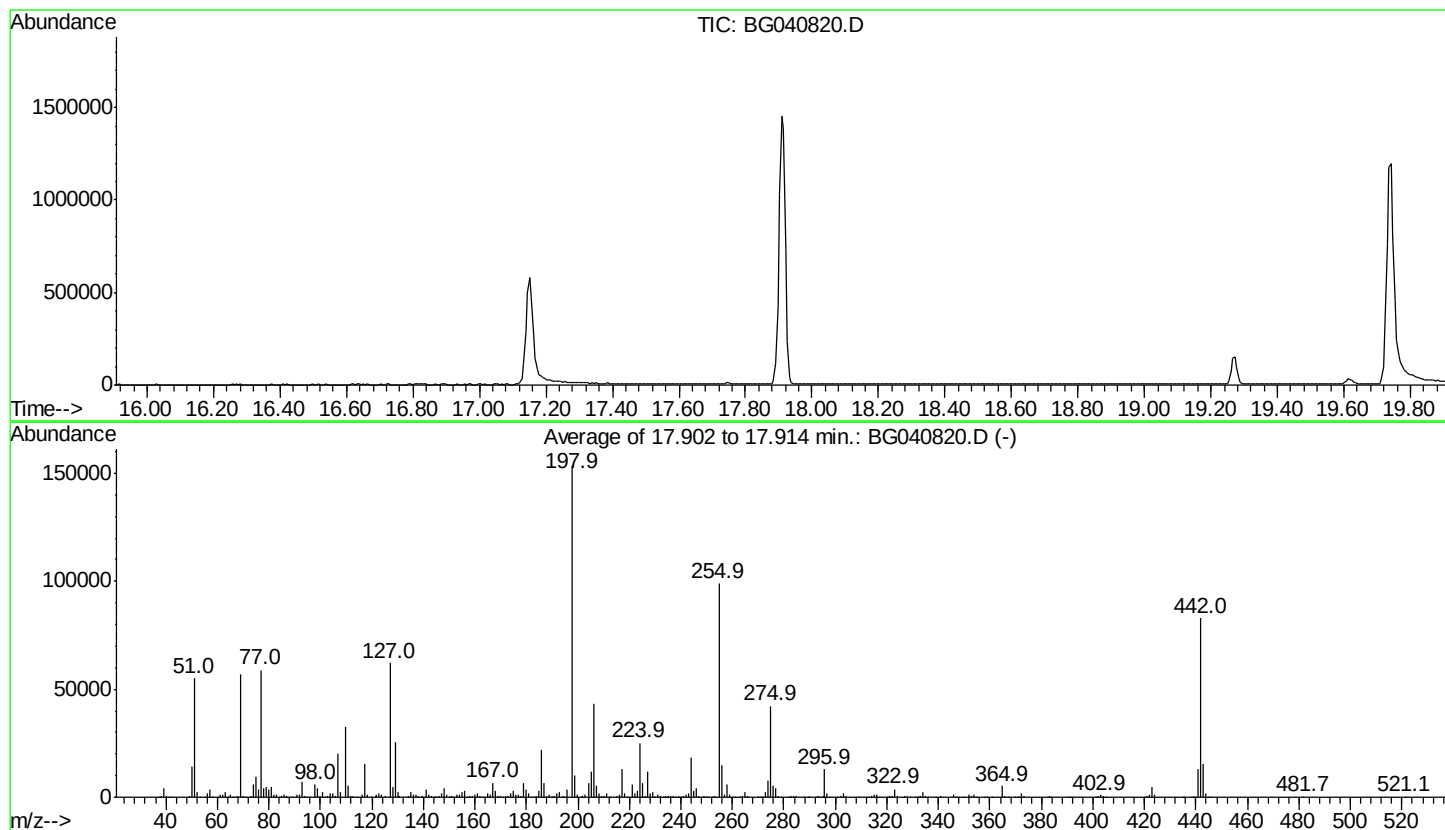

AutoFind: Scans 2521, 2522, 2523; Background Corrected with Scan 2514

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	55064	PASS
68	69	0.00	2	0.7	397	PASS
69	198	0.00	100	37.0	56818	PASS
70	69	0.00	2	0.6	322	PASS
127	198	10	80	40.5	62176	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	153496	PASS
199	198	5	9	6.8	10366	PASS
275	198	10	60	27.6	42354	PASS
365	198	1	100	3.3	5133	PASS
441	198	0.01	100	8.4	12892	PASS
442	198	50	100	53.9	82722	PASS
443	442	15	24	19.0	15696	PASS