

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050924\
 Data File : BG061156.D
 Acq On : 9 May 2024 18:13
 Operator : MA/JU
 Sample : P2415-01 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 1011UMR-SS005-0212-01

Quant Time: May 09 18:50:09 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 01 05:11:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.935	152	26427	20.000	ng	-0.03
21) Naphthalene-d8	10.726	136	101097	20.000	ng	-0.03
39) Acenaphthene-d10	14.563	164	75252	20.000	ng	-0.03
64) Phenanthrene-d10	17.307	188	181381	20.000	ng	-0.03
76) Chrysene-d12	21.566	240	184090	20.000	ng	-0.03
86) Perylene-d12	24.692	264	215819	20.000	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.526	112	27441	21.118	ng	-0.02
7) Phenol-d6	7.113	99	36061	18.760	ng	-0.02
23) Nitrobenzene-d5	9.087	82	26799	13.141	ng	-0.03
42) 2,4,6-Tribromophenol	16.055	330	23624	15.706	ng	-0.02
45) 2-Fluorobiphenyl	13.182	172	68329	13.427	ng	-0.03
79) Terphenyl-d14	19.927	244	132388	11.960	ng	-0.03
Target Compounds						
9) Benzaldehyde	7.113	77	55	Below Cal	Qvalue	# 3
19) n-Nitroso-di-n-propyla...	9.087	70	4001	2.781 ng	#	55
51) 2,6-Dinitrotoluene	14.557	165	9846	7.920 ng	#	15
57) 2,4-Dinitrotoluene	14.557	165	9846	5.353 ng	#	17
77) Benzidine	19.551	184	210	2.852 ng	#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050924\
Data File : BG061156.D
Acq On : 9 May 2024 18:13
Operator : MA/JU
Sample : P2415-01 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
1011UMR-SS005-0212-01

Quant Time: May 09 18:50:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration




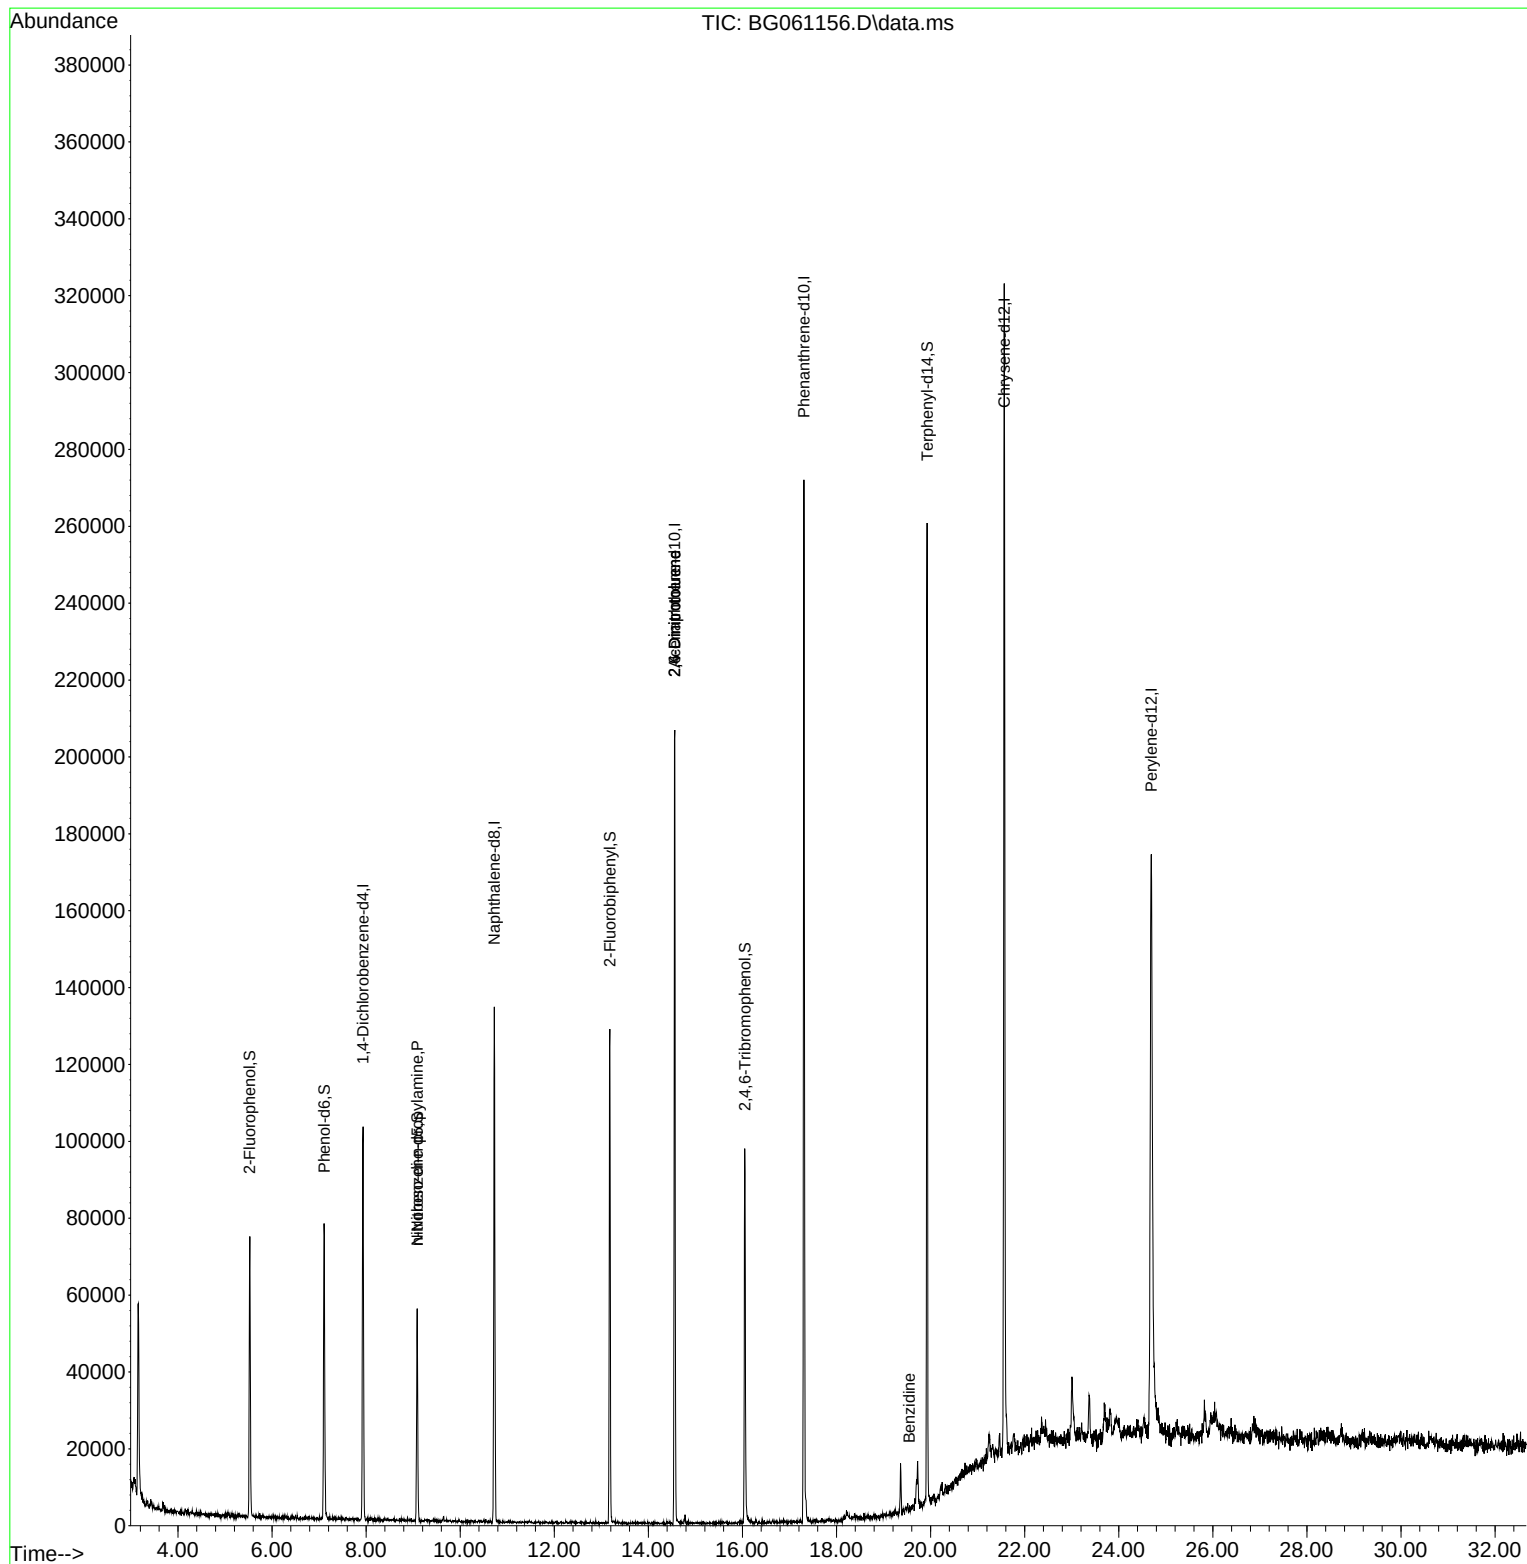




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.935 min Scan# 846
Delta R.T. -0.026 min
Lab File: BG061156.D
Acq: 9 May 2024 18:13




Instrument :
BNA_G
ClientSampleId :
1011UMR-SS005-0212-01


Tgt Ion:152 Resp: 26427
Ion Ratio Lower Upper
152 100
150 155.5 138.3 207.5
115 64.2 48.0 72.0

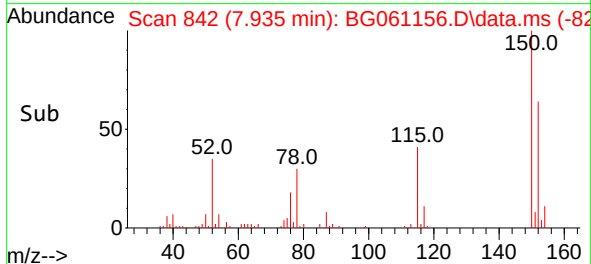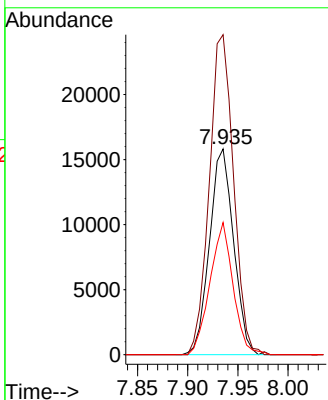

#5
2-Fluorophenol
Concen: 21.118 ng
RT: 5.526 min Scan# 432
Delta R.T. -0.020 min
Lab File: BG061156.D
Acq: 9 May 2024 18:13

Tgt Ion:112 Resp: 27441
Ion Ratio Lower Upper
112 100
64 69.5 55.7 83.5
63 46.1 38.1 57.1


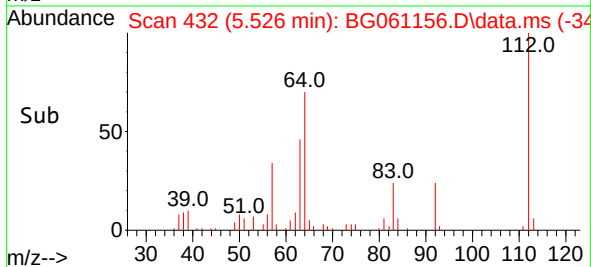
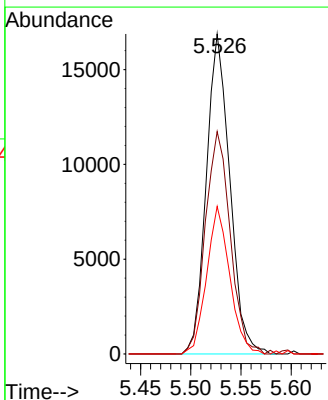
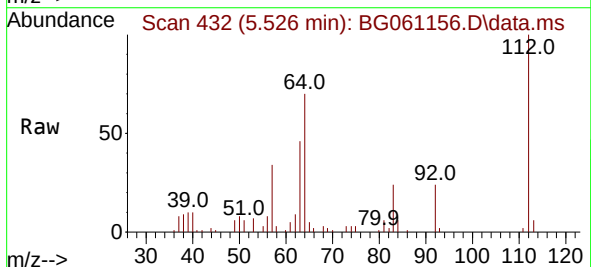




#7
Phenol-d6
Concen: 18.760 ng
RT: 7.113 min Scan# 70
Delta R.T. -0.020 min
Lab File: BG061156.D
Acq: 9 May 2024 18:13




Instrument :
BNA_G
ClientSampleId :
1011UMR-SS005-0212-01


Tgt Ion: 99 Resp: 36061
Ion Ratio Lower Upper
99 100
42 30.3 29.2 43.8
71 43.4 39.7 59.5

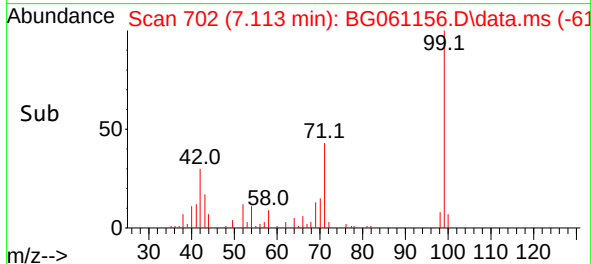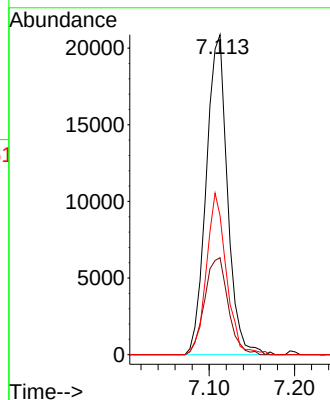

#19
n-Nitroso-di-n-propylamine
Concen: 2.781 ng
RT: 9.087 min Scan# 1038
Delta R.T. 0.320 min
Lab File: BG061156.D
Acq: 9 May 2024 18:13

Tgt Ion: 70 Resp: 4001
Ion Ratio Lower Upper
70 100
42 60.6 86.4 129.6#
101 0.0 7.8 11.8#
130 0.0 19.0 28.4#


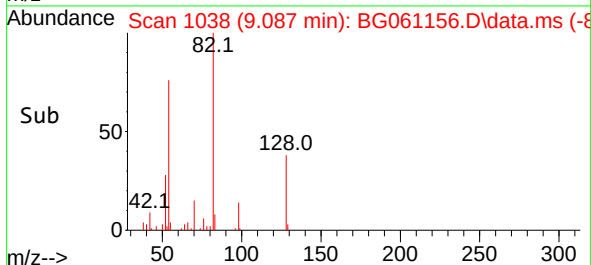
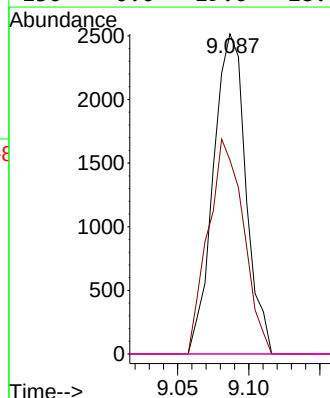
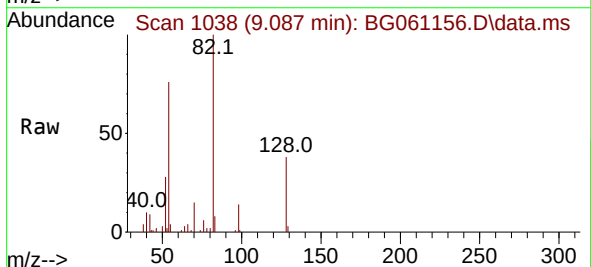




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.726 min Scan# 11
Delta R.T. -0.032 min
Lab File: BG061156.D
Acq: 9 May 2024 18:13




Instrument :
BNA_G
ClientSampleId :
1011UMR-SS005-0212-01


Tgt Ion:	136	Resp:	101097
Ion	Ratio	Lower	Upper
136	100		
137	10.4	7.8	11.6
54	11.7	8.1	12.1
68	3.3	3.0	4.4

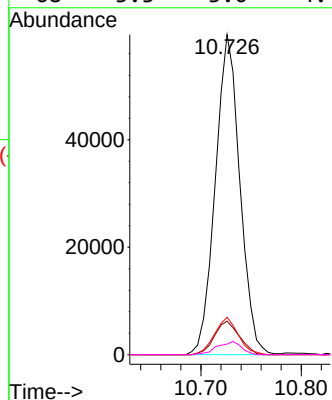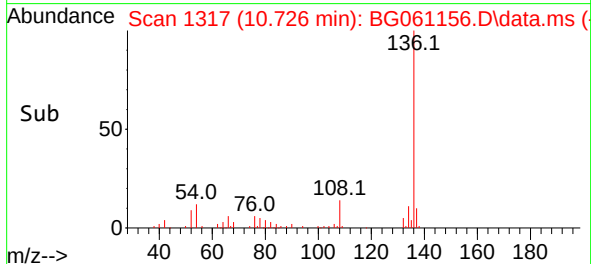

#23
Nitrobenzene-d5
Concen: 13.141 ng
RT: 9.087 min Scan# 1038
Delta R.T. -0.032 min
Lab File: BG061156.D
Acq: 9 May 2024 18:13


Tgt Ion:	82	Resp:	26799
Ion	Ratio	Lower	Upper
82	100		
128	37.6	32.7	49.1
54	75.7	65.6	98.4

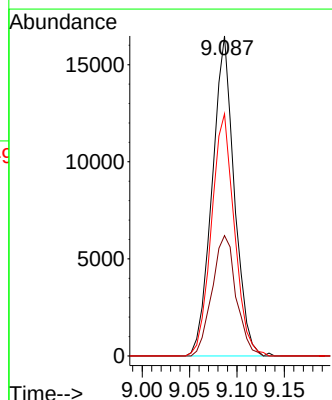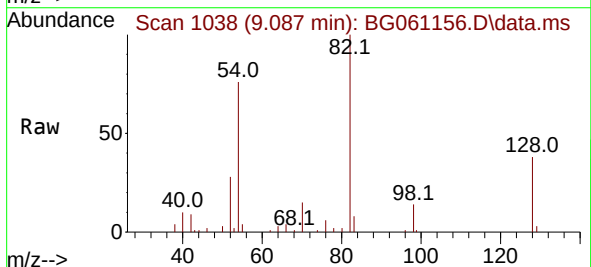






#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.563 min Scan# 1970
Delta R.T. -0.026 min
Lab File: BG061156.D
Acq: 9 May 2024 18:13

Instrument :
BNA_G
ClientSampleId :
1011UMR-SS005-0212-01







Tgt Ion:164 Resp: 75252
Ion Ratio Lower Upper
164 100
162 100.3 79.4 119.2
160 47.0 37.0 55.6

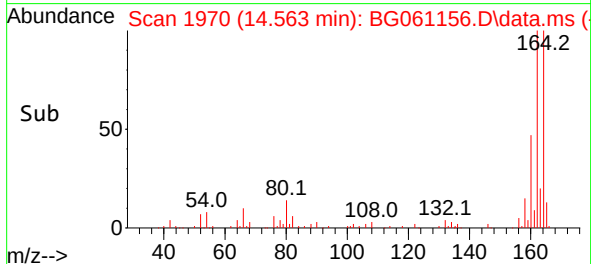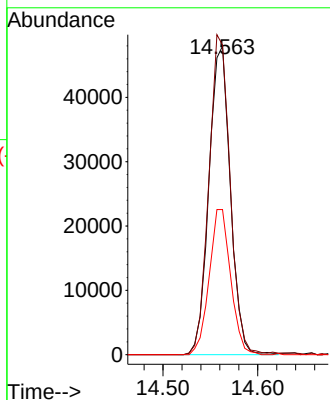

#42
2,4,6-Tribromophenol
Concen: 15.706 ng
RT: 16.055 min Scan# 2224
Delta R.T. -0.020 min
Lab File: BG061156.D
Acq: 9 May 2024 18:13

Tgt Ion:330 Resp: 23624
Ion Ratio Lower Upper
330 100
332 102.1 78.6 117.8
141 26.8 20.5 30.7


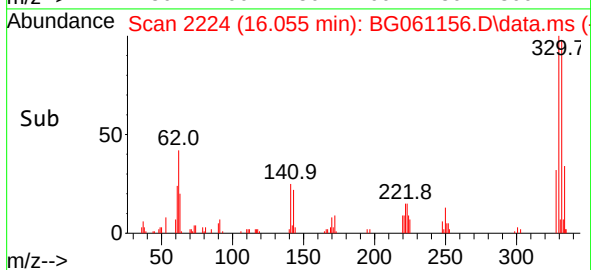
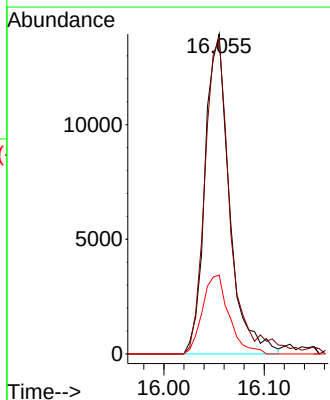
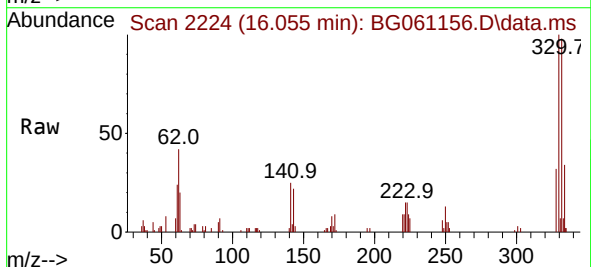




#45
2-Fluorobiphenyl
Concen: 13.427 ng
RT: 13.182 min Scan# 1735
Delta R.T. -0.026 min
Lab File: BG061156.D
Acq: 9 May 2024 18:13




Instrument :
BNA_G
ClientSampleId :
1011UMR-SS005-0212-01


Tgt Ion:	172	Resp:	68329
Ion	Ratio	Lower	Upper
172	100		
171	37.0	29.0	43.6
170	24.8	20.2	30.4

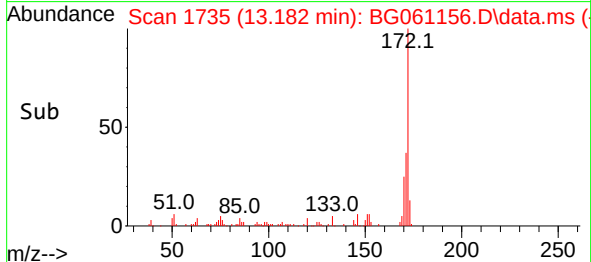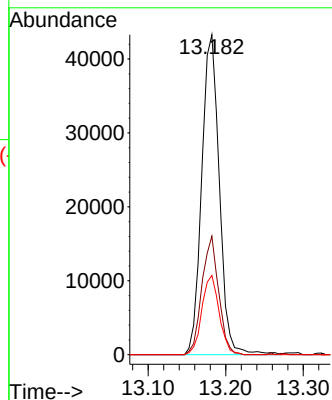

#51
2,6-Dinitrotoluene
Concen: 7.920 ng
RT: 14.557 min Scan# 1969
Delta R.T. 0.397 min
Lab File: BG061156.D
Acq: 9 May 2024 18:13


Tgt Ion:	165	Resp:	9846
Ion	Ratio	Lower	Upper
165	100		
63	0.0	60.0	90.0#
89	0.0	50.9	76.3#

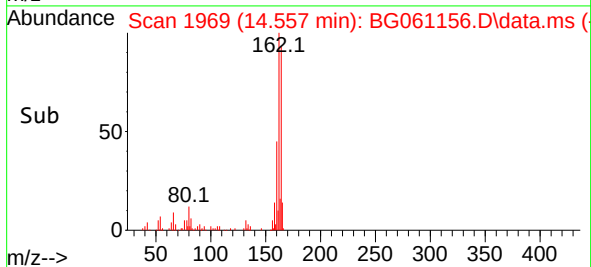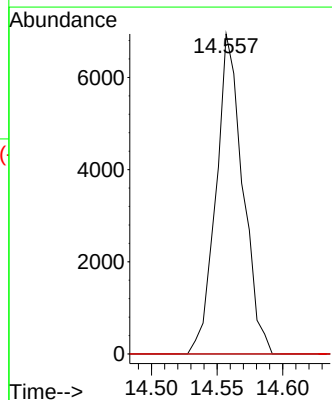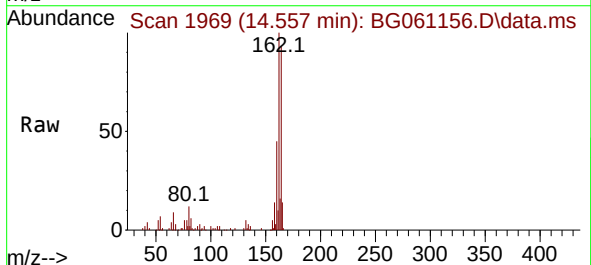






#57
2,4-Dinitrotoluene
Concen: 5.353 ng
RT: 14.557 min Scan# 1969
Delta R.T. -0.390 min
Lab File: BG061156.D
Acq: 9 May 2024 18:13

Instrument :
BNA_G
ClientSampleId :
1011UMR-SS005-0212-01







Tgt Ion:	165	Resp:	9846
Ion Ratio	Lower	Upper	
165	100		
63	0.0	47.3	70.9#
89	0.0	61.8	92.8#
182	0.0	1.8	2.6#

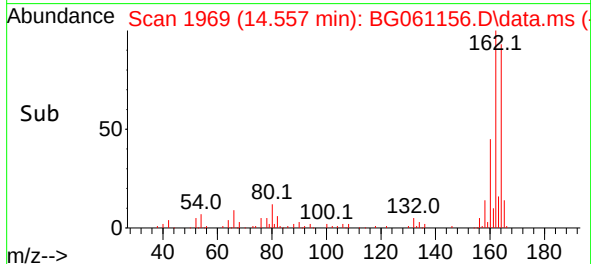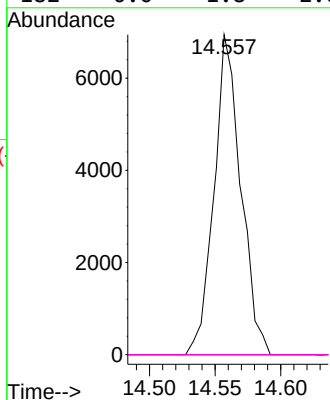

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.307 min Scan# 2437
Delta R.T. -0.026 min
Lab File: BG061156.D
Acq: 9 May 2024 18:13

Tgt Ion:	188	Resp:	181381
Ion Ratio	Lower	Upper	
188	100		
94	3.7	3.6	5.4
80	4.8	4.2	6.2

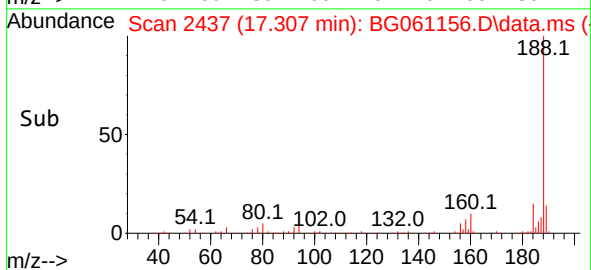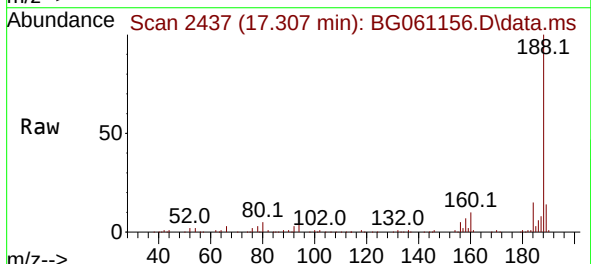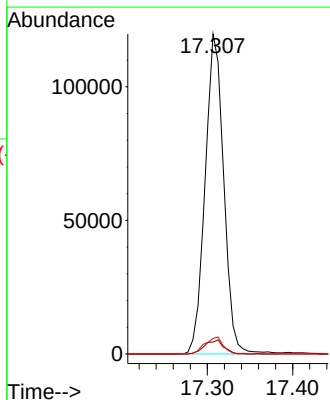



#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.566 min Scan# 3166

Delta R.T. -0.026 min

Lab File: BG061156.D

Acq: 9 May 2024 18:13

Instrument :

BNA_G

ClientSampleId :

1011UMR-SS005-0212-01





Tgt Ion:240 Resp: 184090

Ion Ratio Lower Upper

240 100

120 4.3 3.2 4.8

236 26.9 21.0 31.6

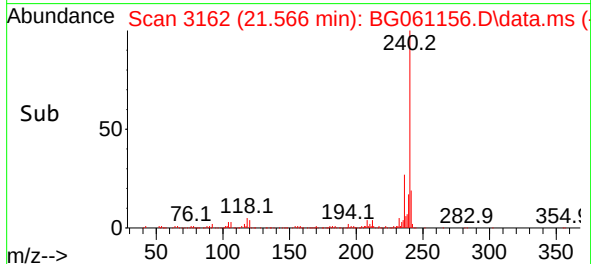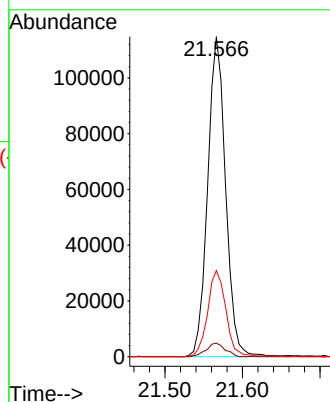

#77

Benzidine

Concen: 2.852 ng

RT: 19.551 min Scan# 2819

Delta R.T. -0.014 min

Lab File: BG061156.D

Acq: 9 May 2024 18:13




Tgt Ion:184 Resp: 210


Ion Ratio Lower Upper

184 100

185 0.0 12.0 18.0#

183 0.0 10.9 16.3#


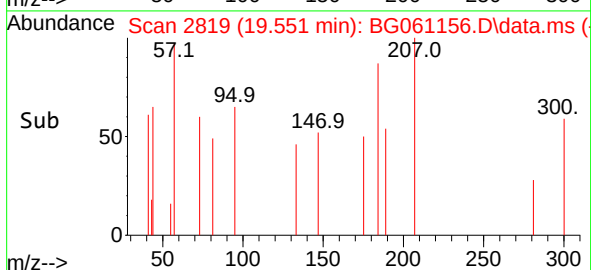
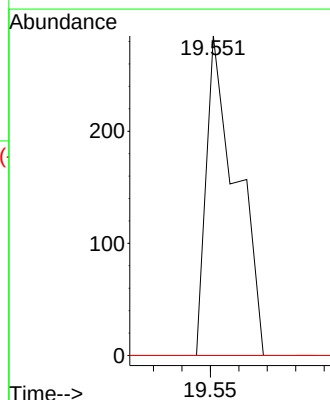





#79
 Terphenyl-d14
 Concen: 11.960 ng
 RT: 19.927 min Scan# 21
 Delta R.T. -0.026 min
 Lab File: BG061156.D
 Acq: 9 May 2024 18:13

Instrument :
 BNA_G
 ClientSampleId :
 1011UMR-SS005-0212-01

Tgt Ion:244 Resp: 132388
 Ion Ratio Lower Upper
 244 100
 212 7.7 5.7 8.5
 122 4.4 4.2 6.2

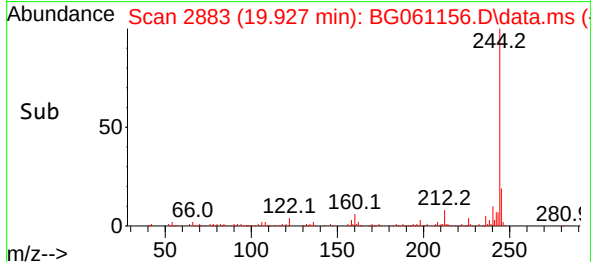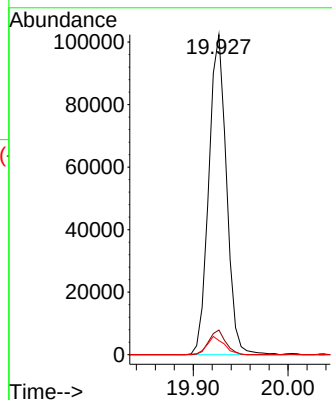

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.692 min Scan# 3694
 Delta R.T. -0.038 min
 Lab File: BG061156.D
 Acq: 9 May 2024 18:13

Tgt Ion:264 Resp: 215819
 Ion Ratio Lower Upper
 264 100
 260 23.2 17.7 26.5
 265 20.4 16.4 24.6

