
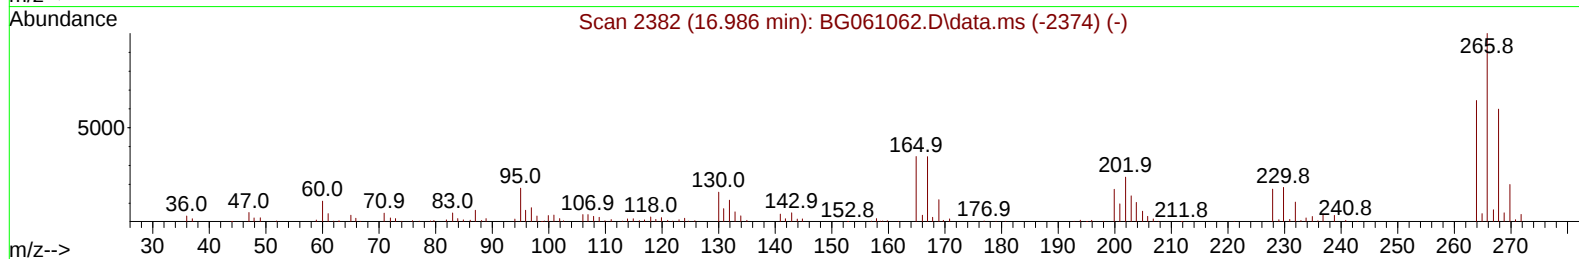
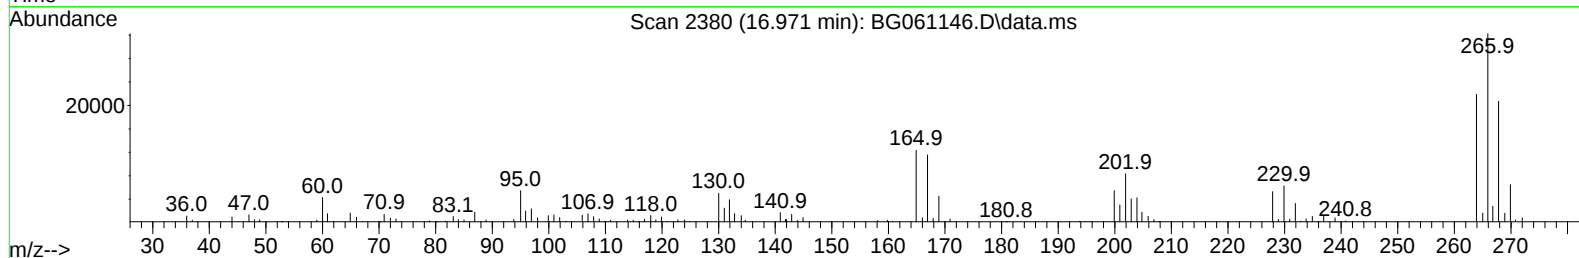


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050924\
Data File : BG061146.D
Acq On : 9 May 2024 10:51
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 09 12:07:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

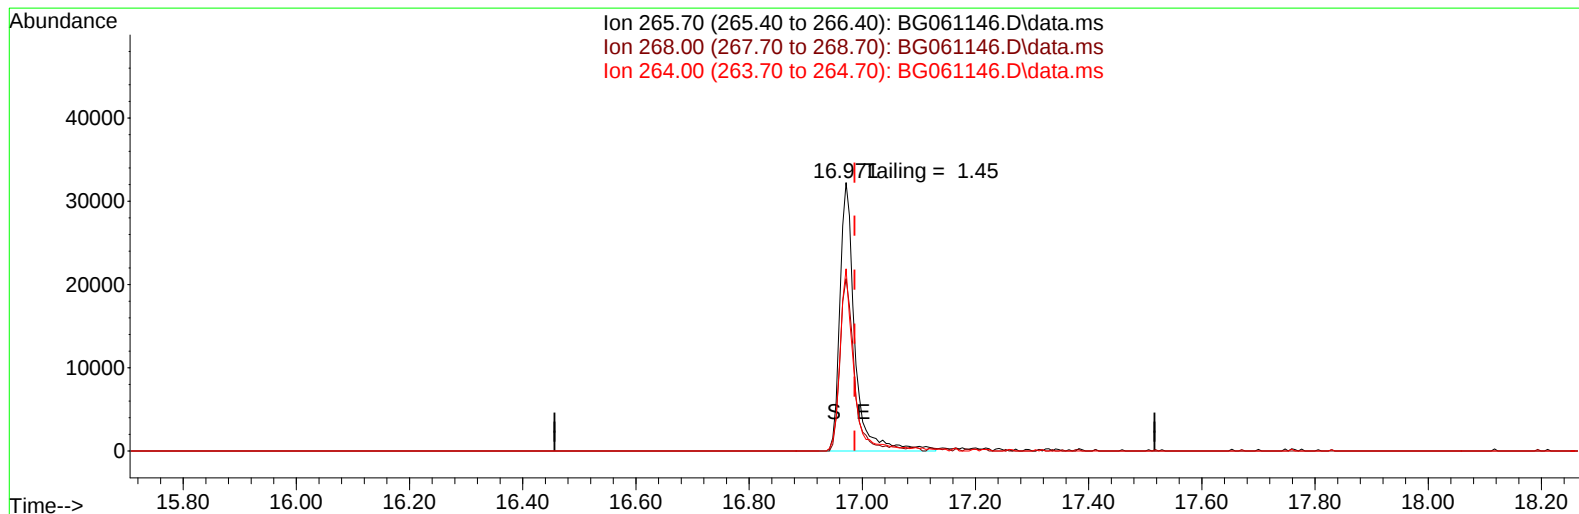

TIC: BG061146.D\data.ms

(70) Pentachlorophenol (C)




16.971min (-0.015) 20580.23 ng

response 58395

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.80	64.24
264.00	64.40	67.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050924\
Data File : BG061146.D
Acq On : 9 May 2024 10:51
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 09 12:07:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

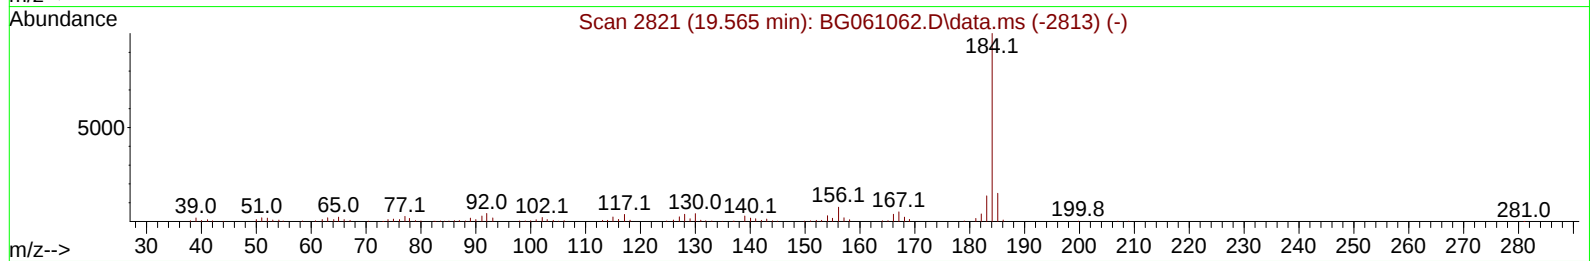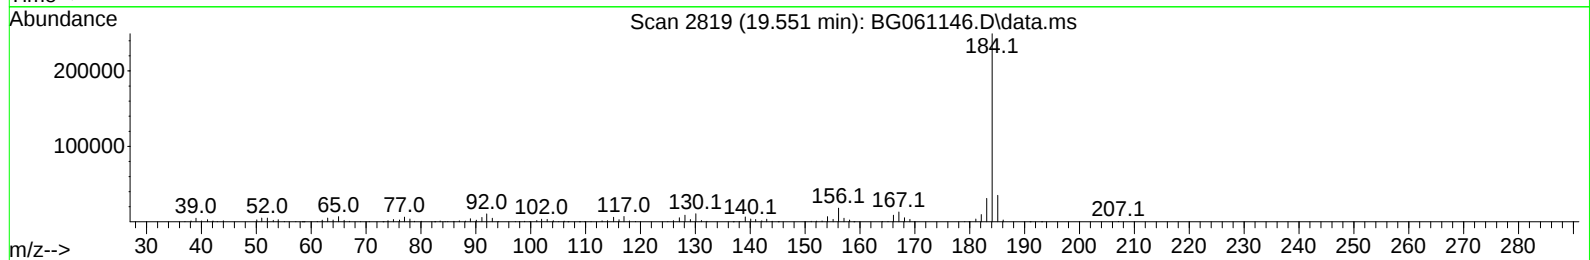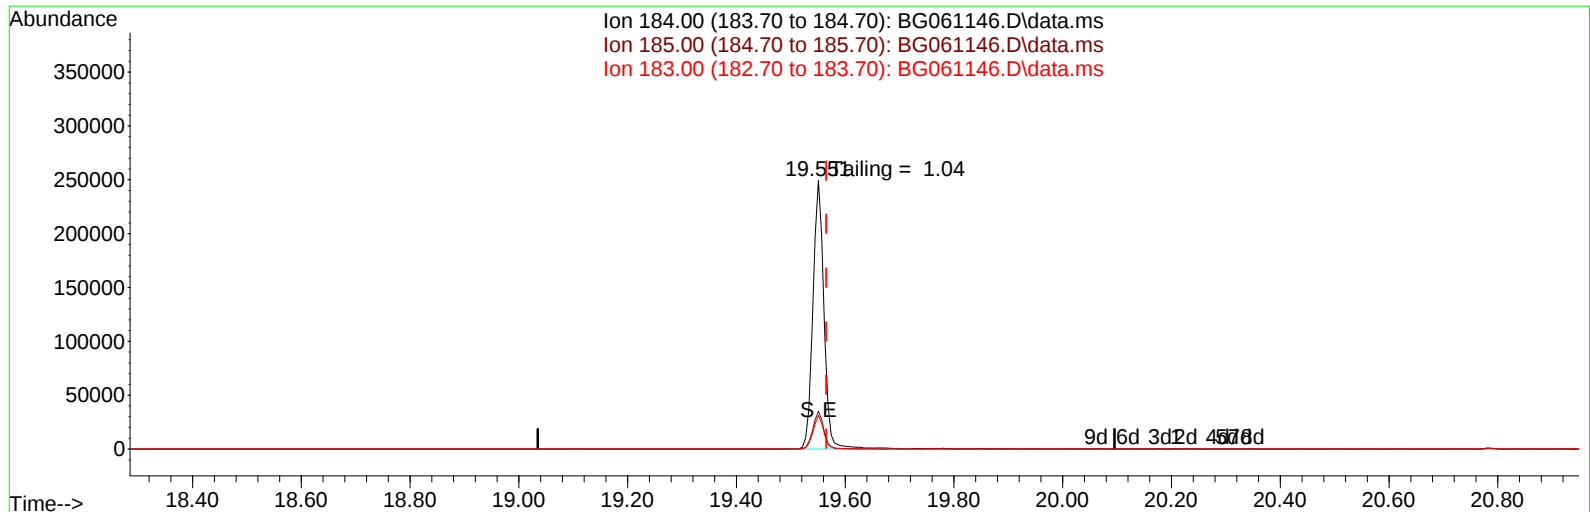

TIC: BG061146.D\data.ms

(77) Benzidine

19.551min (-0.014) 289849.89 ng m

response 357254

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.06
183.00	13.60	12.47
0.00	0.00	0.00