

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050924\
Data File : BG061148.D
Acq On : 9 May 2024 12:13
Operator : MA/JU
Sample : PB160779BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB160779BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG061148.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.526	426	432	447	rVB	449915	698811	26.98%	7.865%
2	7.112	694	702	713	rBV	456671	769090	29.69%	8.656%
3	7.935	836	842	848	rVB2	77401	124612	4.81%	1.402%
4	9.092	1030	1039	1050	rBV	280995	494628	19.09%	5.567%
5	10.731	1310	1318	1326	rBV	99541	173346	6.69%	1.951%
6	13.187	1729	1736	1744	rBV	734953	1177376	45.45%	13.251%
7	14.562	1961	1970	1977	rBV	172088	264215	10.20%	2.974%
8	16.054	2217	2224	2239	rBV	729818	1168199	45.10%	13.147%
9	17.312	2432	2438	2447	rBV	267845	397457	15.34%	4.473%
10	19.932	2878	2884	2896	rVB	2061525	2590444	100.00%	29.154%
11	21.571	3157	3163	3173	rVB2	300063	491243	18.96%	5.529%
12	24.697	3684	3695	3713	rBV2	171224	536067	20.69%	6.033%




Sum of corrected areas: 8885488

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050924\
Data File : BG061148.D
Acq On : 9 May 2024 12:13
Operator : MA/JU
Sample : PB160779BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB160779BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

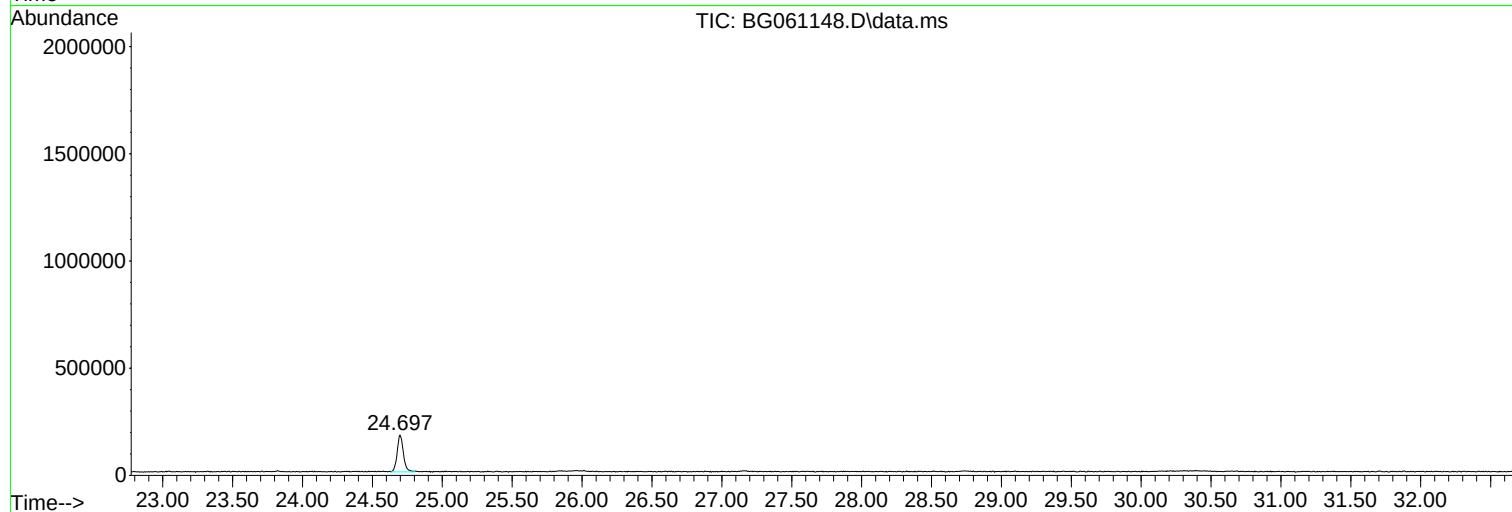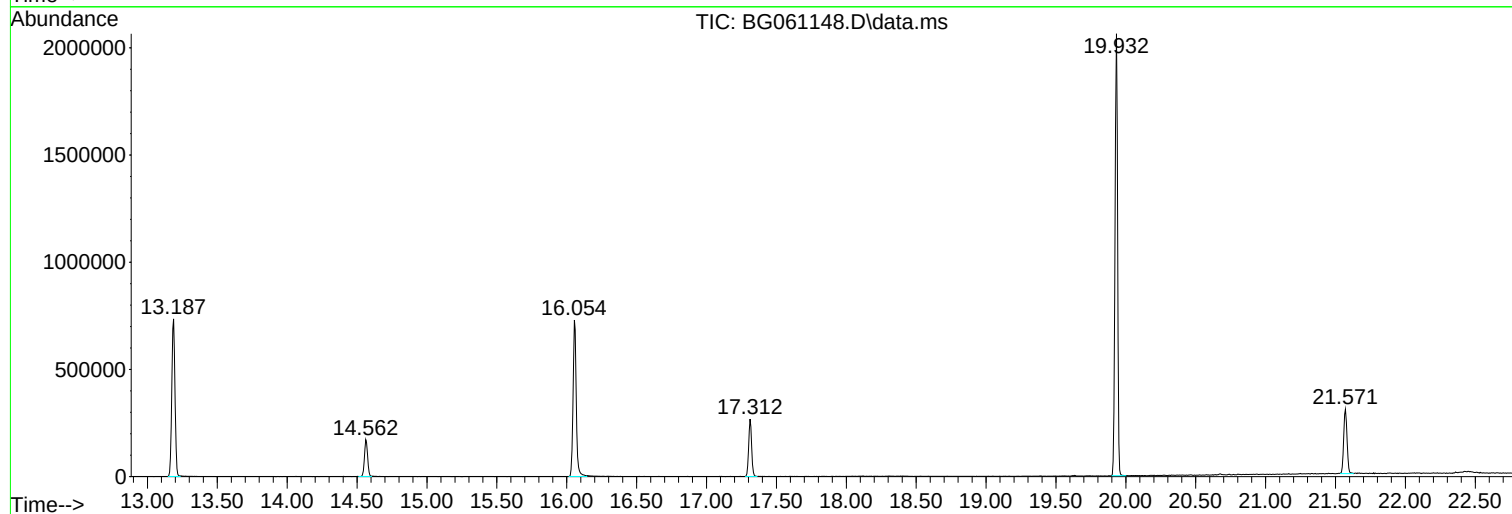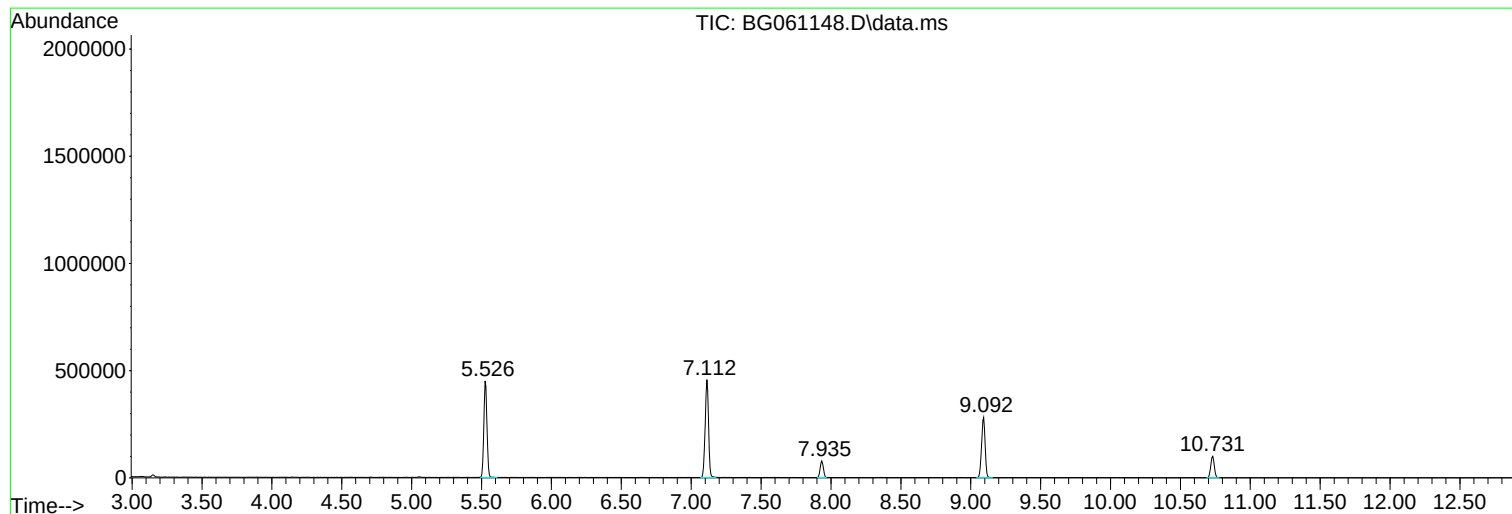

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050924\
Data File : BG061148.D
Acq On : 9 May 2024 12:13
Operator : MA/JU
Sample : PB160779BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB160779BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050924\
Data File : BG061148.D
Acq On : 9 May 2024 12:13
Operator : MA/JU
Sample : PB160779BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB160779BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------