


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050924\
Data File : BG061146.D
Acq On : 9 May 2024 10:51
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 01 05:11:25 2024

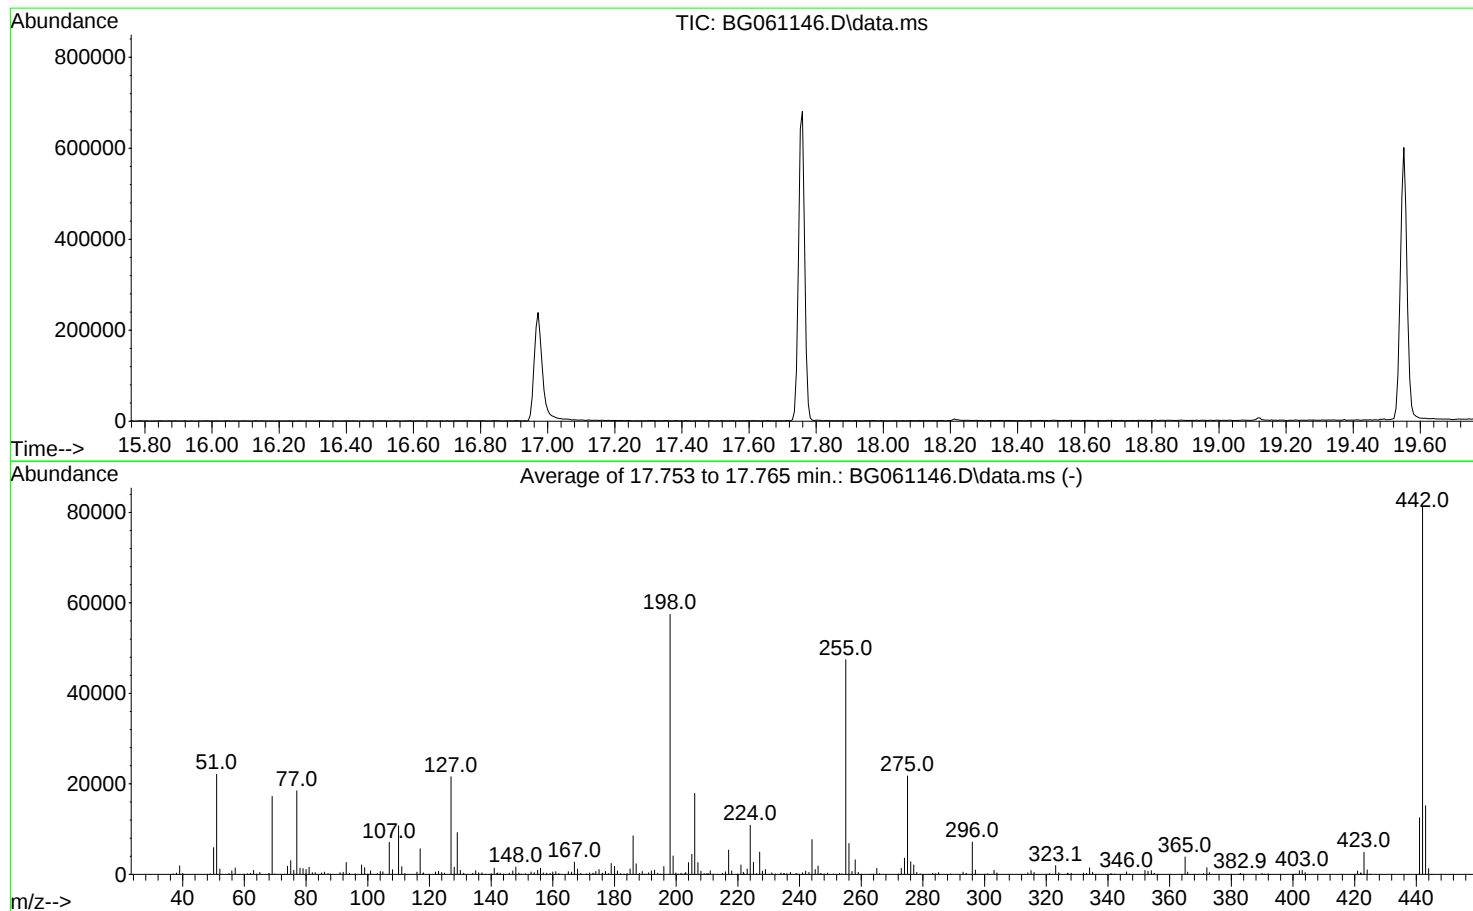

AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.5	22115	PASS
68	69	0.00	2	1.1	193	PASS
69	198	0.00	100	29.9	17211	PASS
70	69	0.00	2	0.3	57	PASS
127	198	10	80	37.5	21566	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	57477	PASS
199	198	5	9	7.1	4080	PASS
275	198	10	60	37.8	21744	PASS
365	198	1	100	6.7	3840	PASS
441	198	0.01	100	21.8	12534	PASS
442	442	50	100	100.0	81304	PASS
443	442	15	24	18.6	15157	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/9/2024	BNA_G	<u>BG061146.D</u>
Compound Name	Response	Retention Time
DDT	219508	20.785
DDD	5825	20.35
DDE	476	19.85
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6301	225809	2.79

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050924\
Data File : BG061146.D
Acq On : 9 May 2024 10:51
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 09 12:07:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

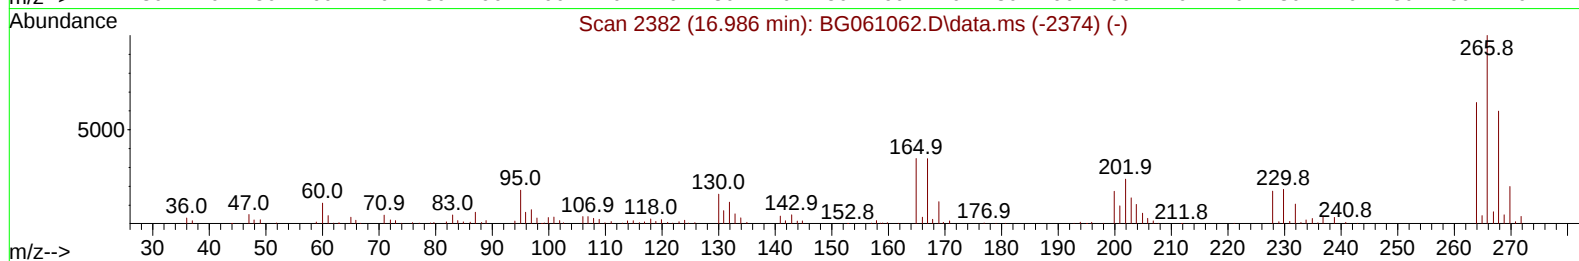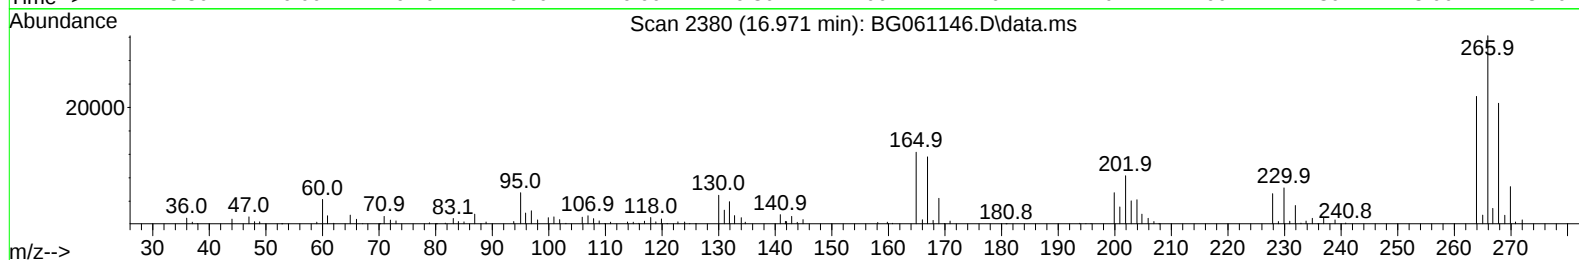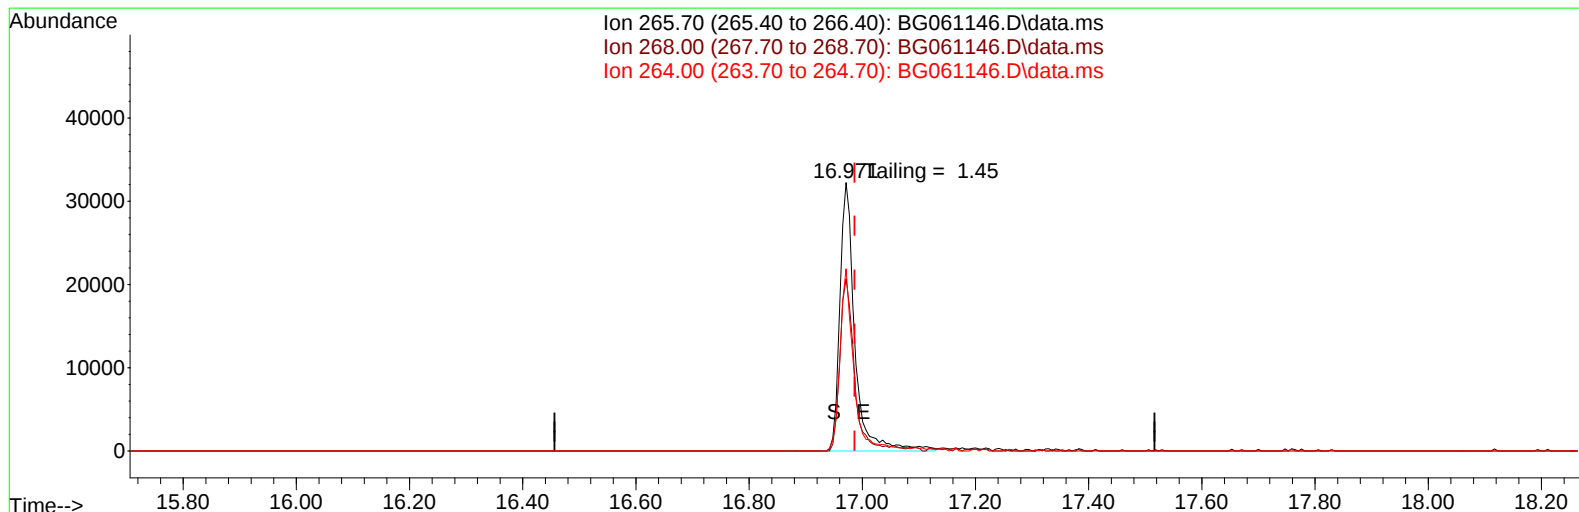

TIC: BG061146.D\data.ms

(70) Pentachlorophenol (C)

16.971min (-0.015) 20580.23 ng




response 58395

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.80	64.24
264.00	64.40	67.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050924\
Data File : BG061146.D
Acq On : 9 May 2024 10:51
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 09 12:07:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

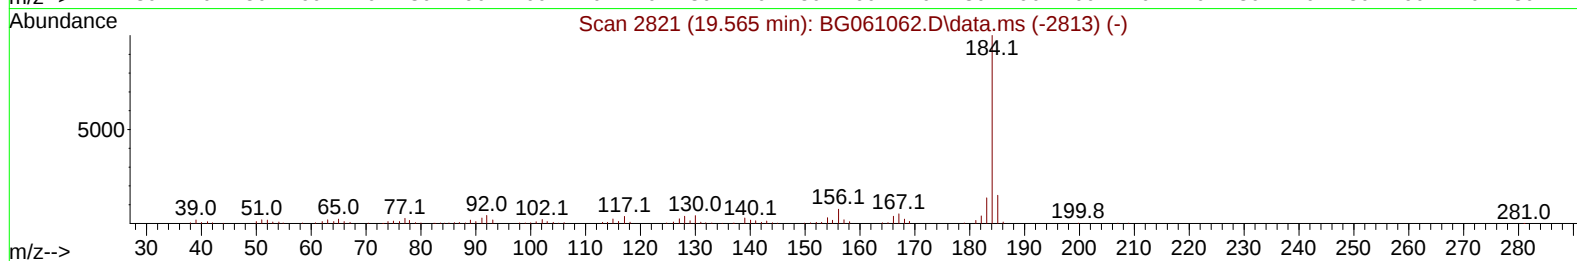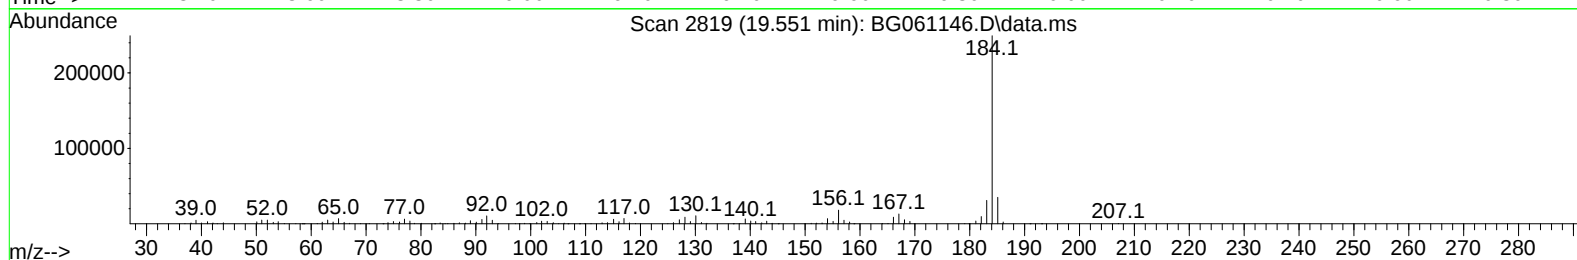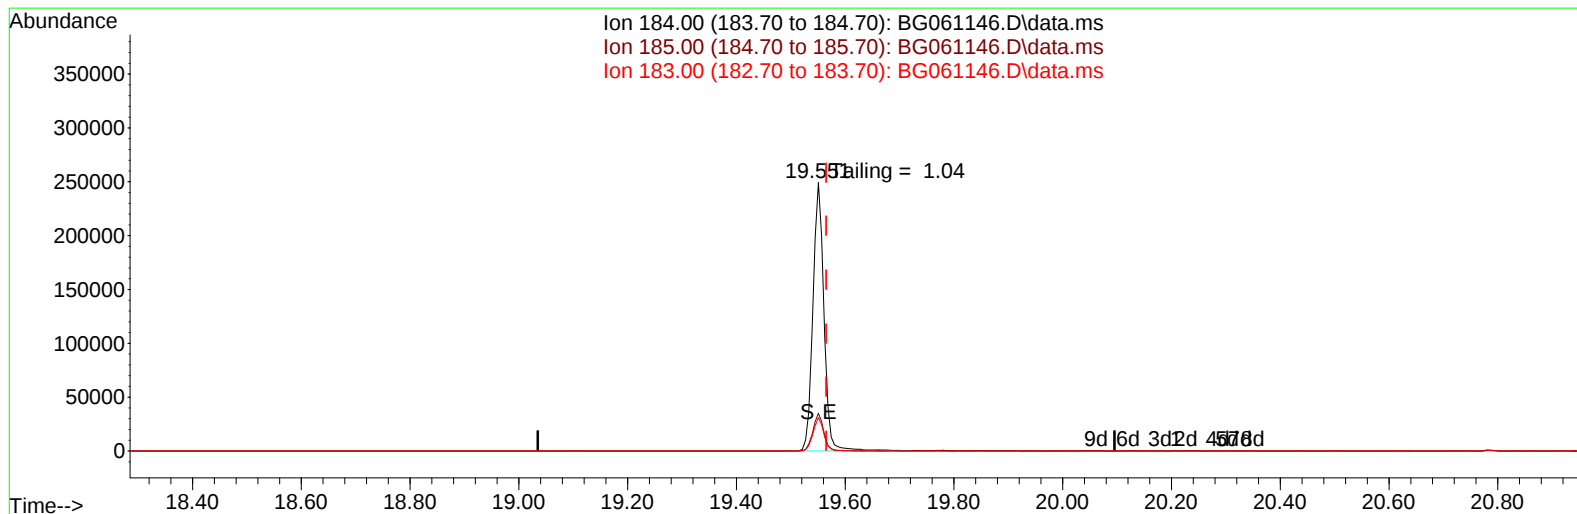

TIC: BG061146.D\data.ms

(77) Benzidine

19.551min (-0.014) 289849.89 ng m

response 357254

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.06
183.00	13.60	12.47
0.00	0.00	0.00