

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_G\DATA\BG051019\  
 Data File : BG040859.D  
 Acq On : 10 May 2019 23:51  
 Operator : HP/JU  
 Sample : K2792-01  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DRUM-COMP

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON  
 Sampling : 1  
 Start Thrs: 0.2  
 Stop Thrs : 0  
 Filtering: 5  
 Min Area: 3 % of largest Peak  
 Max Peaks: 100  
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG042319.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.147       | 5             | 10          | 20           | rVV      | 142100         | 277309        | 5.09%           | 1.104%        |
| 2         | 3.235       | 20            | 25          | 38           | rVB      | 630685         | 905181        | 16.61%          | 3.604%        |
| 3         | 3.535       | 72            | 76          | 81           | rBV      | 54280          | 68314         | 1.25%           | 0.272%        |
| 4         | 5.203       | 355           | 360         | 368          | rVB      | 125521         | 194110        | 3.56%           | 0.773%        |
| 5         | 5.668       | 432           | 439         | 447          | rBV      | 981339         | 1571239       | 28.83%          | 6.256%        |
| 6         | 7.272       | 704           | 712         | 725          | rBV      | 961290         | 1672268       | 30.68%          | 6.658%        |
| 7         | 7.659       | 771           | 778         | 798          | rBV      | 1058864        | 1799399       | 33.02%          | 7.165%        |
| 8         | 8.135       | 850           | 859         | 867          | rBV      | 190485         | 336821        | 6.18%           | 1.341%        |
| 9         | 8.458       | 905           | 914         | 921          | rBV      | 753507         | 1288145       | 23.64%          | 5.129%        |
| 10        | 9.310       | 1051          | 1059        | 1070         | rBV      | 673927         | 1186434       | 21.77%          | 4.724%        |
| 11        | 10.955      | 1330          | 1339        | 1347         | rBV      | 246164         | 434220        | 7.97%           | 1.729%        |
| 12        | 11.713      | 1459          | 1468        | 1474         | rBV2     | 34461          | 71046         | 1.30%           | 0.283%        |
| 13        | 13.388      | 1744          | 1753        | 1760         | rBV      | 1849391        | 2787685       | 51.15%          | 11.100%       |
| 14        | 13.594      | 1781          | 1788        | 1797         | rVB      | 78550          | 120255        | 2.21%           | 0.479%        |
| 15        | 14.763      | 1979          | 1987        | 1995         | rBV2     | 413400         | 663167        | 12.17%          | 2.640%        |
| 16        | 16.249      | 2231          | 2240        | 2251         | rBV      | 1761659        | 2719383       | 49.90%          | 10.828%       |
| 17        | 17.507      | 2446          | 2454        | 2463         | rBV2     | 649759         | 947416        | 17.38%          | 3.772%        |
| 18        | 19.328      | 2760          | 2764        | 2773         | rBV      | 121888         | 167442        | 3.07%           | 0.667%        |
| 19        | 20.104      | 2889          | 2896        | 2903         | rBV      | 4112877        | 5450015       | 100.00%         | 21.700%       |
| 20        | 21.790      | 3175          | 3183        | 3198         | rBV      | 717835         | 1243685       | 22.82%          | 4.952%        |
| 21        | 23.282      | 3432          | 3437        | 3444         | rVB6     | 35228          | 69575         | 1.28%           | 0.277%        |
| 22        | 25.133      | 3740          | 3752        | 3763         | rBV3     | 379507         | 1142180       | 20.96%          | 4.548%        |


Sum of corrected areas: 25115289

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_G\DATA\BG051019\  
Data File : BG040859.D  
Acq On : 10 May 2019 23:51  
Operator : HP/JU  
Sample : K2792-01  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DRUM-COMP

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG042319.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

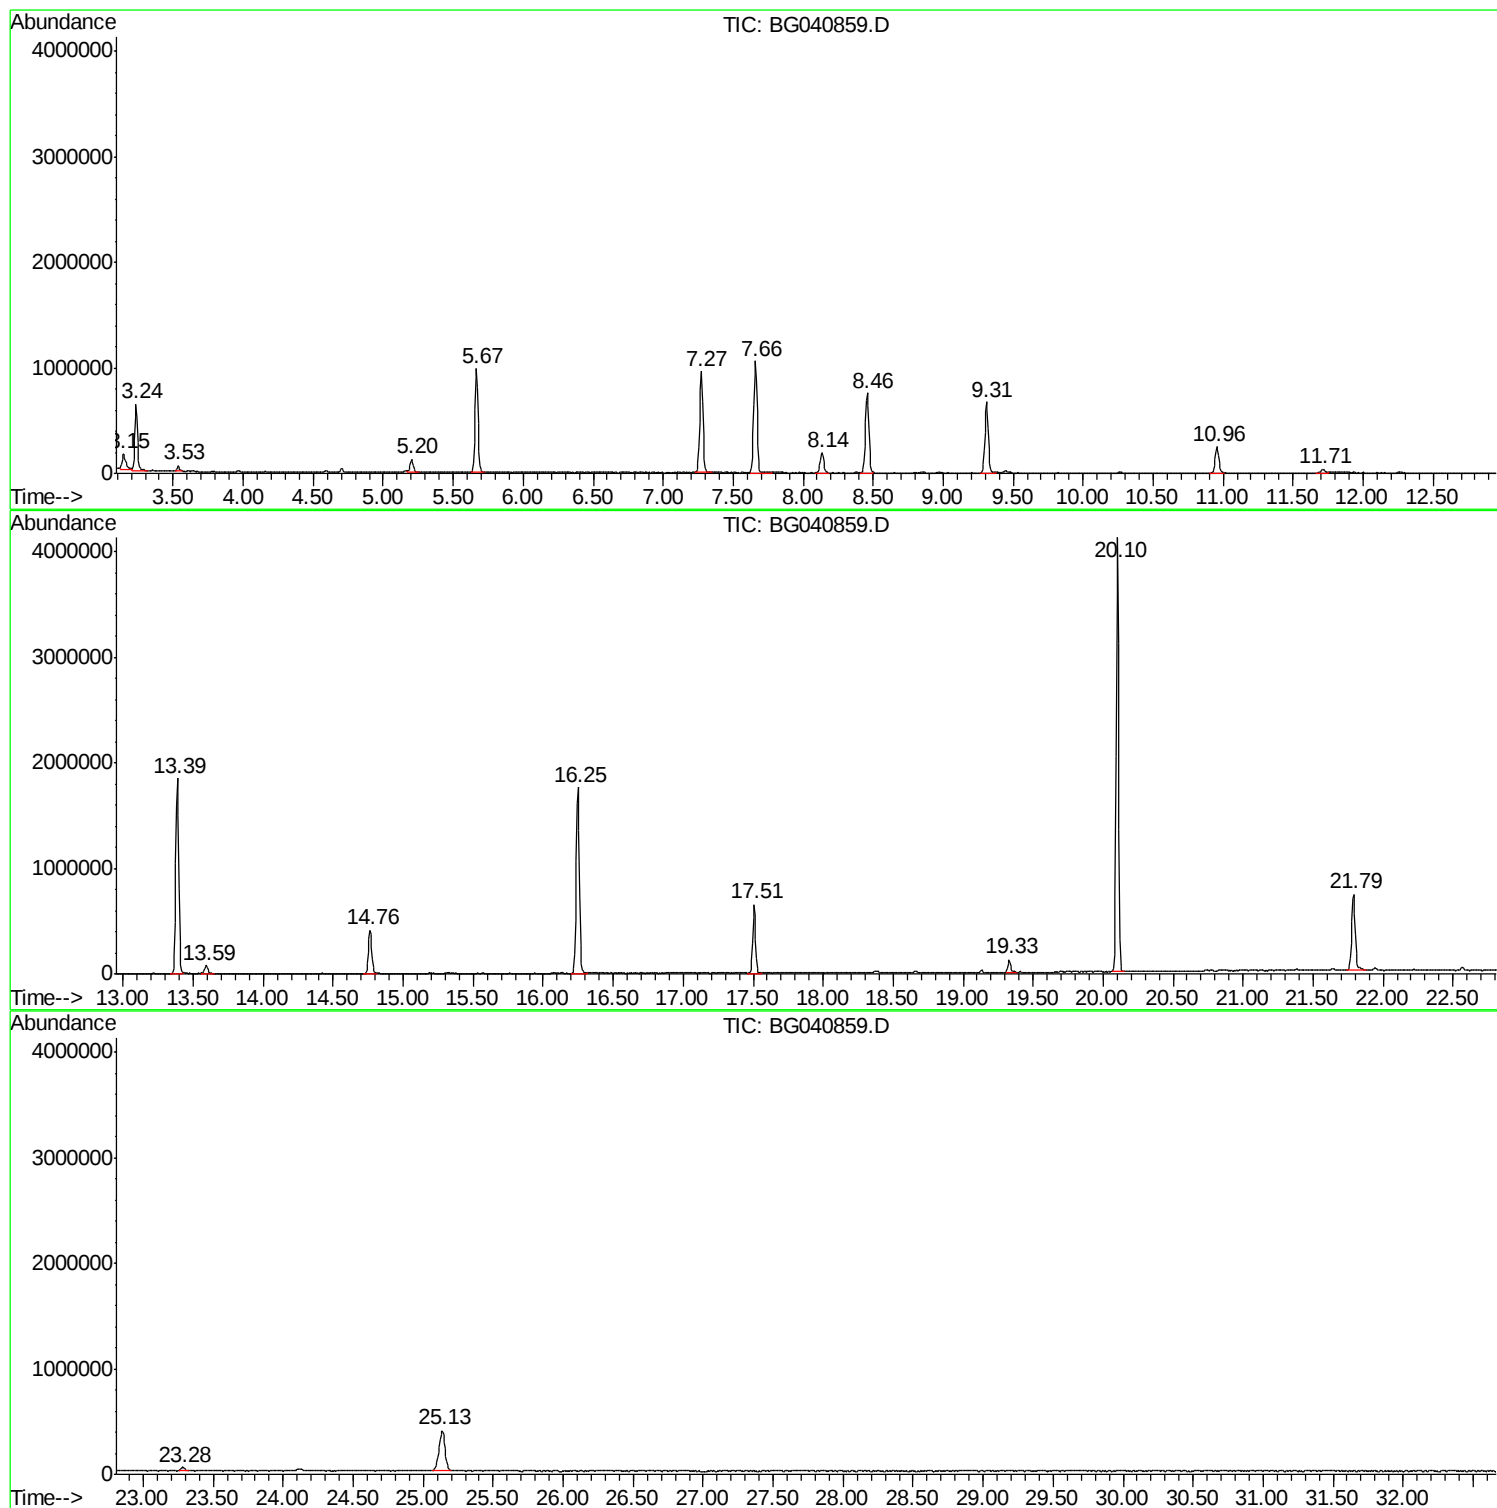

DbaaaPath::ZZ\SS00SSRVNRP00001BBNAGGDATA\BB0050099\  
 DbaaaFile::BB0000899DD  
 Aeqq00n ::100May2009 233551  
 Operator::HPPJU  
 Sample::K0292001  
 Misc::  
 AASSVal::77 SampleMultiplier:11

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DRUM-COMP

QqaantMebdd::ZZ\SS00SSRVNRP00001BBNAGGMEH00582200BB002339MM  
 QqaantTitle::ASBPBNASSANDABBSF00R55P000NTCALIBRATION

TICLibrary::CC\DaabbaaeN0\$T11LL  
 TICIntegratíonParameters:LS6CNTPP

| TIC Top Hit name | RT | EstConc | Units | Response | Internal Standard |
|------------------|----|---------|-------|----------|-------------------|
|                  |    |         |       | #        | RT Resp Conc      |

No Library Search Compounds Detected

\*\*\*\*\*