


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG051119\
 Data File : BG040891.D
 Acq On : 12 May 2019 3:26
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 24 05:35:33 2019

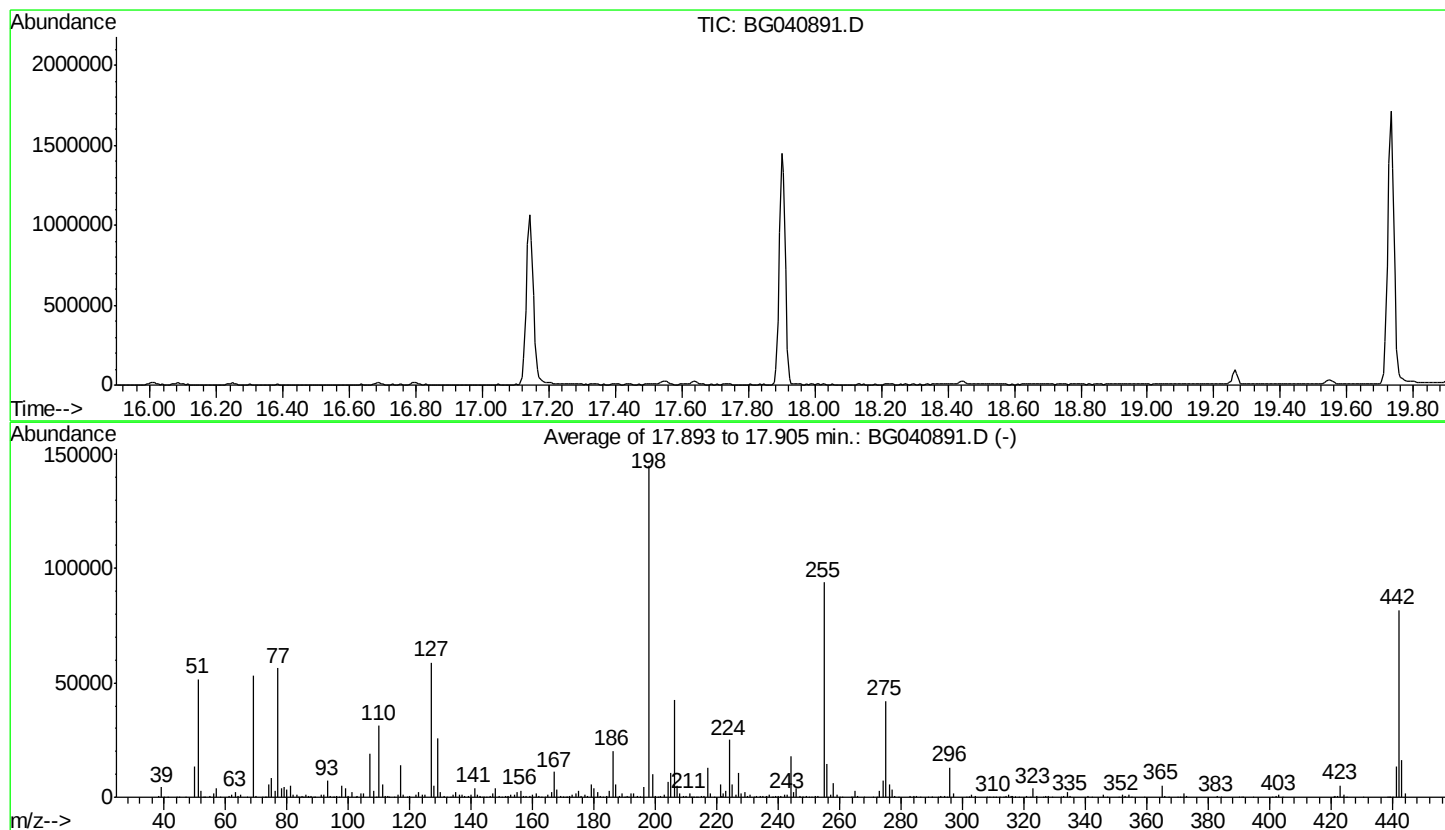

AutoFind: Scans 2520, 2521, 2522; Background Corrected with Scan 2514

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	51581	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.6	53080	PASS
70	69	0.00	2	0.8	408	PASS
127	198	10	80	40.6	58794	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	144896	PASS
199	198	5	9	7.1	10271	PASS
275	198	10	60	29.1	42202	PASS
365	198	1	100	3.7	5295	PASS
441	198	0.01	100	9.3	13414	PASS
442	198	50	100	56.5	81869	PASS
443	442	15	24	20.0	16354	PASS