
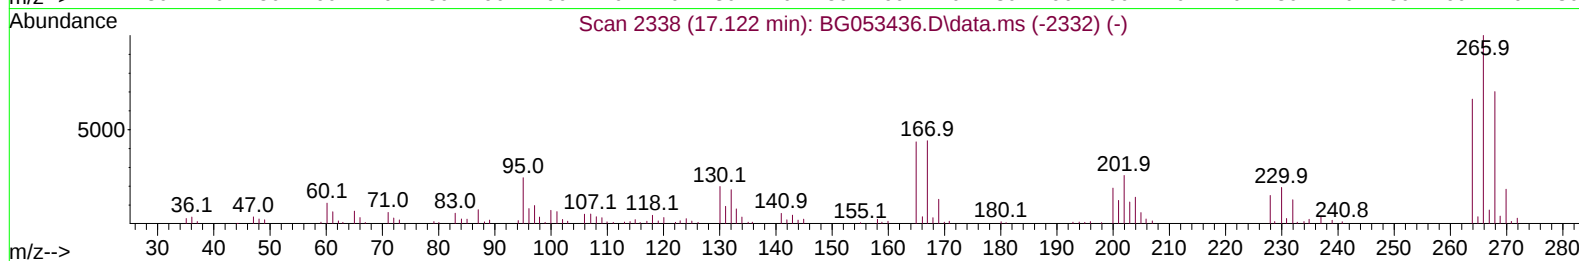
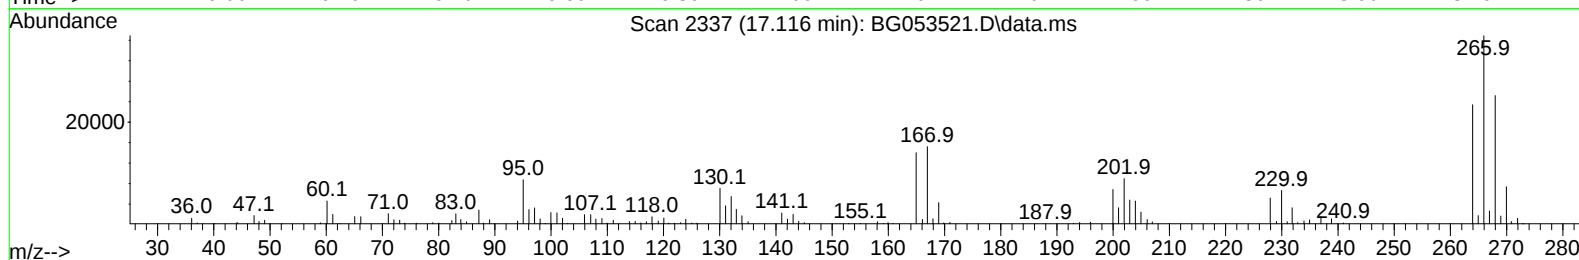


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051122\
Data File : BG053521.D
Acq On : 11 May 2022 11:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 11 19:05:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

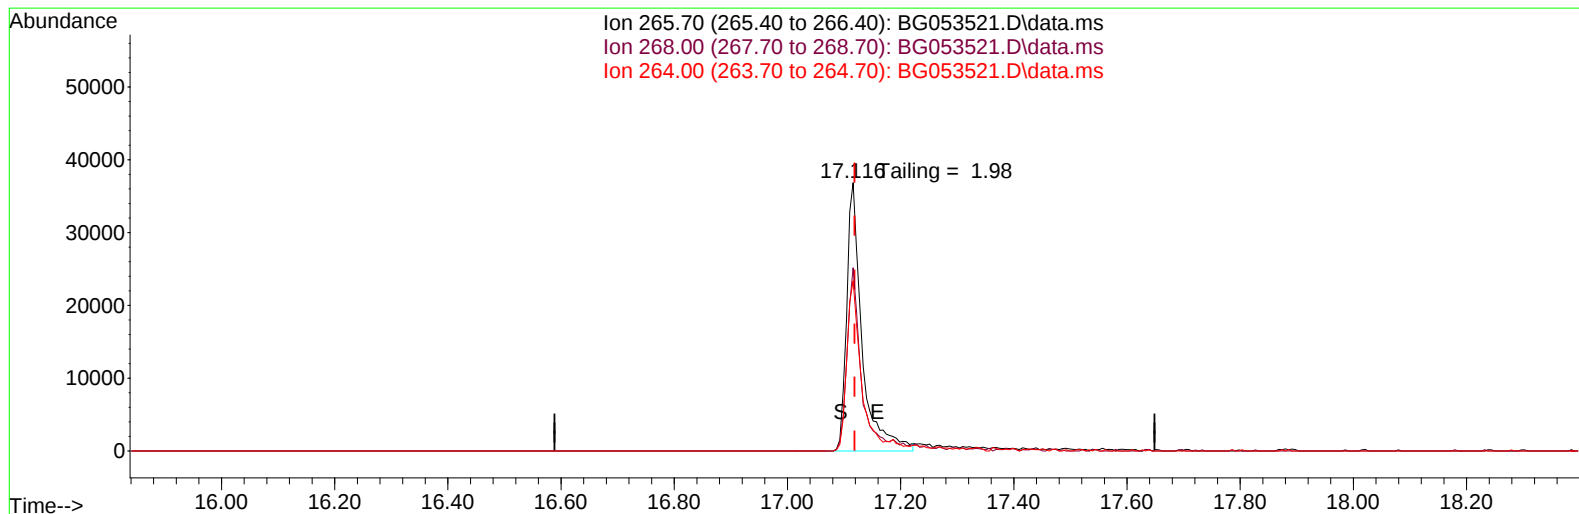

TIC: BG053521.D\data.ms

(70) Pentachlorophenol (C)


17.116min (-0.002) 157909.45 ng

response 71597

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	68.30
264.00	66.20	63.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051122\
Data File : BG053521.D
Acq On : 11 May 2022 11:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 11 19:05:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

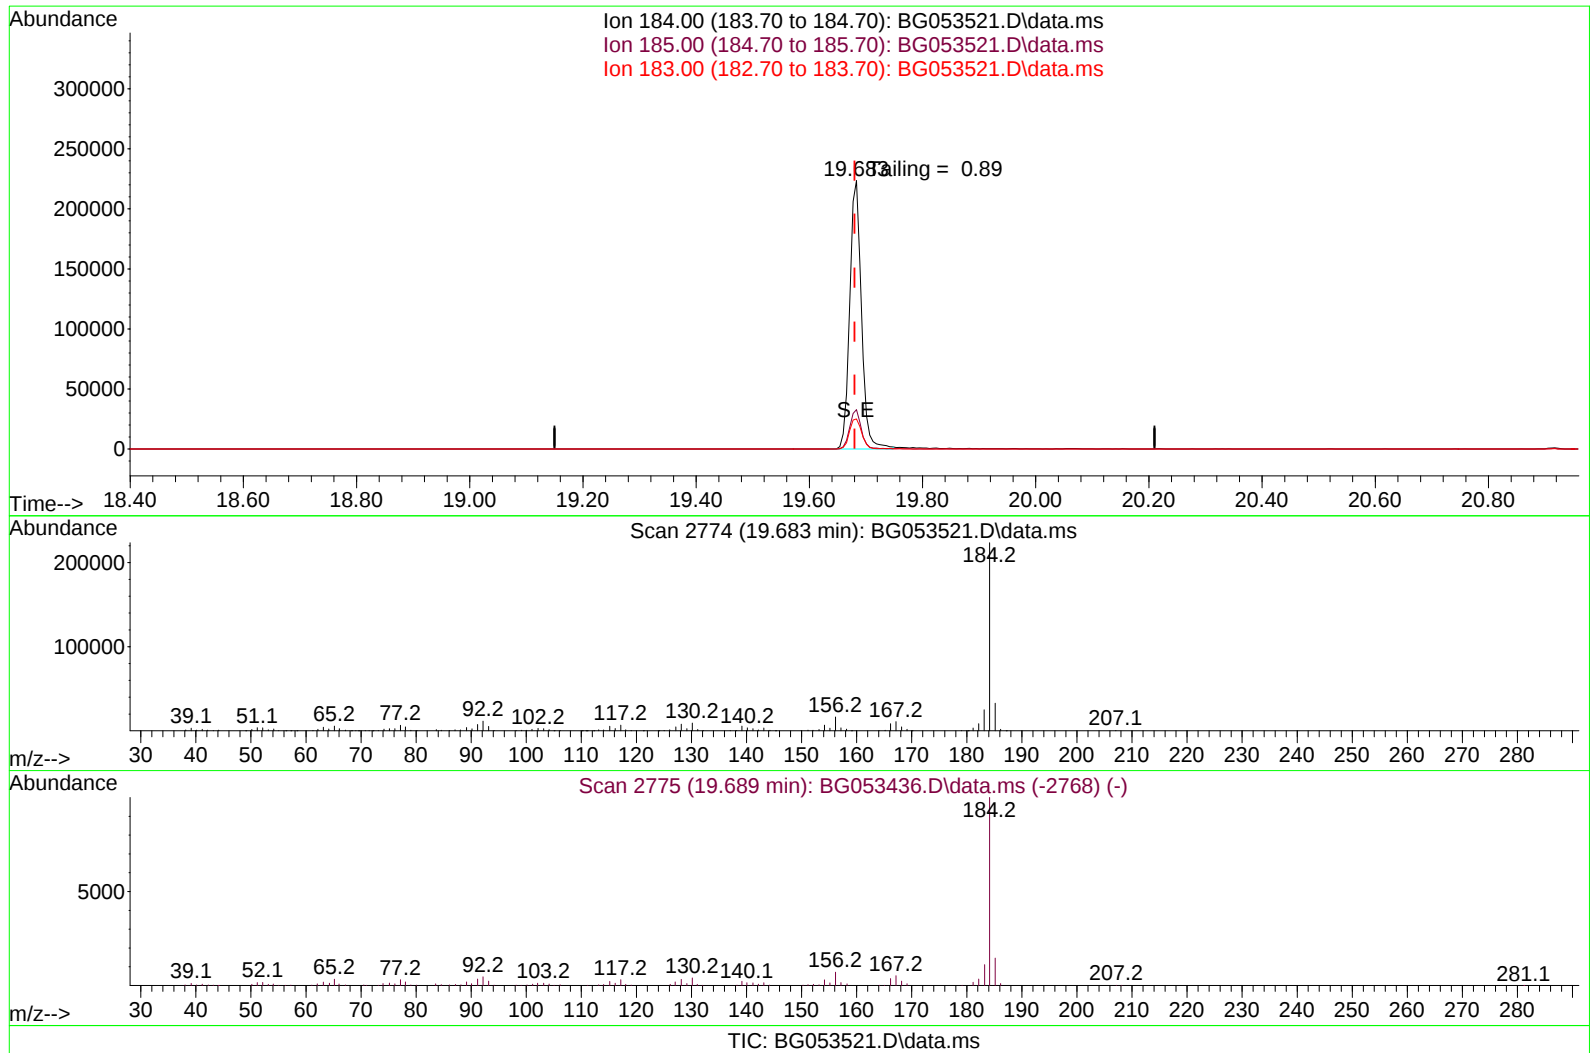**(77) Benzidine**

19.683min (+ 0.004) 5792.80 ng m

response 318883

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.69
183.00	11.10	11.24
0.00	0.00	0.00