
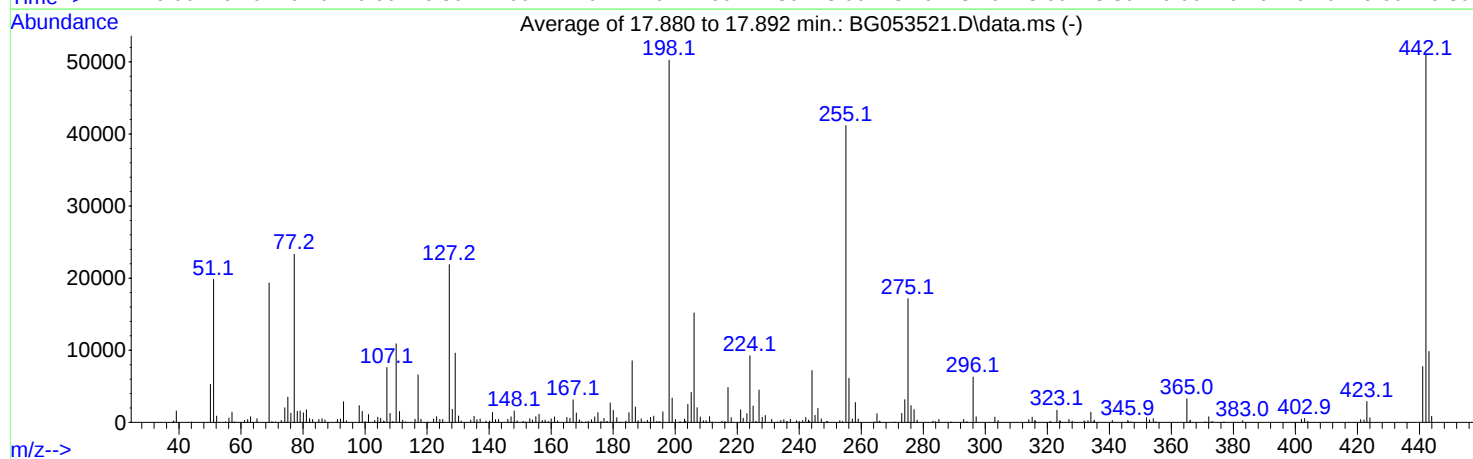


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051122\
 Data File : BG053521.D
 Acq On : 11 May 2022 11:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 11 06:00:46 2022

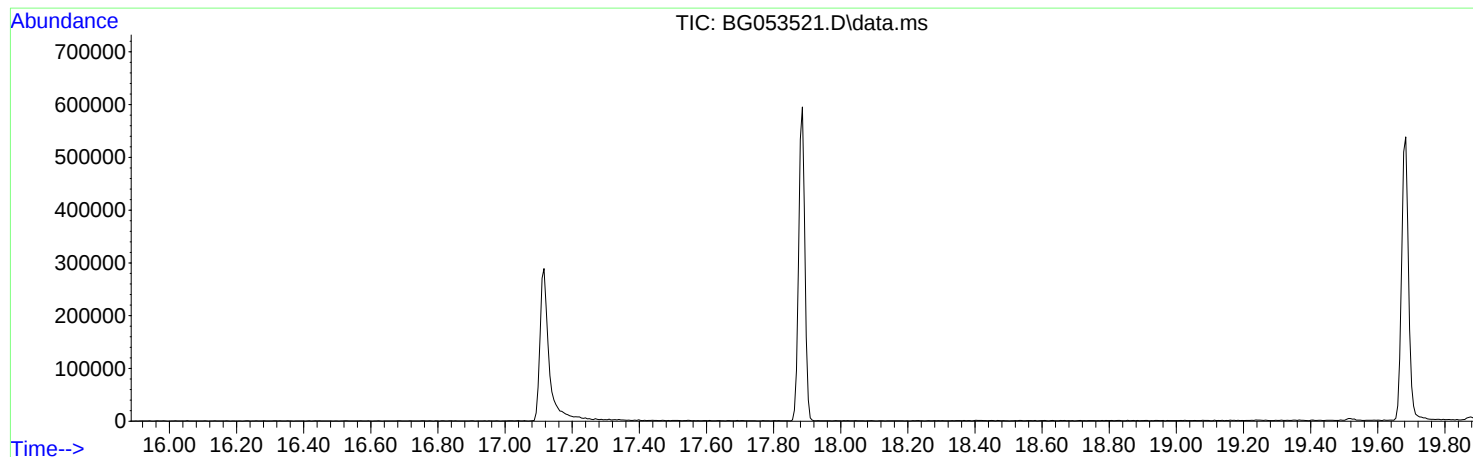




AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.5	19839	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.5	19335	PASS
70	69	0.00	2	0.5	105	PASS
127	198	10	80	43.6	21891	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	50253	PASS
199	198	5	9	6.7	3364	PASS
275	198	10	60	34.1	17152	PASS
365	198	1	100	6.5	3273	PASS
441	198	0.01	100	15.4	7750	PASS
442	442	50	100	100.0	51019	PASS
443	442	15	24	19.3	9832	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051122\
Data File : BG053521.D
Acq On : 11 May 2022 11:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 11 19:05:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

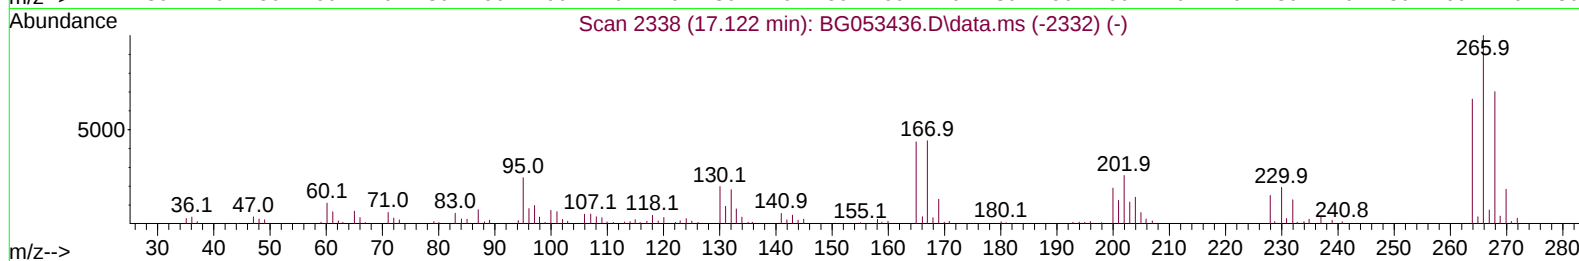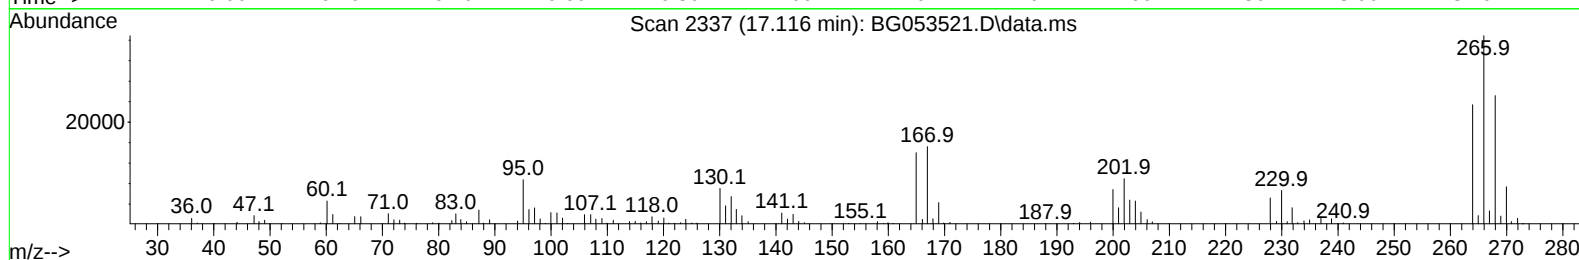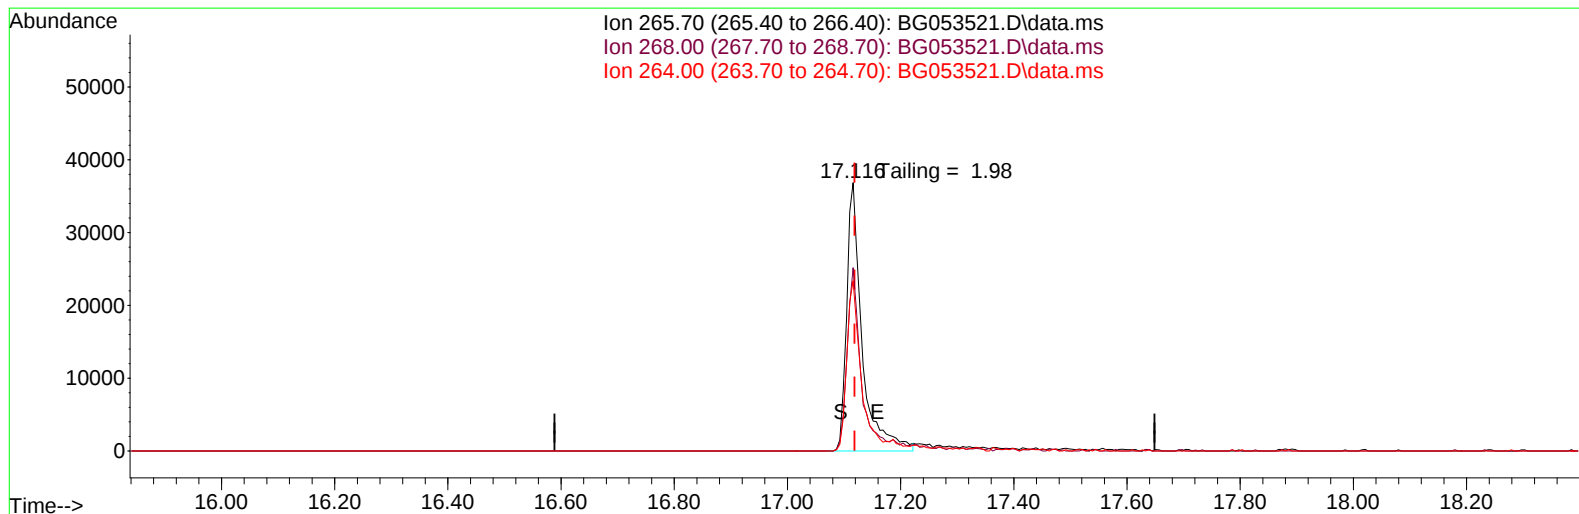

TIC: BG053521.D\data.ms

(70) Pentachlorophenol (C)

17.116min (-0.002) 157909.45 ng




response 71597

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	68.30
264.00	66.20	63.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051122\
Data File : BG053521.D
Acq On : 11 May 2022 11:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 11 19:05:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

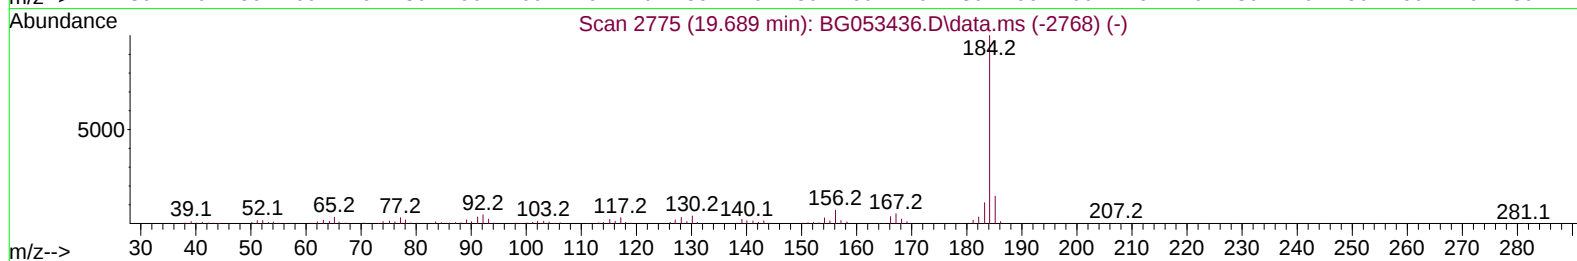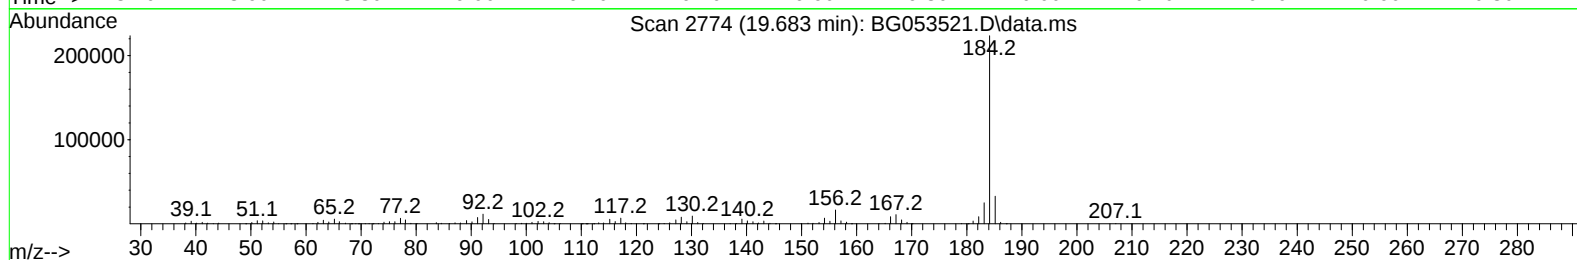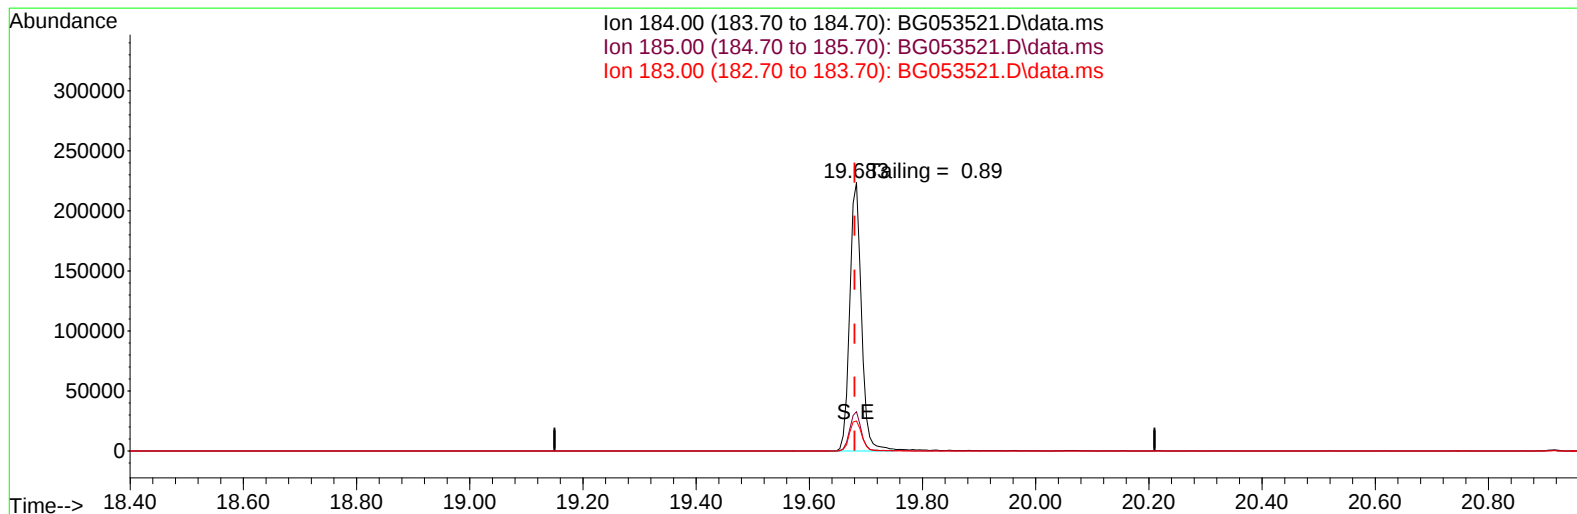

TIC: BG053521.D\data.ms

(77) Benzidine

19.683min (+ 0.004) 5792.80 ng m

response 318883

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.69
183.00	11.10	11.24
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/11/2022	BNA_G	BG053521.D
Compound Name	Response	Retention Time
DDT	186586	20.91
DDD	3203	20.47
DDE	785	19.97
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3988	190574	2.09

Instrument :
BNA_G
ClientSampleId :
DFTPP