
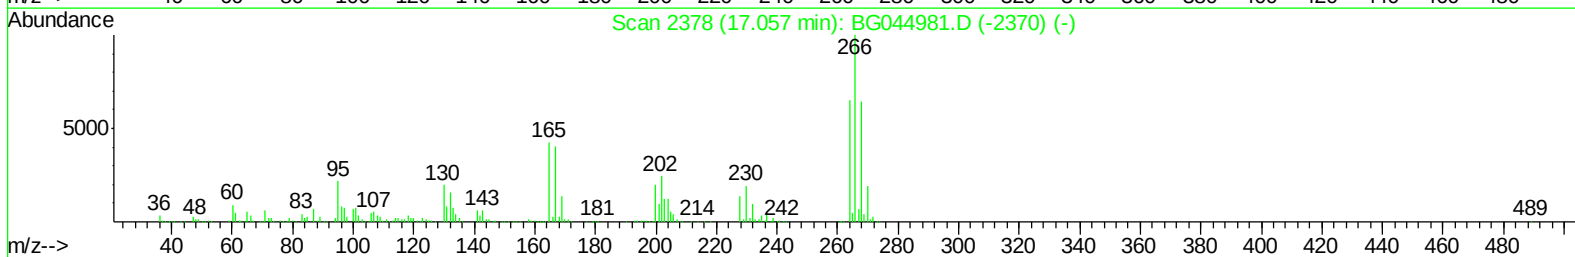
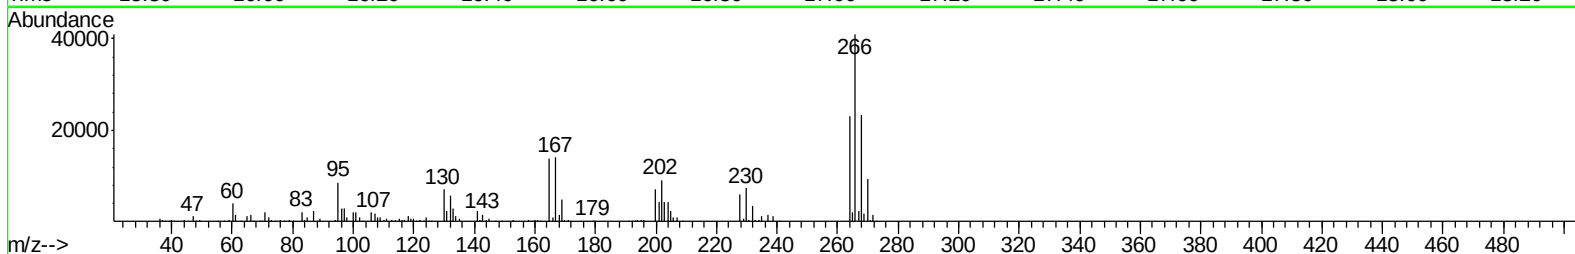


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG051220\
Data File : BG045327.D
Acq On : 12 May 2020 13:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 13 04:05:01 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 12 15:48:20 2020
Response via : Initial Calibration

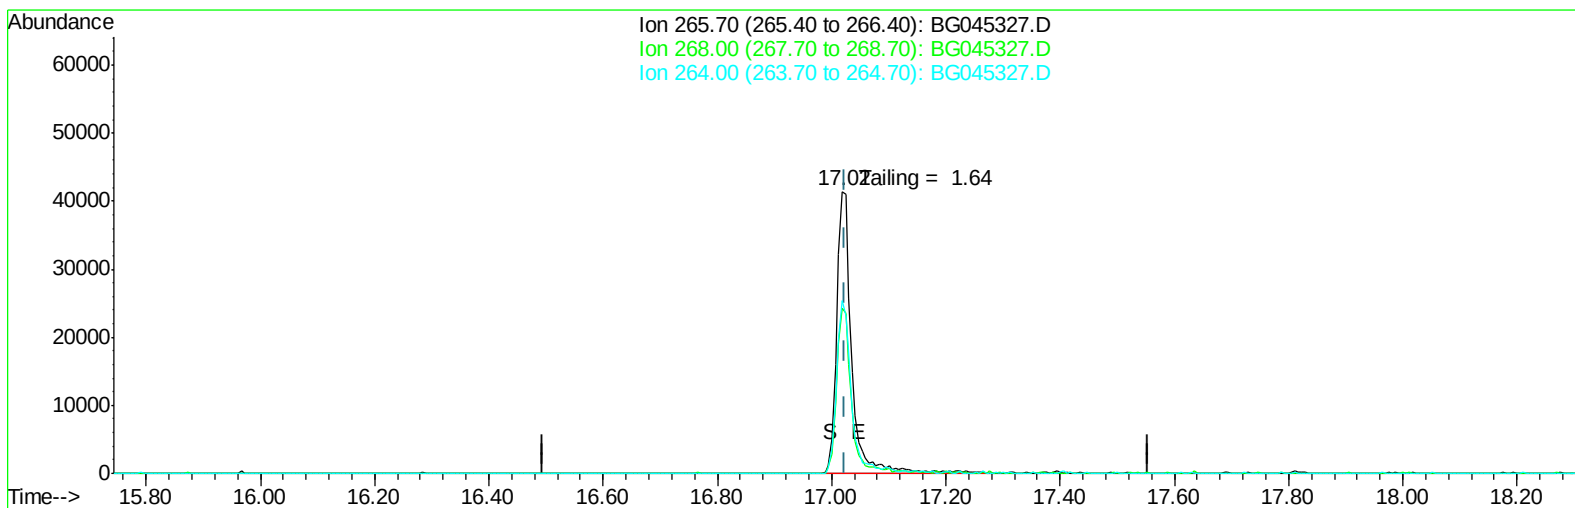

TIC: BG045327.D

(70) Pentachlorophenol (C)




17.018min (-0.007) 52401.83ng

response 73979

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	58.87
264.00	65.30	61.43
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG051220\
Data File : BG045327.D
Acq On : 12 May 2020 13:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 13 04:05:01 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 12 15:48:20 2020
Response via : Initial Calibration

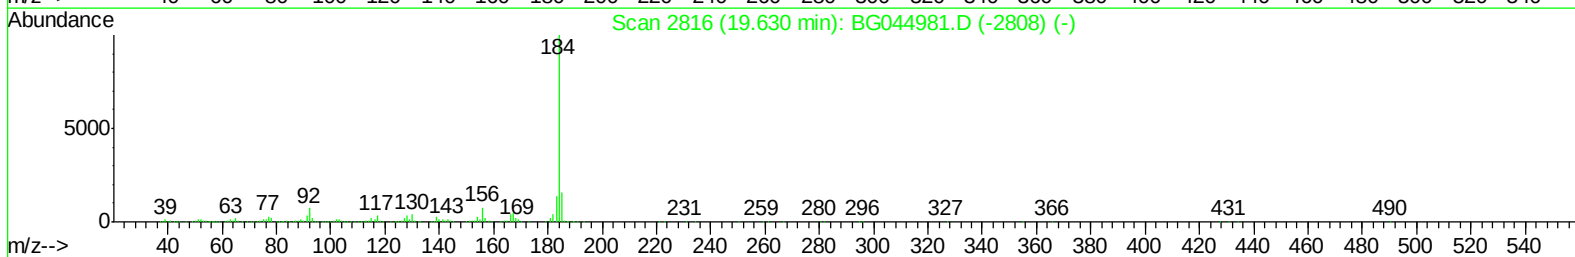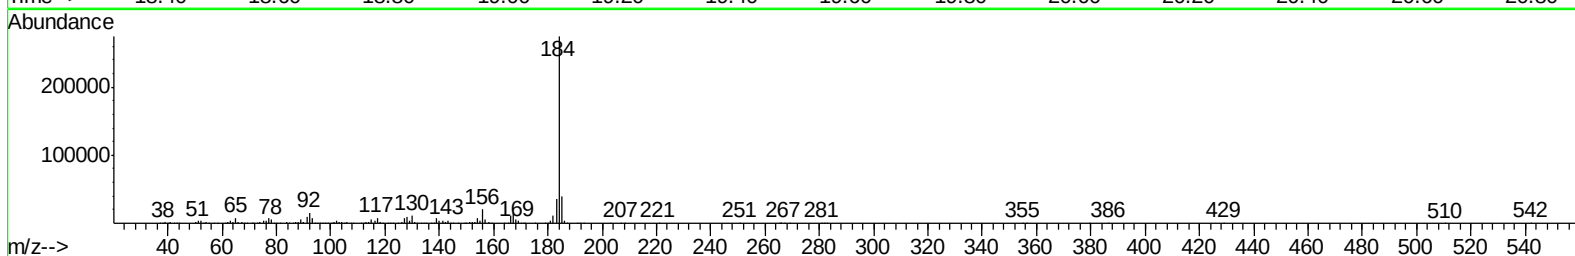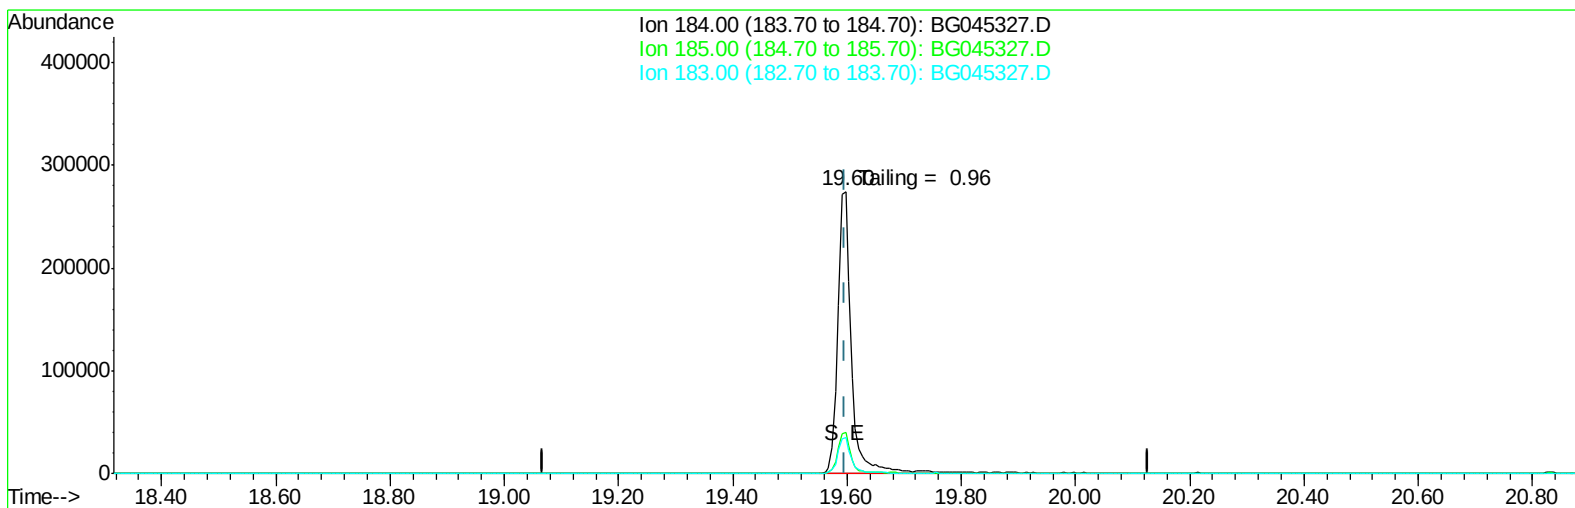

TIC: BG045327.D

(77) Benzidine

19.597min (-0.001) 1987.81ng

response 445085

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	14.69
183.00	14.10	12.90
0.00	0.00	0.00