
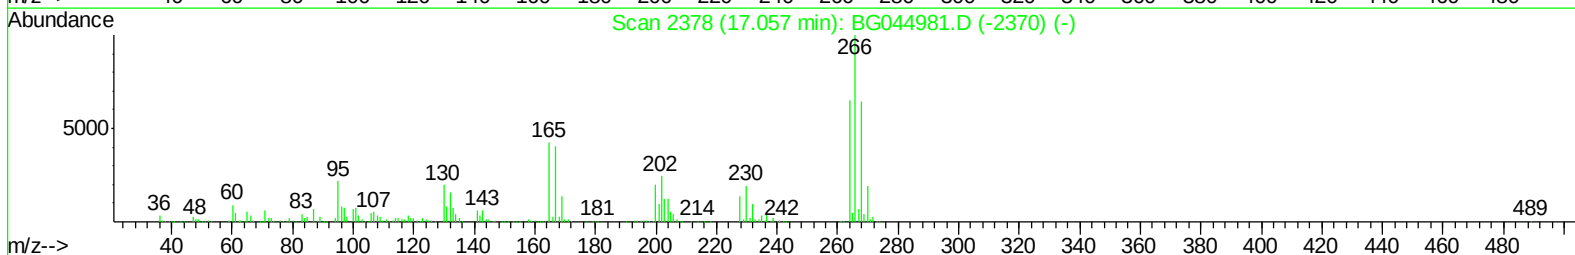
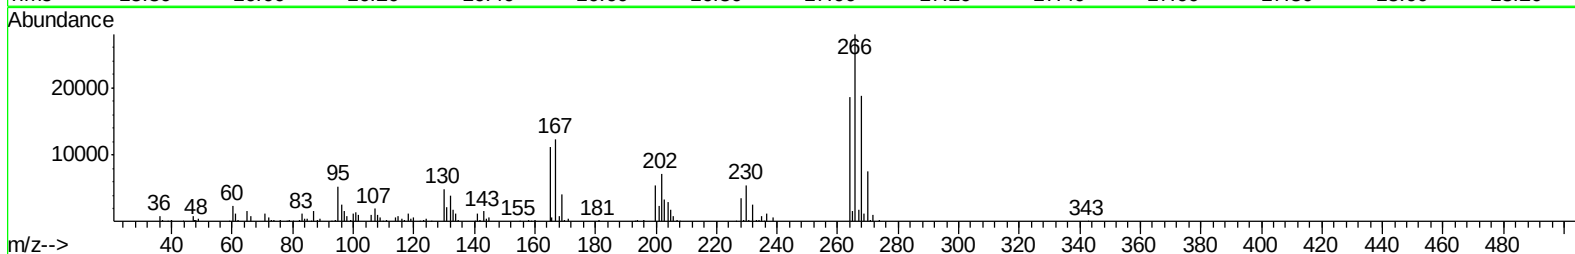


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG051220\  
 Data File : BG045354.D  
 Acq On : 13 May 2020 9:02  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 26 Sample Multiplier: 1

Quant Time: May 13 09:41:14 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue May 12 15:48:20 2020  
 Response via : Initial Calibration

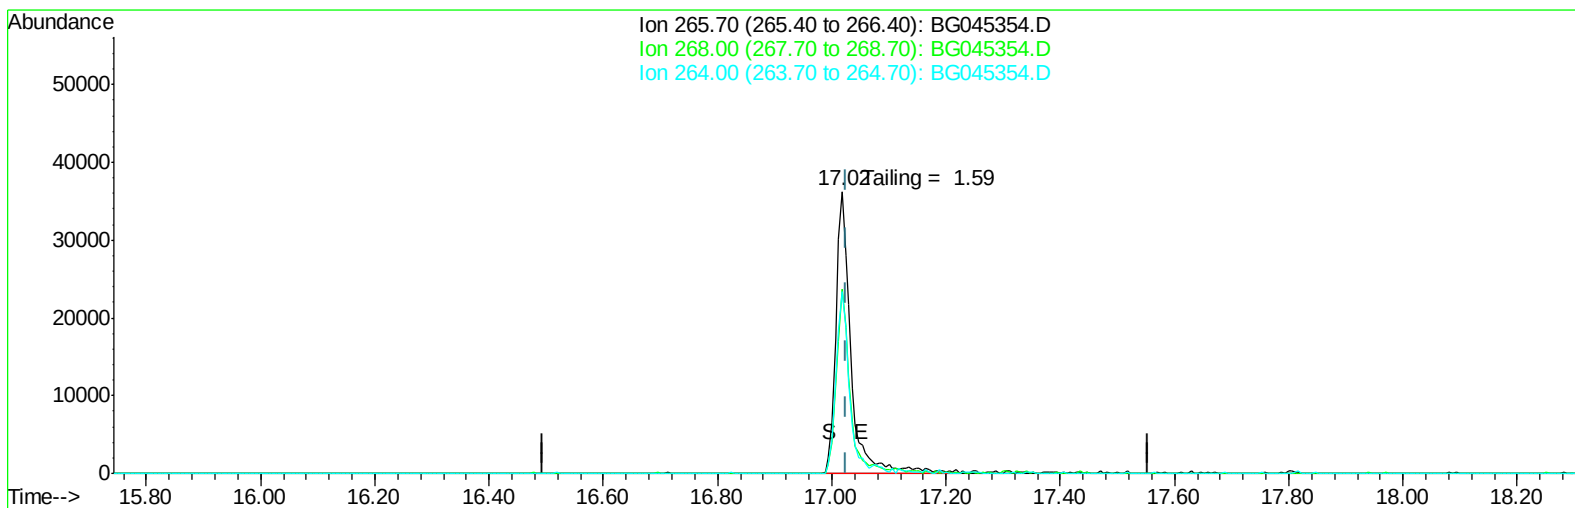

TIC: BG045354.D

(70) Pentachlorophenol (C)




17.018min (-0.007) 109224.52ng

response 63652

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 64.40 | 65.47 |
| 264.00 | 65.30 | 64.61 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG051220\  
 Data File : BG045354.D  
 Acq On : 13 May 2020 9:02  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 26 Sample Multiplier: 1

Quant Time: May 13 09:41:14 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue May 12 15:48:20 2020  
 Response via : Initial Calibration

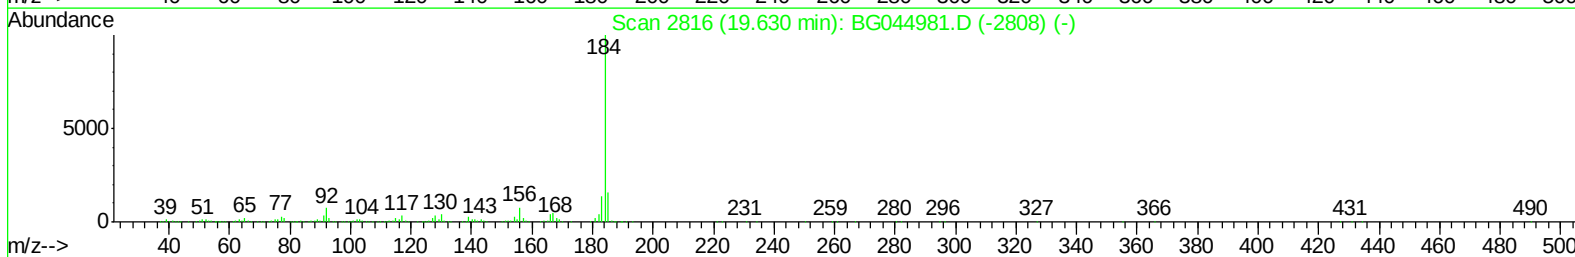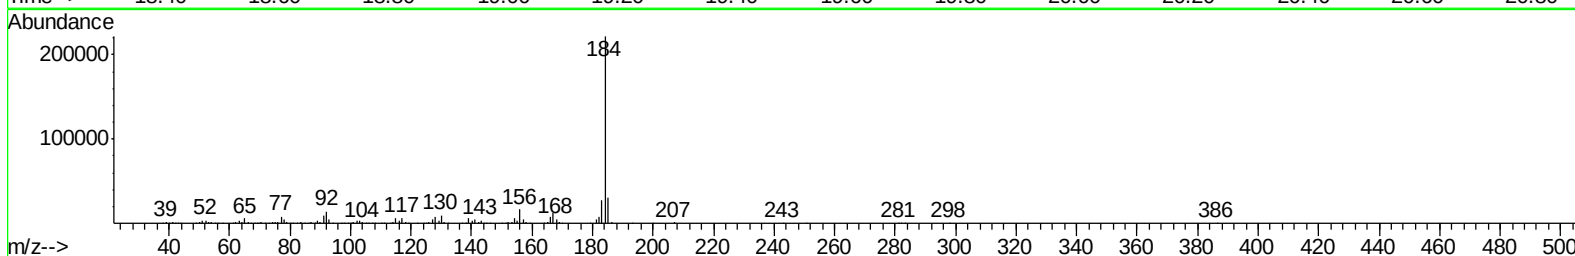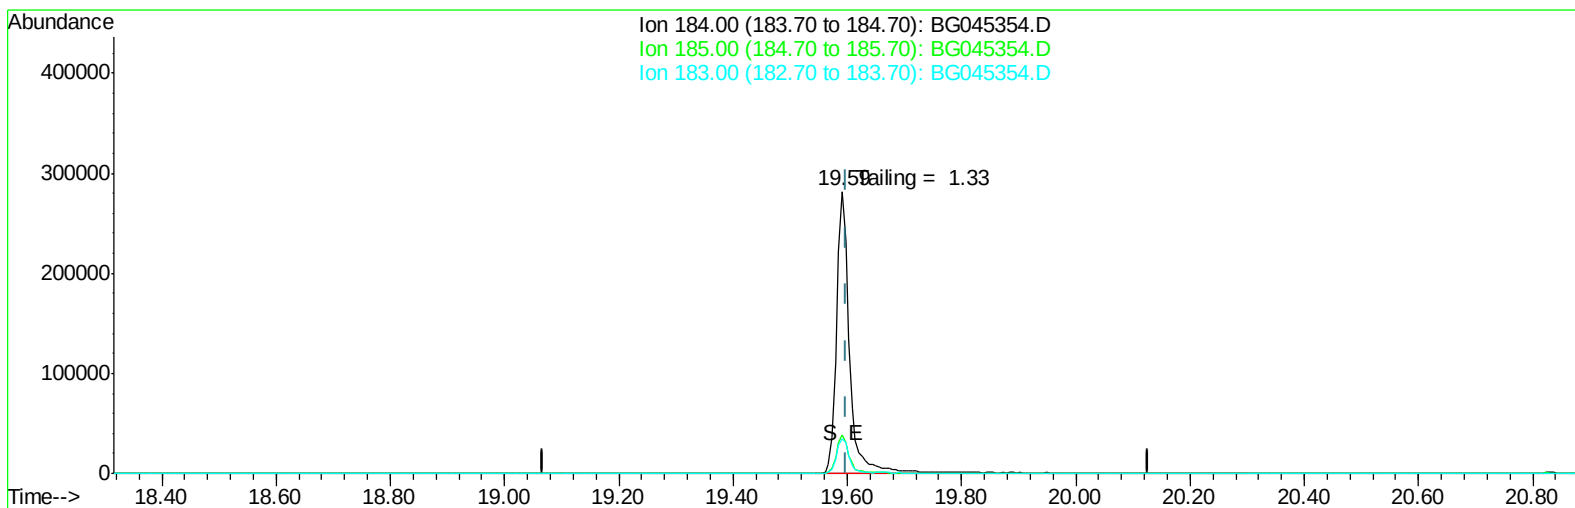

TIC: BG045354.D

(77) Benzidine

19.591min (-0.007) 133745.68ng

response 436971

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.80 | 13.55 |
| 183.00 | 14.10 | 12.43 |
| 0.00   | 0.00  | 0.00  |